

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120823\
 Data File : VU056699.D
 Acq On : 08 Dec 2023 15:02
 Operator : MD/SY
 Sample : 05627-05 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCLC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	107	rBV	143538	164571	17.80%	2.123%
2	1.907	180	192	204	rBV	96478	139774	15.12%	1.803%
3	2.563	385	396	412	rVB	223506	367945	39.80%	4.746%
4	3.042	536	545	554	rBV4	8952	18929	2.05%	0.244%
5	3.174	579	586	599	rVB3	12625	28038	3.03%	0.362%
6	4.621	1026	1036	1060	rBV	111662	302963	32.77%	3.908%
7	5.055	1157	1171	1187	rBV2	178722	405927	43.90%	5.236%
8	5.721	1359	1378	1400	rBV2	357503	924582	100.00%	11.927%
9	6.245	1529	1541	1557	rBV	318804	618504	66.90%	7.978%
10	6.685	1665	1678	1696	rBV2	212457	419161	45.34%	5.407%
11	7.560	1939	1950	1967	rBV2	107507	205023	22.17%	2.645%
12	7.894	2043	2054	2072	rBV	415145	745357	80.62%	9.615%
13	8.177	2130	2142	2155	rBV3	63972	119871	12.96%	1.546%
14	8.631	2271	2283	2308	rBV2	395273	780347	84.40%	10.066%
15	9.415	2514	2527	2553	rBV	443409	824536	89.18%	10.636%
16	9.695	2607	2614	2626	rVB4	14477	22912	2.48%	0.296%
17	10.116	2734	2745	2757	rBV5	14529	33582	3.63%	0.433%
18	10.753	2931	2943	2959	rVB	142695	236817	25.61%	3.055%
19	11.807	3259	3271	3292	rBV	417383	710878	76.89%	9.170%
20	12.190	3376	3390	3408	rBV	357913	651340	70.45%	8.402%
21	13.843	3896	3904	3914	rBV5	18848	31130	3.37%	0.402%




Sum of corrected areas: 7752187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120823\
Data File : VU056699.D
Acq On : 08 Dec 2023 15:02
Operator : MD/SY
Sample : 05627-05 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

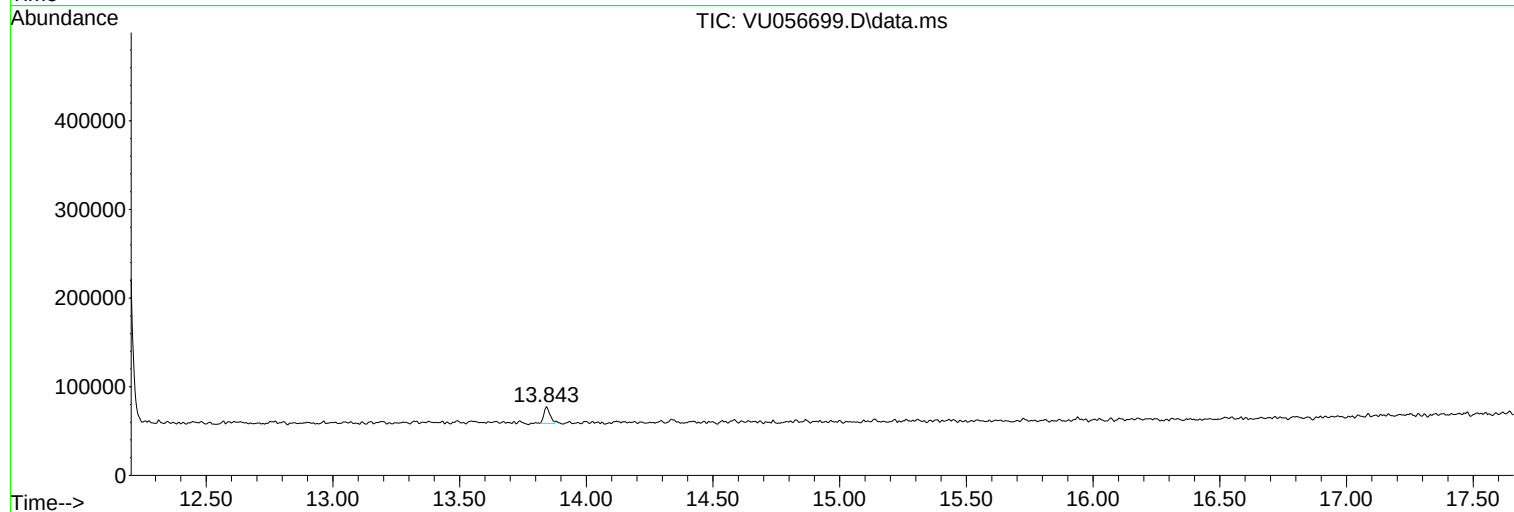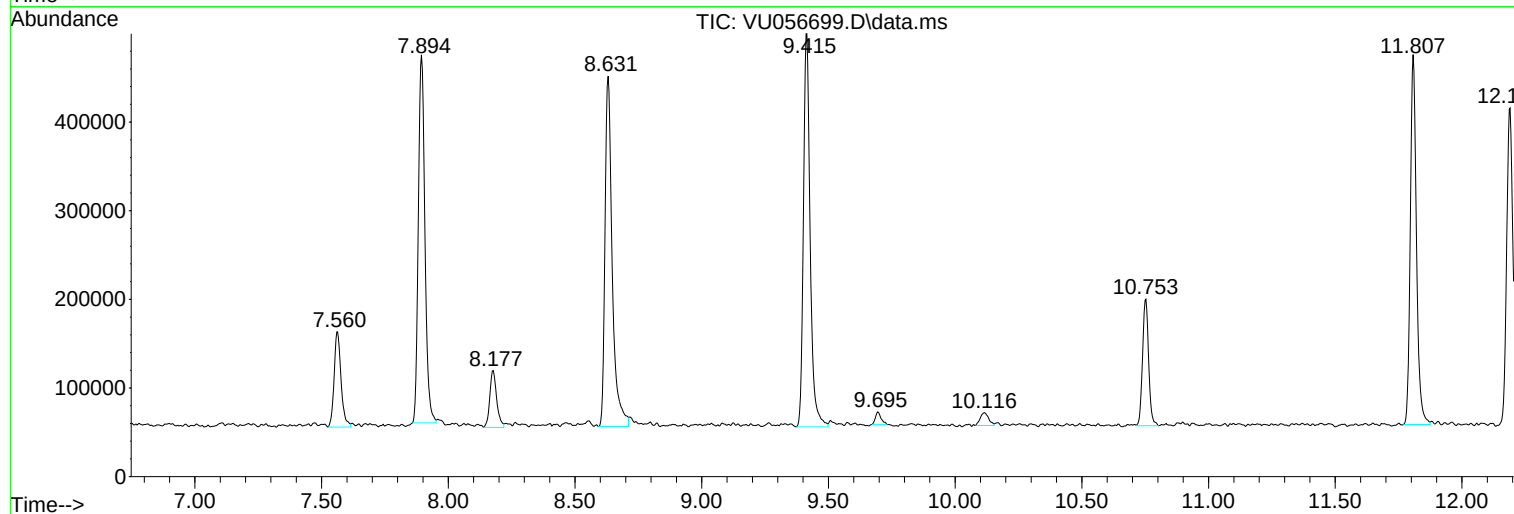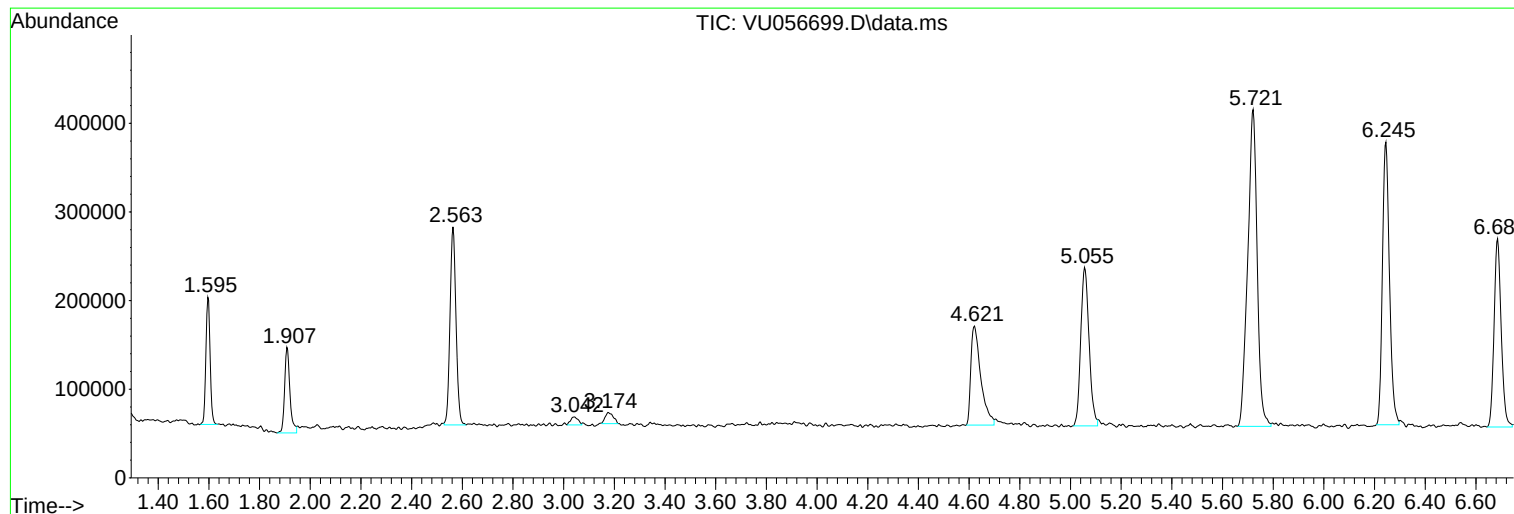

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120823\
Data File : VU056699.D
Acq On : 08 Dec 2023 15:02
Operator : MD/SY
Sample : 05627-05 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120823\
Data File : VU056699.D
Acq On : 08 Dec 2023 15:02
Operator : MD/SY
Sample : 05627-05 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCLC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc