

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U120919\
 Data File : VU036062.D
 Acq On : 09 Dec 2019 21:21
 Operator : JC/MD
 Sample : K6132-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1

Quant Time: Dec 10 03:36:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Dec 10 01:47:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	254911	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	268891	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	117823	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	100202	4.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.20%
7) Chloroethane-d5	1.93	69	120473	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	2.59	63	123458	2.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.40%#
20) 2-Butanone-d5	4.70	46	219628	56.73	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.46%
24) Chloroform-d	5.11	84	173842	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.75	65	91502	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.77	84	344239	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.73	67	102826	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.93	98	286295	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloropropene-	8.21	79	40254	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	8.68	63	184006	59.45	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.90%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	96509	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	117139	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.62	62	103195	4.043	ug/L #	1
8) Chloroethane	1.95	64	93408	4.810	ug/L #	76
13) Acetone	2.69	43	38716	7.878	ug/L	95
15) Methyl Acetate	3.00	43	1677	0.231	ug/L #	62
16) Methylene chloride	3.08	84	15235	0.592	ug/L	99
18) trans-1,2-Dichloroethene	3.39	96	2320	0.123	ug/L #	70
19) 1,1-Dichloroethane	3.92	63	255996	7.535	ug/L	98
21) 2-Butanone	4.78	43	91920	18.686	ug/L	99
22) cis-1,2-Dichloroethene	4.72	96	276031	13.894	ug/L	95
25) Chloroform	5.14	83	43546	1.150	ug/L	96
29) 1,1,1-Trichloroethane	5.36	97	113782	3.754	ug/L	98
33) Benzene	5.82	78	126274	1.718	ug/L	100
34) Trichloroethene	6.58	95	5045	0.259	ug/L	94
38) Bromodichloromethane	7.15	83	6074	0.245	ug/L	87
42) Toluene	8.00	91	44123	0.560	ug/L	99
51) Chlorobenzene	9.48	112	76554	1.394	ug/L	96
52) Ethylbenzene	9.60	91	14704	0.178	ug/L	94

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120919\
Data File : VU036062.D
Acq On : 09 Dec 2019 21:21
Operator : JC/MD
Sample : K6132-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQW1

Quant Time: Dec 10 03:36:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 10 01:47:47 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
53) m,p-Xylene	9.72	106	11380	0.346	ug/L	92
54) o-Xylene	10.13	106	7984	0.259	ug/L	86
55) Styrene	10.14	104	7371	0.139	ug/L	95
62) 1,3-Dichlorobenzene	11.77	146	4549	0.118	ug/L	94
63) 1,4-Dichlorobenzene	11.86	146	16408	0.432	ug/L	93
65) 1,2-Dichlorobenzene	12.24	146	15312	0.402	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU120919\
Data File : VU036062.D
Acq On : 09 Dec 2019 21:21
Operator : JC/MD
Sample : K6132-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQW1

Quant Time: Dec 10 03:36:51 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Dec 10 01:47:47 2019
Response via : Initial Calibration

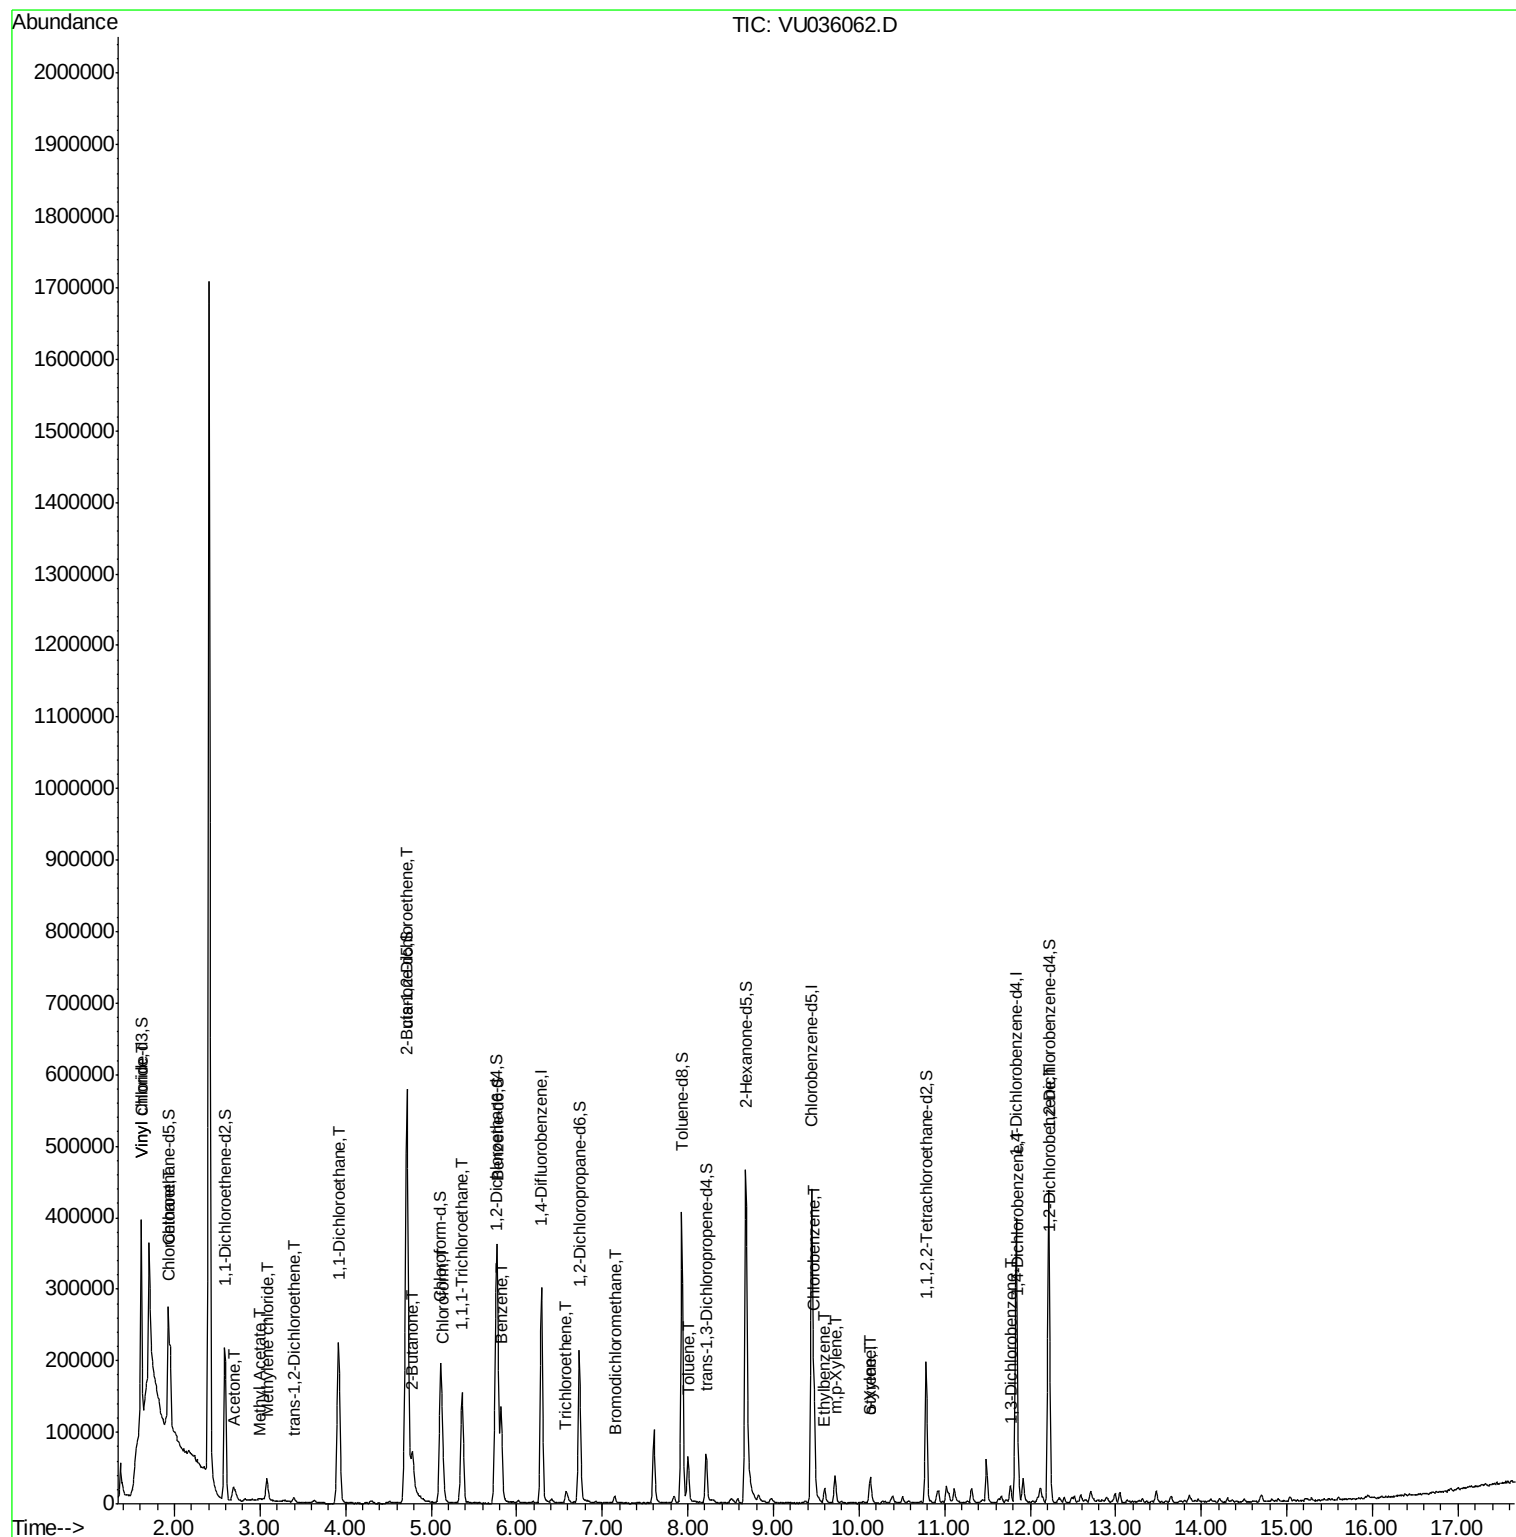



#5

Vinyl chloride

Concen: 4.043 ug/L

RT: 1.62 min Scan# 86

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :





BFQW1

Tot Ion: 62 Resp: 103195

Ion Ratio Lower Upper

62 100

64 100.7 24.3 45.1#

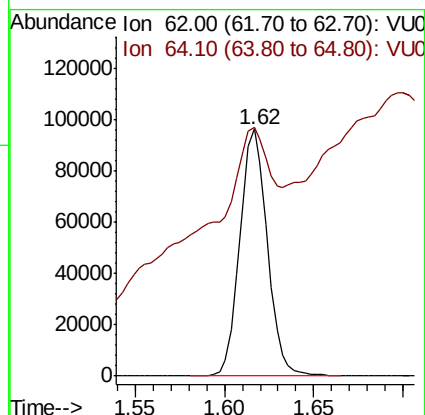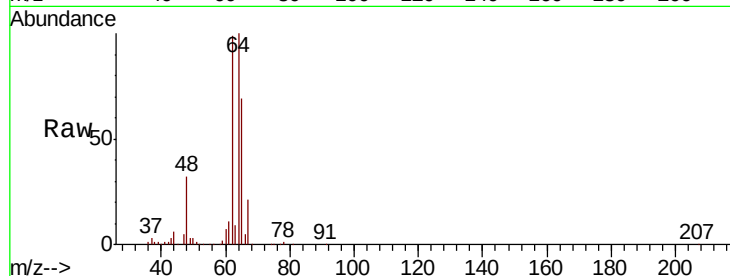

#8

Chloroethane

Concen: 4.810 ug/L

RT: 1.95 min Scan# 190

Delta R.T. -0.00 min

Lab File: VU036062.D




Acq: 09 Dec 2019 21:21


Tgt Ion: 64 Resp: 93408

Ion Ratio Lower Upper

64 100

66 17.5 21.5 39.9#

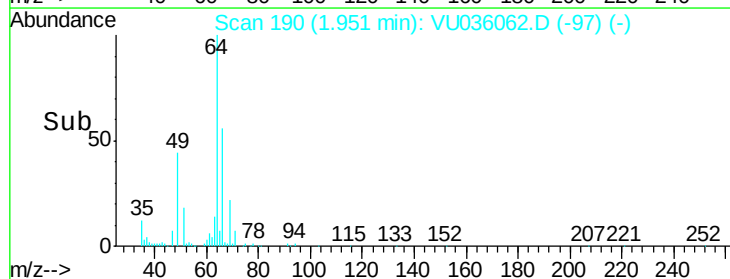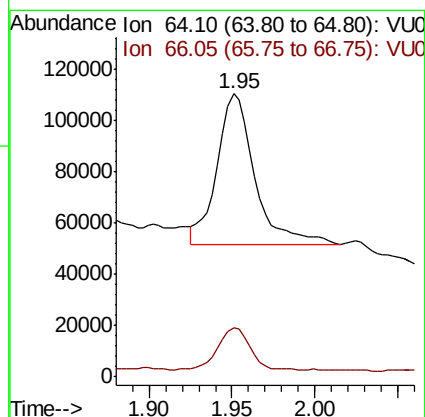

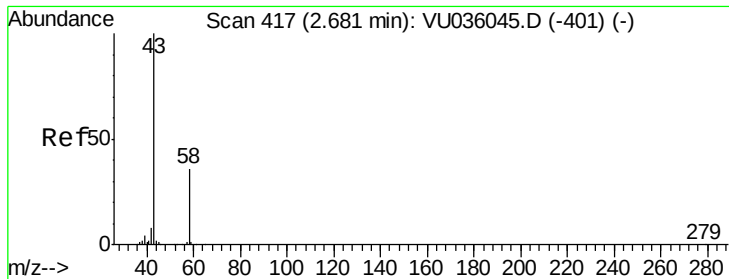

#13

Acetone

Concen: 7.878 ug/L

RT: 2.69 min Scan# 419

Delta R.T. 0.01 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :





BFQW1

Tot Ion: 43 Resp: 38716

Ion Ratio Lower Upper

43 100

58 34.0 0.0 74.2

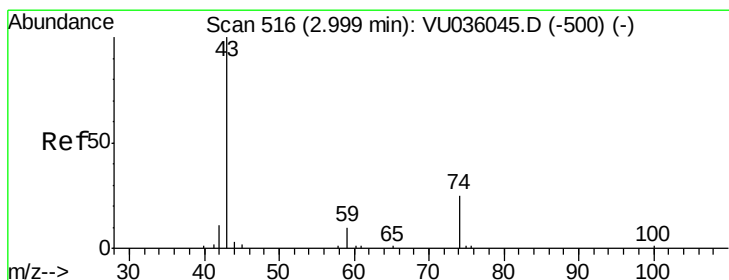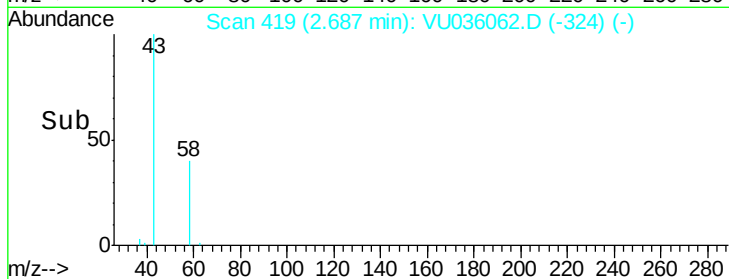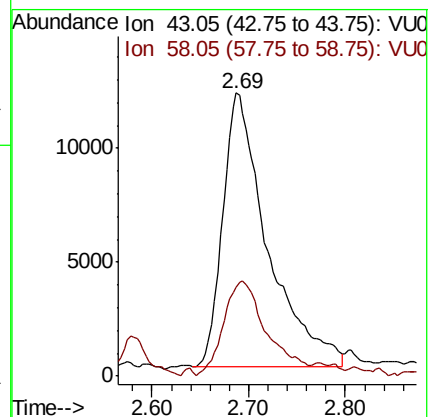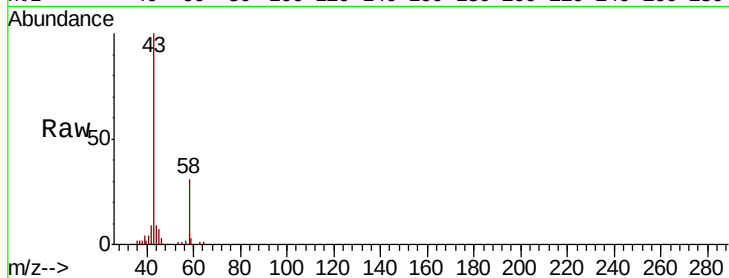

#15

Methyl Acetate

Concen: 0.231 ug/L

RT: 3.00 min Scan# 517

Delta R.T. 0.00 min

Lab File: VU036062.D




Acq: 09 Dec 2019 21:21




Tgt Ion: 43 Resp: 1677

Ion Ratio Lower Upper

43 100

74 45.7 21.0 31.4#

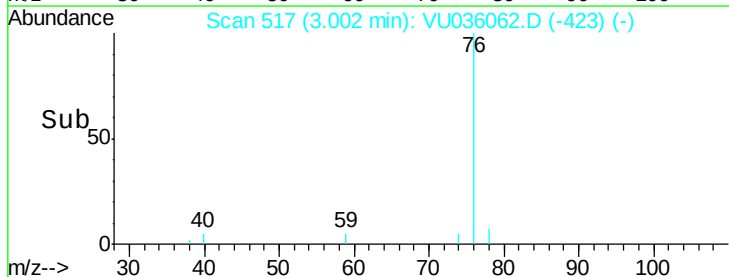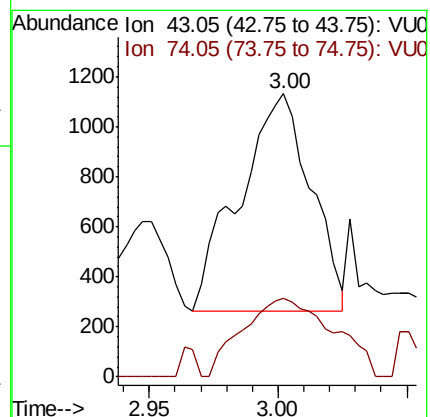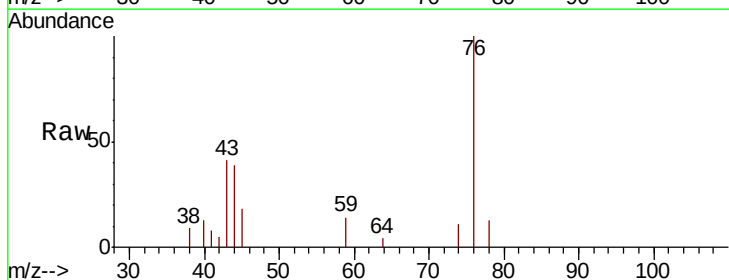

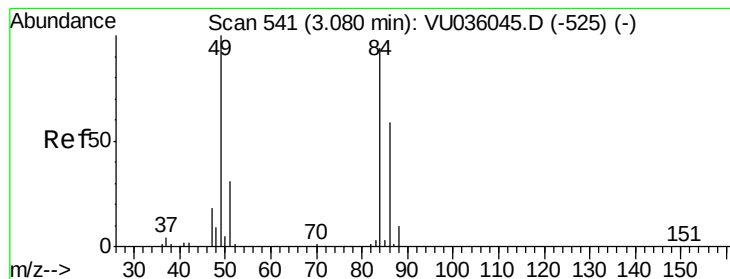

#16

Methylene chloride

Concen: 0.592 ug/L

RT: 3.08 min Scan# 542

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

BFQW1





Tot Ion: 84 Resp: 15235

Ion Ratio Lower Upper

84 100

86 65.7 47.5 88.3

49 110.2 76.9 142.9

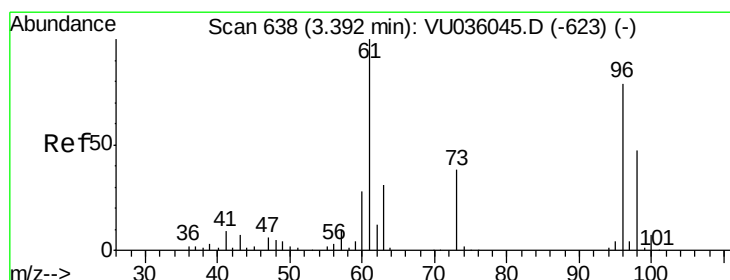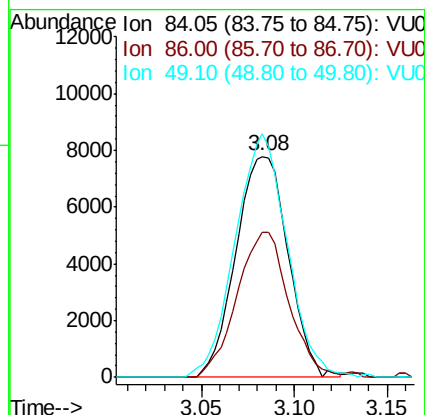

#18

trans-1,2-Dichloroethene

Concen: 0.123 ug/L

RT: 3.39 min Scan# 639

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21


Tgt Ion: 96 Resp: 2320


Ion Ratio Lower Upper

96 100

61 93.6 92.0 170.8

98 44.0 44.6 82.8#

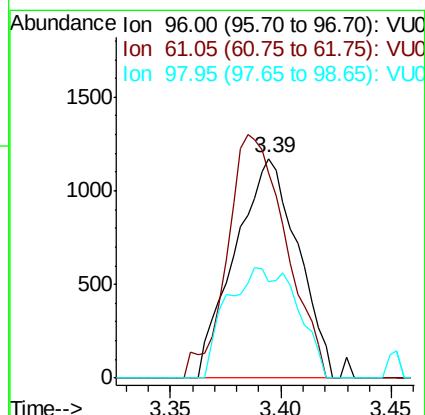

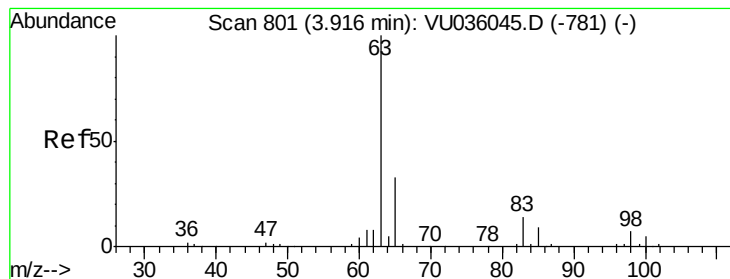

#19

1,1-Dichloroethane

Concen: 7.535 ug/L

RT: 3.92 min Scan# 802

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion: 63 Resp: 255996

Ion Ratio Lower Upper




63 100

65 32.2 21.8 40.4

83 14.3 10.1 18.9



Abundance Ion 63.10 (62.80 to 63.80): VU036062.D (-708) (-)

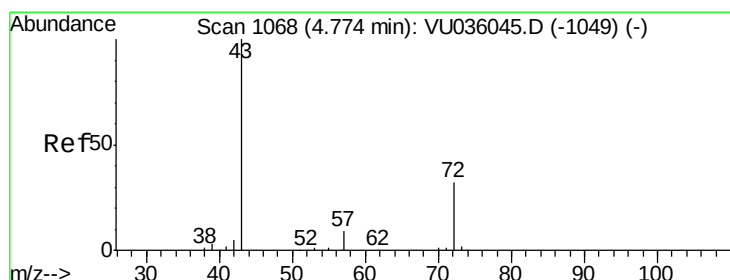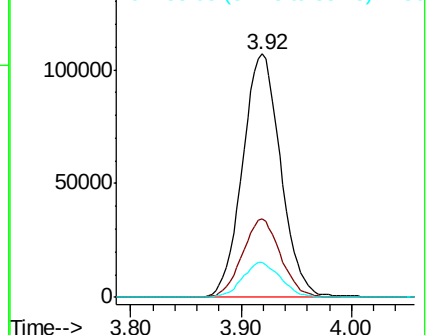

#21

2-Butanone

Concen: 18.686 ug/L

RT: 4.78 min Scan# 1070

Delta R.T. 0.01 min

Lab File: VU036062.D


Acq: 09 Dec 2019 21:21

Tgt Ion: 43 Resp: 91920



Ion Ratio Lower Upper


43 100

72 30.5 15.0 45.0



Abundance Ion 43.05 (42.75 to 43.75): VU036062.D (-975) (-)

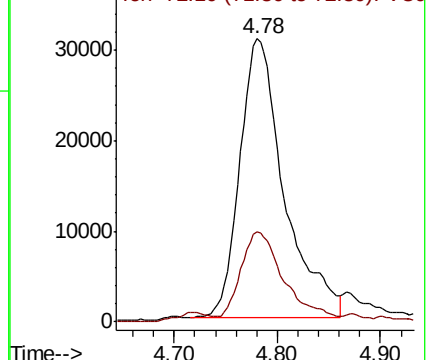

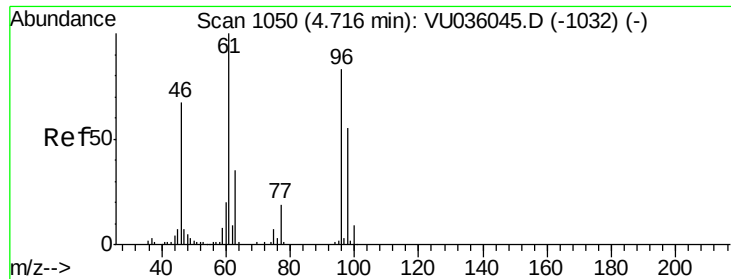

#22

cis-1,2-Dichloroethene

Concen: 13.894 ug/L

RT: 4.72 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion: 96 Resp: 276031

Ion Ratio Lower Upper

96 100

61 112.7 83.0 154.2




68 0.0 0.0 0.0

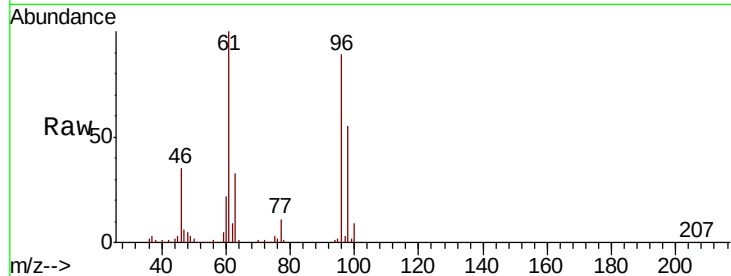

Abundance Ion 96.00 (95.70 to 96.70): VU036062.D (-957) (-)

Ion 61.05 (60.75 to 61.75): VU036062.D (-957) (-)

Ion 68.15 (67.85 to 68.85): VU036062.D (-957) (-)

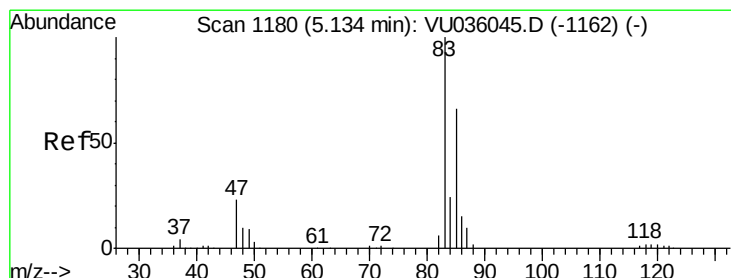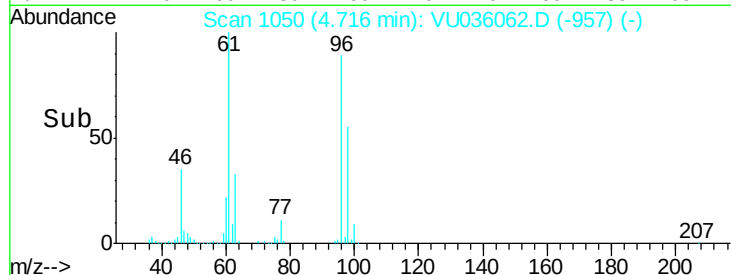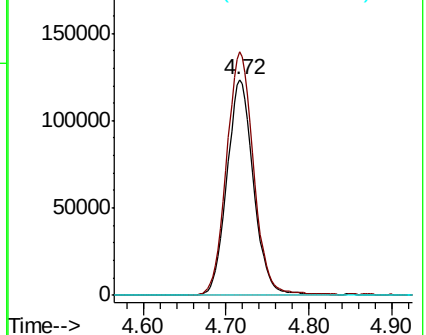

#25

Chloroform

Concen: 1.150 ug/L

RT: 5.14 min Scan# 1181

Delta R.T. 0.00 min

Lab File: VU036062.D


Acq: 09 Dec 2019 21:21

Tgt Ion: 83 Resp: 43546

Ion Ratio Lower Upper



83 100


85 66.1 43.9 81.5

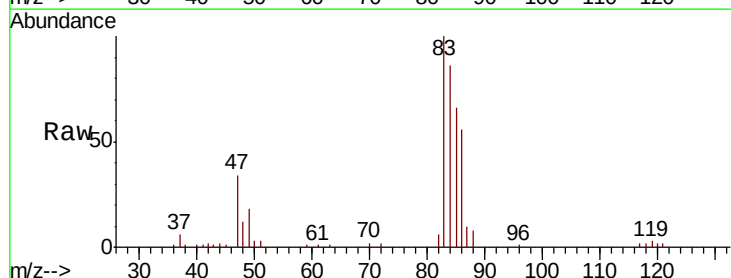

Abundance Ion 83.05 (82.75 to 83.75): VU036062.D (-1087) (-)

Ion 85.00 (84.70 to 85.70): VU036062.D (-1087) (-)



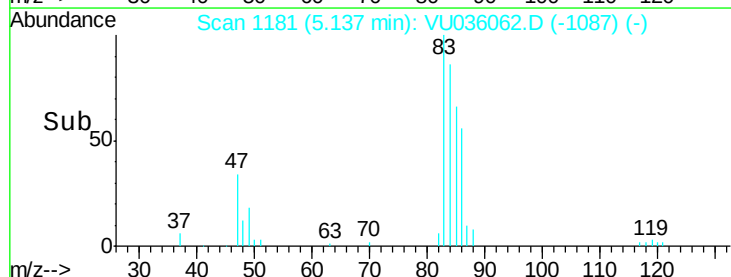
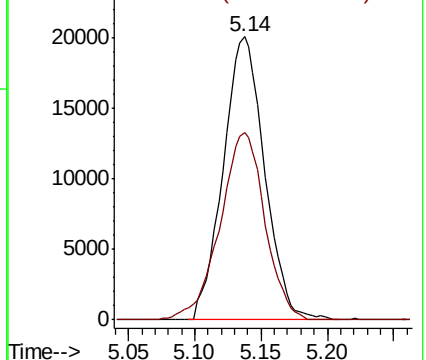







#29
 1,1,1-Trichloroethane
 Concen: 3.754 ug/L
 RT: 5.36 min Scan# 1251
 Delta R.T. 0.00 min
 Lab File: VU036062.D
 Acq: 09 Dec 2019 21:21


Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1

Tot Ion: 97 Resp: 113782
 Ion Ratio Lower Upper
 97 100
 99 63.9 52.2 78.2
 61 41.9 34.7 52.1

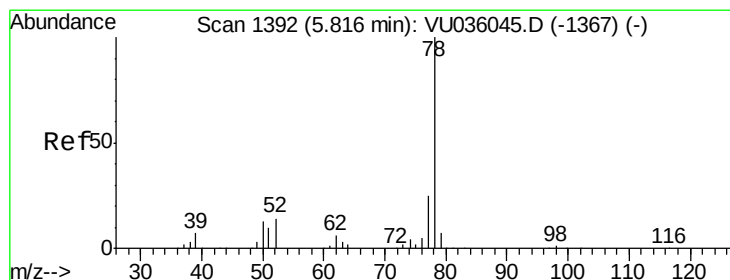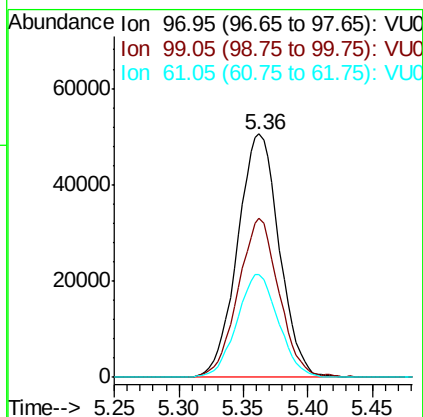

#33
 Benzene
 Concen: 1.718 ug/L
 RT: 5.82 min Scan# 1392
 Delta R.T. -0.00 min
 Lab File: VU036062.D
 Acq: 09 Dec 2019 21:21
 Tgt Ion: 78 Resp: 126274

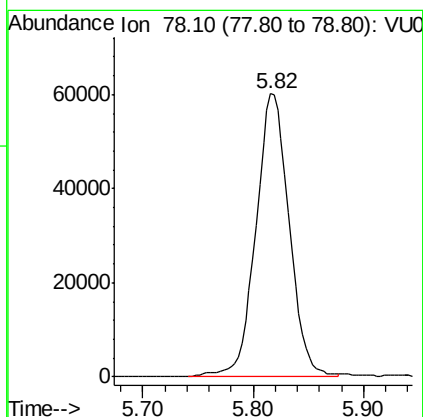

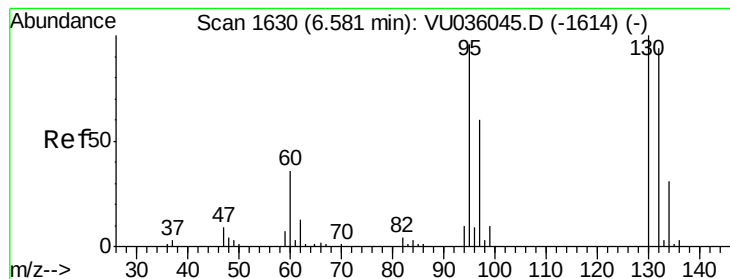

#34

Trichloroethene

Concen: 0.259 ug/L

RT: 6.58 min Scan# 1630

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

BFQW1

Tot Ion: 95 Resp: 5045


Ion Ratio Lower Upper

95 100

97 56.5 44.4 82.4

132 100.6 73.4 136.4

130 102.1 75.9 141.1






Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

Time-->

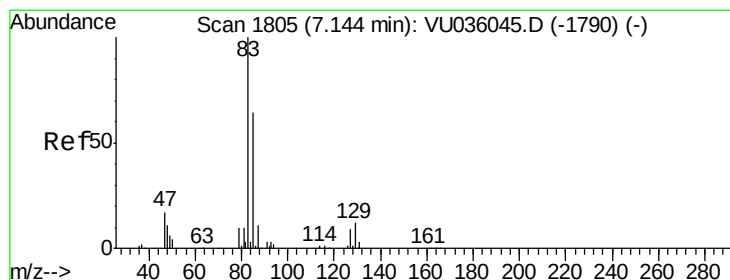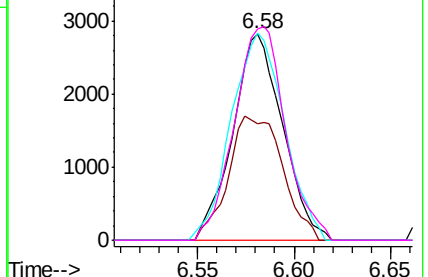

#38

Bromodichloromethane

Concen: 0.245 ug/L

RT: 7.15 min Scan# 1806

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21


Tgt Ion: 83 Resp: 6074

Ion Ratio Lower Upper

83 100

85 75.7 45.2 84.0

127 10.2 7.4 11.2






Abundance Ion 82.95 (82.65 to 83.65): VU0

Ion 85.00 (84.70 to 85.70): VU0

Ion 126.90 (126.60 to 127.60): V

Time-->

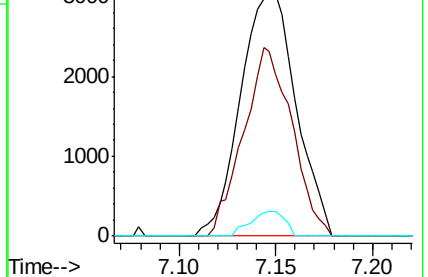



#42

Toluene

Concen: 0.560 ug/L

RT: 8.00 min Scan# 2072

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion: 91 Resp: 44123

Ion Ratio Lower Upper

91 100

92 57.6 40.0 74.4



Abundance Ion 91.15 (90.85 to 91.85): VU036045.D (-2057) (-)

Ion 92.15 (91.85 to 92.85): VU036045.D (-2057) (-)

8.00

25000

20000

15000



10000

5000

0

7.95 8.00 8.05

Time-->



#51

Chlorobenzene

Concen: 1.394 ug/L

RT: 9.48 min Scan# 2531

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21


Tgt Ion: 112 Resp: 76554

Ion Ratio Lower Upper

112 100

114 29.7 22.3 41.5

77 57.7 43.8 65.8



Abundance Ion 112.10 (111.80 to 112.80): VU036045.D (-2516) (-)

Ion 114.05 (113.75 to 114.75): VU036045.D (-2516) (-)

Ion 77.10 (76.80 to 77.80): VU036045.D (-2516) (-)

9.48

60000

50000

40000

30000


20000


10000

0

9.40 9.45 9.50 9.55

Time-->



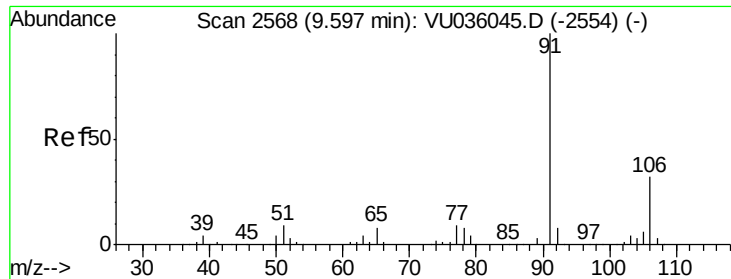

#52

Ethylbenzene

Concen: 0.178 ug/L

RT: 9.60 min Scan# 2569

Delta R.T. 0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion: 91 Resp: 14704

Ion Ratio Lower Upper




91 100

106 34.9 22.0 41.0

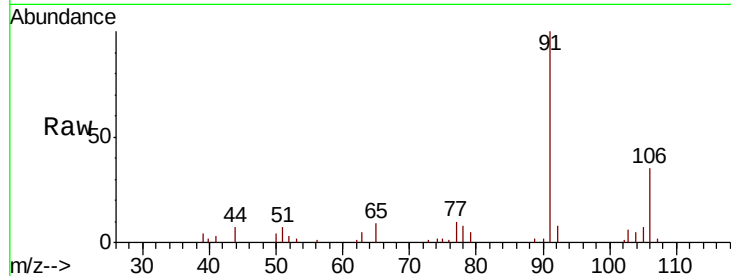

Abundance Ion 91.15 (90.85 to 91.85): VU0

Ion 106.15 (105.85 to 106.85): V

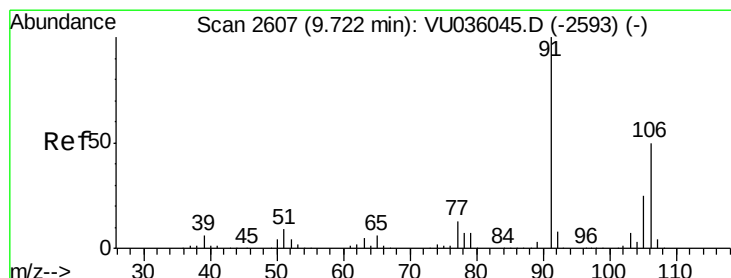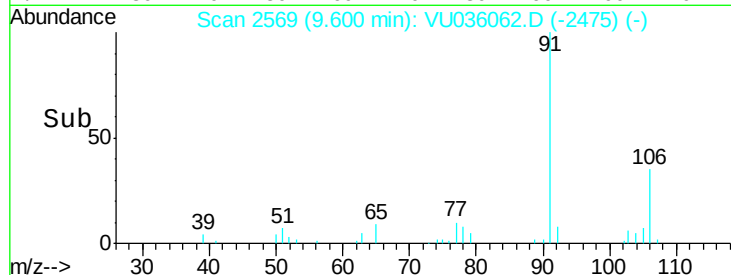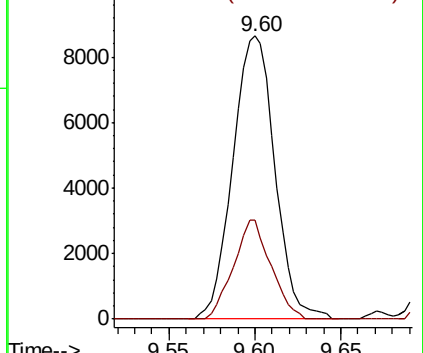

#53

m,p-Xylene

Concen: 0.346 ug/L

RT: 9.72 min Scan# 2606

Delta R.T. -0.00 min

Lab File: VU036062.D


Acq: 09 Dec 2019 21:21

Tgt Ion: 106 Resp: 11380

Ion Ratio Lower Upper



106 100


91 183.3 136.9 254.3

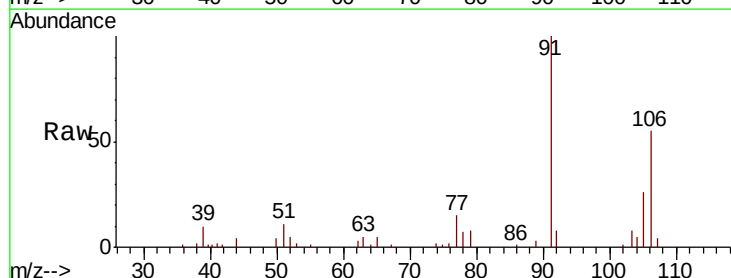

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

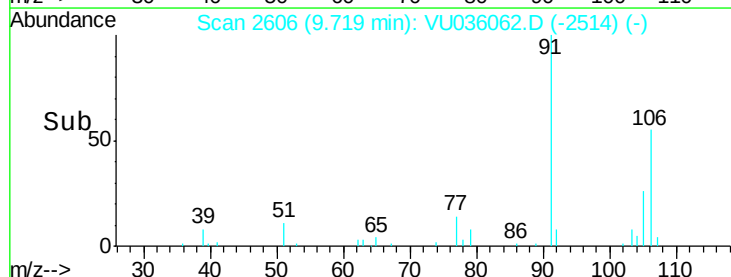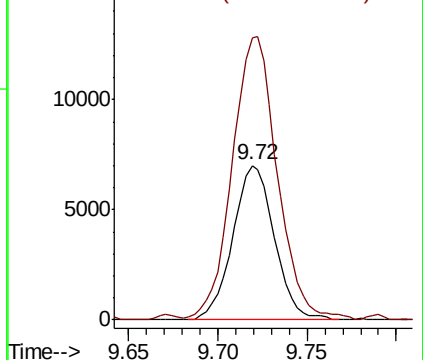

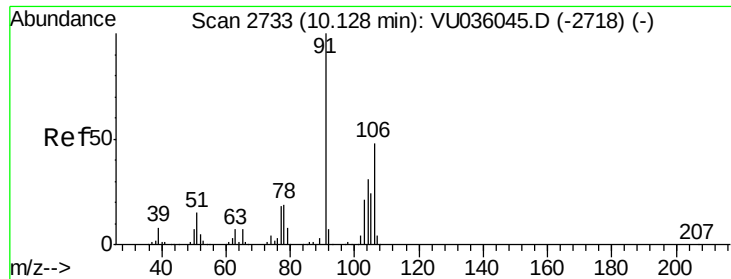

#54

o-Xylene

Concen: 0.259 ug/L

RT: 10.13 min Scan# 2733

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :


BFQW1

Tot Ion:106 Resp: 7984




Ion Ratio Lower Upper

106 100

91 222.7 140.6 261.2

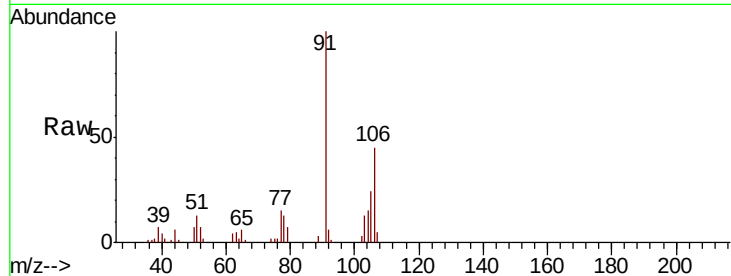

Abundance Ion 106.15 (105.85 to 106.85): V

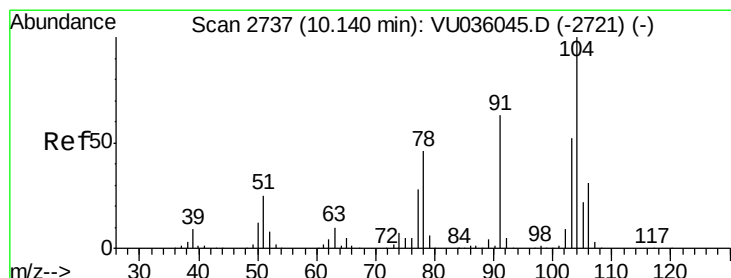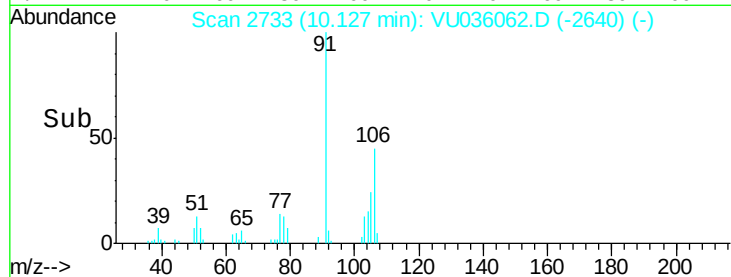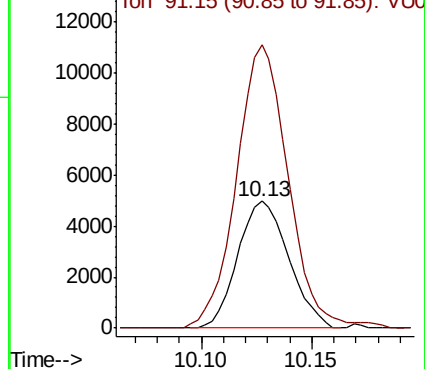

#55

Styrene

Concen: 0.139 ug/L

RT: 10.14 min Scan# 2737

Delta R.T. -0.00 min

Lab File: VU036062.D


Acq: 09 Dec 2019 21:21

Tgt Ion:104 Resp: 7371



Ion Ratio Lower Upper


104 100

78 40.6 30.5 56.7

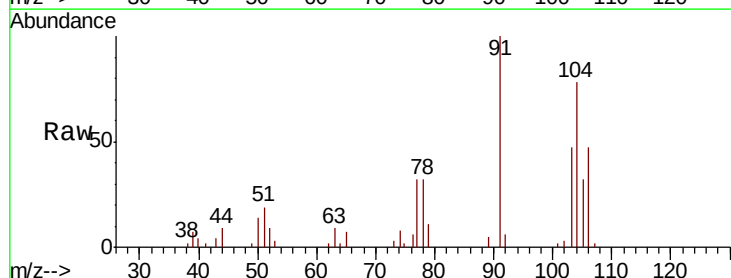

Abundance Ion 104.10 (103.80 to 104.80): V



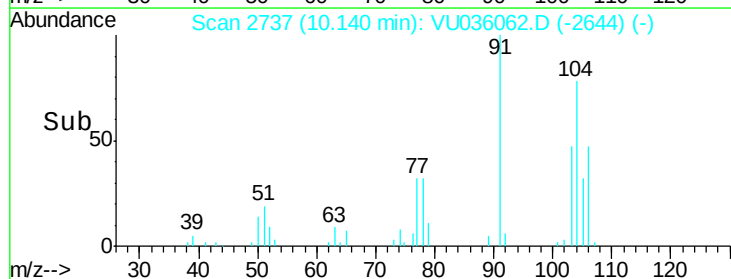
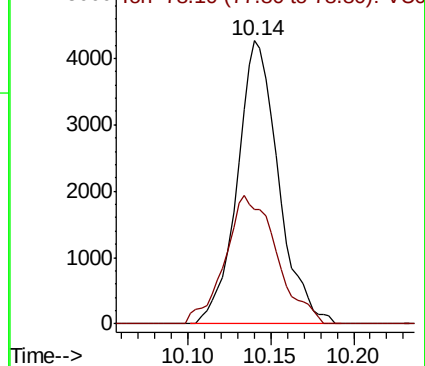


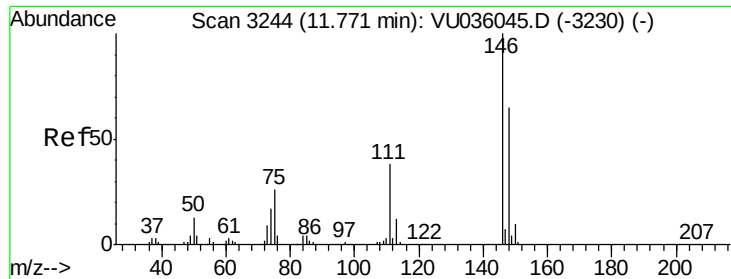

#62
 1,3-Dichlorobenzene
 Concen: 0.118 ug/L
 RT: 11.77 min Scan# 3244
 Delta R.T. -0.00 min
 Lab File: VU036062.D
 Acq: 09 Dec 2019 21:21




Instrument :
 MSVOA_U
 ClientSampleId :
 BFQW1


Tot Ion:146 Resp: 4549
 Ion Ratio Lower Upper
 146 100
 111 38.1 26.0 48.2
 148 55.7 43.7 81.1

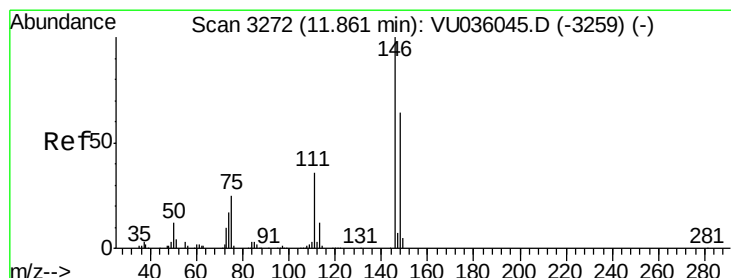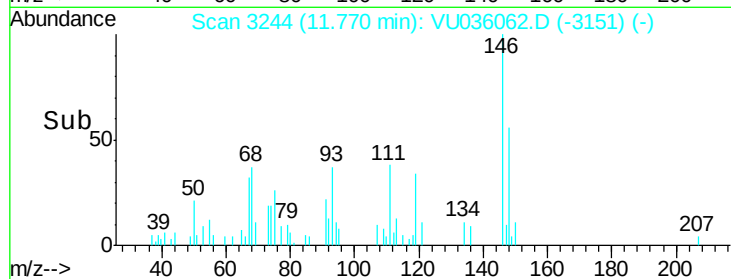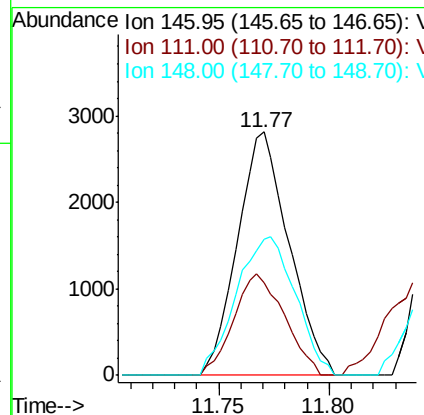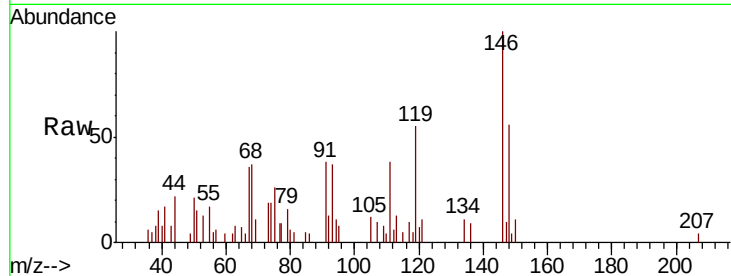

#63
 1,4-Dichlorobenzene
 Concen: 0.432 ug/L
 RT: 11.86 min Scan# 3272
 Delta R.T. -0.00 min
 Lab File: VU036062.D
 Acq: 09 Dec 2019 21:21

Tgt Ion:146 Resp: 16408
 Ion Ratio Lower Upper
 146 100
 111 38.6 26.2 48.6
 148 56.7 44.9 83.5

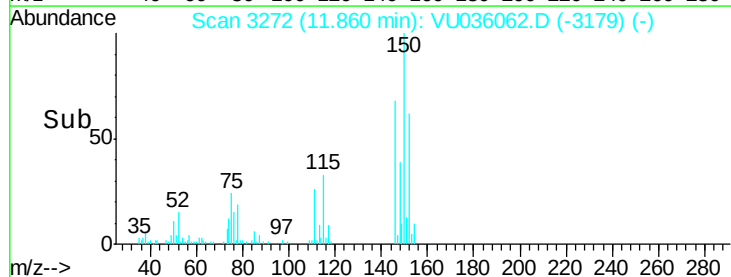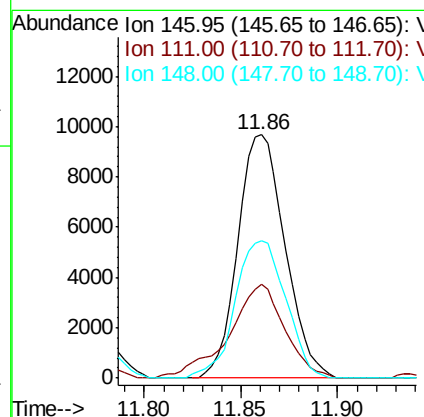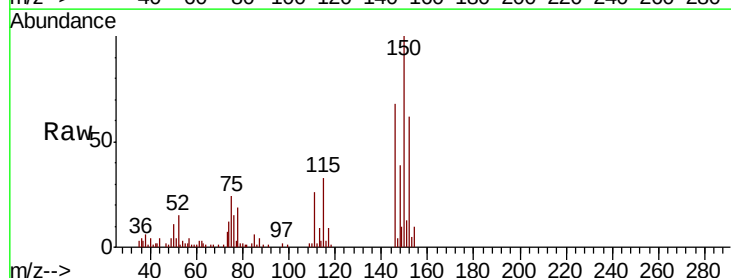

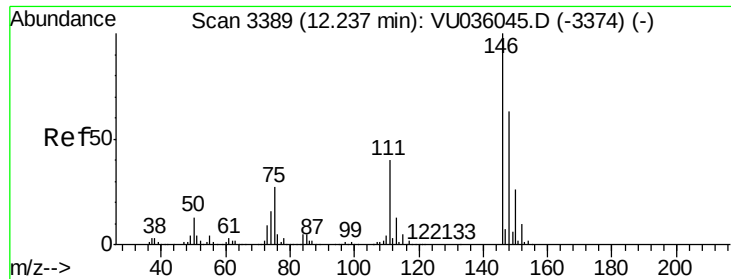

#65

1,2-Dichlorobenzene

Concen: 0.402 ug/L

RT: 12.24 min Scan# 3389

Delta R.T. -0.00 min

Lab File: VU036062.D

Acq: 09 Dec 2019 21:21

Instrument :

MSVOA_U

ClientSampleId :

BFQW1


Tot Ion:146 Resp: 15312

Ion Ratio Lower Upper

146 100

111 45.4 31.3 46.9

148 75.6 50.5 75.7

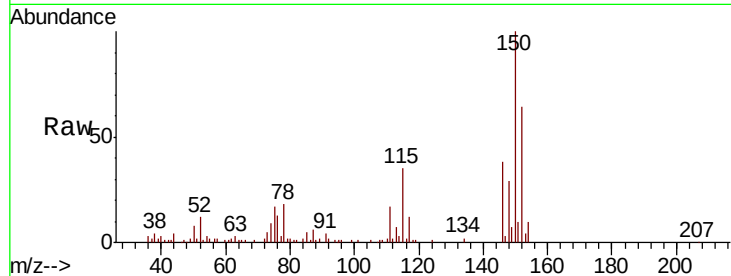

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

