


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120919\
Data File : VU036037.D
Acq On : 09 Dec 2019 09:09
Operator : JC/MD
Sample : BFB14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Dec 11 07:30:58 2019

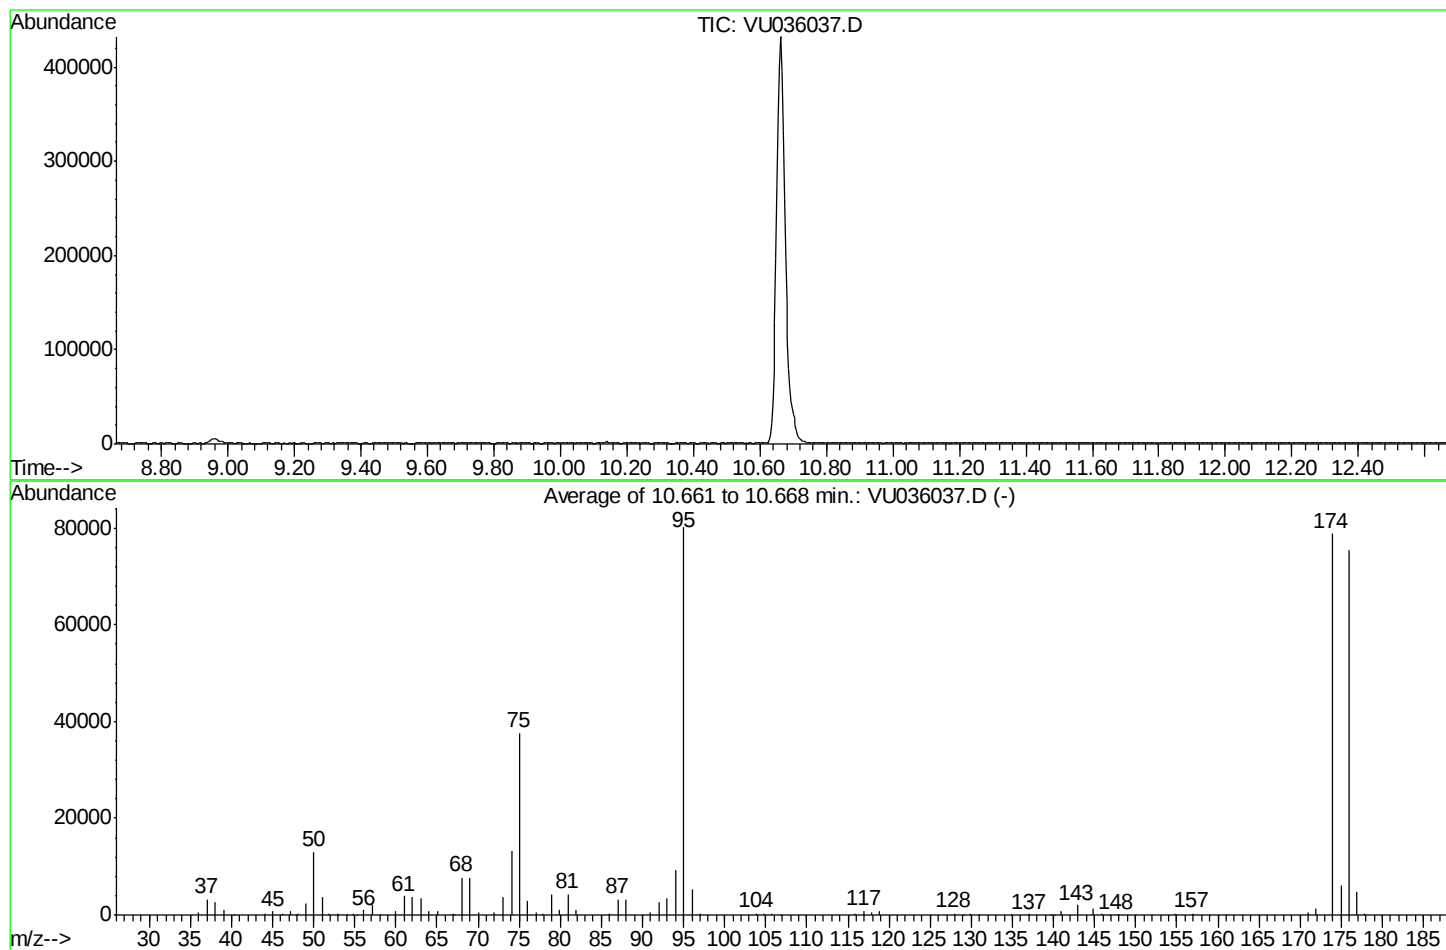

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	13001	PASS
75	95	30	80	46.9	37642	PASS
95	95	100	100	100.0	80176	PASS
96	95	5	9	6.6	5323	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.3	78810	PASS
175	174	5	9	7.7	6075	PASS
176	174	95	101	95.9	75546	PASS
177	176	5	9	6.3	4743	PASS

m/z	Abundance
36.00	704.0
37.00	3484.0
38.10	2792.0
39.00	1289.0
40.20	157.0
44.00	1149.0
45.00	747.0
46.30	212.0
47.10	727.0
48.10	449.0
49.00	2631.0
50.00	13493.0
51.00	3834.0
51.90	190.0
52.90	163.0
54.80	277.0
56.10	1105.0
57.10	2234.0
60.00	924.0
61.00	4026.0
62.00	3944.0
63.10	3914.0
64.00	926.0
65.10	816.0
66.90	290.0
68.00	7929.0
69.00	8170.0
70.10	715.0
71.90	518.0
73.00	3601.0
74.10	13941.0
75.00	39456.0
76.00	3270.0
77.10	484.0
77.90	204.0
78.90	4338.0
80.00	1234.0
80.90	4515.0
81.90	1016.0
86.00	230.0
87.00	3386.0
87.90	2886.0
90.90	491.0
92.10	2666.0
93.00	3701.0
94.10	9464.0
95.10	82376.0
96.00	5880.0
97.00	159.0
103.90	367.0
104.80	163.0
105.80	306.0
106.80	128.0
115.90	345.0
117.00	909.0
117.90	438.0
118.80	718.0
128.00	334.0
129.10	161.0
129.80	351.0
134.80	128.0
137.00	165.0
139.70	102.0
140.90	826.0
142.90	2177.0
144.80	1288.0
145.90	214.0
147.70	238.0
154.80	261.0
156.90	313.0
161.00	127.0
170.90	607.0
172.00	1374.0
173.90	79584.0
175.00	6166.0
175.90	77968.0
176.90	4904.0
177.80	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	651.0
37.00	3390.0
38.00	2632.0
39.10	1176.0
40.30	199.0
44.00	1047.0
45.00	793.0
46.30	239.0
47.10	717.0
48.10	332.0
49.00	2497.0
50.00	13494.0
51.00	3789.0
51.90	180.0
52.90	210.0
54.10	115.0
54.80	250.0
56.10	1058.0
57.10	2321.0
60.00	811.0
61.00	4039.0
62.00	3967.0
63.10	3508.0
64.00	940.0
65.10	895.0
66.90	222.0
68.00	8178.0
69.00	7869.0
70.10	636.0
72.00	430.0
73.00	3753.0
74.10	13872.0
75.00	38600.0
76.00	3068.0
77.10	546.0
77.90	228.0
78.90	4416.0
80.00	1143.0
80.90	4365.0
82.00	1099.0
86.00	222.0
87.00	3327.0
88.00	3083.0
90.90	473.0
92.00	2804.0
93.00	3634.0
94.10	9580.0
95.10	82520.0
96.00	5543.0
97.00	152.0
103.90	319.0
104.80	186.0
105.80	269.0
106.80	126.0
115.90	400.0
116.90	880.0
117.90	426.0
118.80	758.0
127.90	391.0
129.10	104.0
129.80	345.0
130.90	104.0
134.80	125.0
137.10	164.0
140.10	125.0
140.90	888.0
143.00	2091.0
144.90	1415.0
145.80	188.0
146.90	173.0
147.70	177.0
154.70	270.0
156.90	313.0
159.10	101.0
161.00	136.0
170.90	653.0
171.90	1418.0
173.90	80784.0
175.00	6307.0
175.90	77712.0
176.90	4817.0
177.80	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	541.0
37.00	2990.0
38.00	2485.0
39.10	1013.0
39.80	333.0
44.00	907.0
45.00	660.0
46.00	249.0
47.10	609.0
47.80	242.0
48.00	243.0
49.00	2311.0
50.10	12017.0
51.00	3401.0
51.90	163.0
52.90	166.0
54.90	171.0
55.20	164.0
56.10	977.0
57.10	2143.0
58.10	102.0
60.00	708.0
61.00	3830.0
62.00	3613.0
63.10	2979.0
64.00	927.0
65.10	866.0
67.10	159.0
68.00	7276.0
69.00	6883.0
69.90	494.0
72.00	348.0
73.10	3421.0
74.10	12246.0
75.00	34872.0
76.10	2771.0
77.20	509.0
77.90	228.0
78.90	4152.0
79.90	995.0
80.90	4068.0
82.00	1015.0
86.00	228.0
87.00	2970.0
88.00	3238.0
90.90	340.0
92.00	2481.0
93.00	3347.0
94.10	9025.0
95.00	75632.0
96.00	4548.0
97.00	169.0
103.90	313.0
104.80	156.0
105.80	266.0
115.90	371.0
116.90	750.0
117.90	410.0
118.80	649.0
128.00	394.0
129.80	297.0
134.90	114.0
137.10	126.0
140.10	128.0
140.90	889.0
143.00	2034.0
144.90	1375.0
145.80	137.0
146.90	193.0
148.00	132.0
149.90	112.0
154.80	205.0
155.00	202.0
156.90	248.0
159.00	123.0
161.00	133.0
170.90	563.0
171.90	1351.0
173.90	76064.0
175.00	5752.0
176.00	70960.0
176.90	4508.0
177.80	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Scan 2884 (10.613 min): VU036037.D
BFB14

m/z	Abundance
40.00	163.0
44.00	810.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14