


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU120920\
 Data File : VU041503.D
 Acq On : 09 Dec 2020 09:30
 Operator : SY/MD
 Sample : BFB21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Dec 10 04:45:04 2020

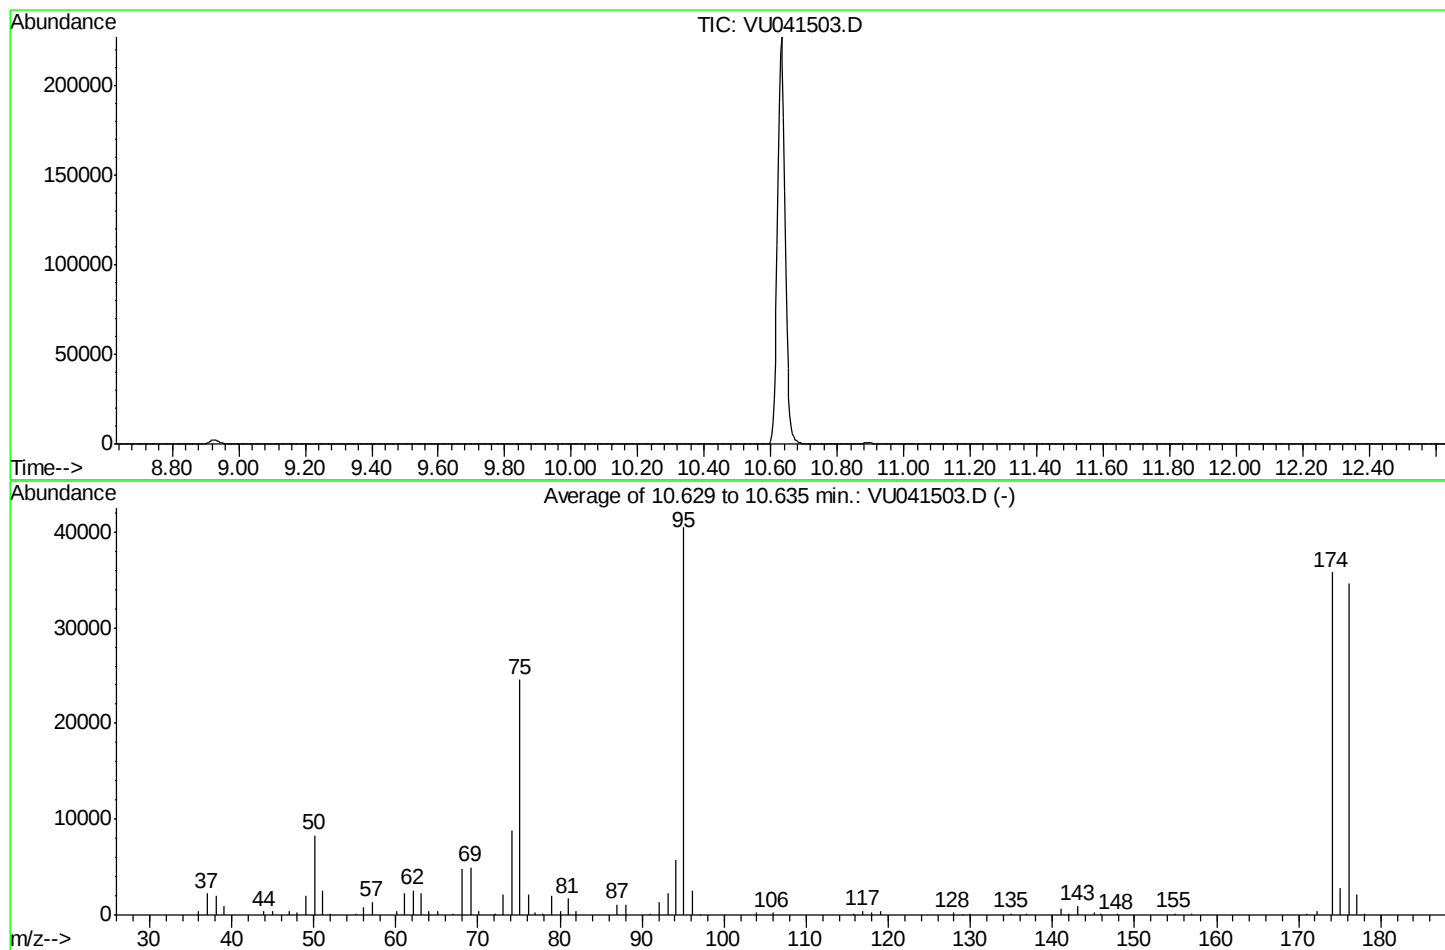

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	8348	PASS
75	95	30	80	60.6	24541	PASS
95	95	100	100	100.0	40485	PASS
96	95	5	9	6.4	2596	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.4	35800	PASS
175	174	5	9	7.8	2800	PASS
176	174	95	101	96.7	34610	PASS
177	176	5	9	6.1	2108	PASS

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	496.0
37.00	2292.0
38.10	1927.0
39.10	882.0
44.00	302.0
45.00	384.0
47.00	359.0
48.00	310.0
49.00	1918.0
50.10	8369.0
51.10	2520.0
52.10	154.0
55.20	131.0
56.10	748.0
57.10	1346.0
60.00	434.0
61.10	2227.0
62.10	2686.0
63.10	2253.0
64.00	407.0
65.10	445.0
66.90	191.0
68.10	4878.0
69.10	5167.0
70.00	367.0
71.90	201.0
73.10	2065.0
74.10	8720.0
75.10	24880.0
76.10	2175.0
77.00	216.0
77.90	132.0
78.90	1978.0
80.00	498.0
81.00	1721.0
81.90	381.0
87.00	1127.0
88.00	990.0
91.00	206.0
92.10	1435.0
93.10	2278.0
94.10	5518.0
95.10	40376.0
96.10	2646.0
104.00	230.0
105.90	247.0
115.90	194.0
116.90	428.0
118.00	281.0
119.00	450.0
127.90	201.0
130.00	186.0
135.00	137.0
136.80	119.0
141.00	561.0
141.90	115.0
143.10	996.0
145.10	223.0
145.90	148.0
147.90	127.0
154.90	143.0
171.00	150.0
172.20	366.0
174.10	34888.0
175.10	2853.0
176.10	33952.0
177.10	2128.0
178.00	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	482.0
37.00	2326.0
38.10	2034.0
39.10	917.0
44.00	370.0
45.00	343.0
47.00	384.0
48.00	348.0
49.00	2052.0
50.10	8597.0
51.10	2593.0
52.00	152.0
55.20	137.0
56.10	790.0
57.10	1407.0
60.10	462.0
61.10	2368.0
62.10	2652.0
63.10	2314.0
64.00	406.0
65.10	468.0
66.90	210.0
68.10	4908.0
69.10	5155.0
70.10	378.0
72.20	241.0
73.10	2151.0
74.10	9159.0
75.10	25392.0
76.10	2190.0
77.00	221.0
77.90	157.0
78.90	2061.0
80.00	472.0
81.00	1797.0
81.90	412.0
87.00	1147.0
88.00	1069.0
91.00	208.0
92.10	1448.0
93.10	2446.0
94.10	5939.0
95.10	41736.0
96.10	2686.0
97.10	100.0
104.00	252.0
105.90	268.0
115.80	174.0
116.90	438.0
117.90	272.0
119.00	422.0
127.90	210.0
129.00	112.0
130.00	215.0
135.00	157.0
136.80	117.0
141.00	657.0
142.00	124.0
143.10	1007.0
145.00	238.0
145.90	115.0
147.90	122.0
154.90	157.0
156.90	117.0
170.90	141.0
172.20	354.0
174.10	36952.0
175.10	2887.0
176.10	35768.0
177.10	2135.0
178.00	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
35.90	425.0
37.00	2106.0
38.00	1966.0
39.10	852.0
43.90	400.0
45.10	312.0
47.00	357.0
48.00	330.0
49.00	1930.0
50.10	8080.0
51.00	2341.0
52.00	135.0
55.00	116.0
56.00	713.0
57.10	1270.0
60.00	490.0
61.10	2260.0
62.10	2403.0
63.00	2199.0
64.00	406.0
65.10	463.0
66.90	154.0
68.10	4465.0
69.10	4676.0
70.10	317.0
72.10	263.0
73.00	2022.0
74.10	8639.0
75.10	23352.0
76.10	2041.0
77.00	227.0
77.90	198.0
79.00	1941.0
80.00	441.0
81.00	1689.0
81.90	453.0
87.00	1040.0
88.00	1086.0
91.00	191.0
92.00	1331.0
93.10	2259.0
94.10	5714.0
95.10	39344.0
96.10	2456.0
104.00	243.0
105.90	233.0
115.80	155.0
116.90	402.0
117.90	248.0
119.00	336.0
128.00	234.0
129.00	102.0
129.90	214.0
135.00	136.0
136.90	111.0
141.00	685.0
142.10	117.0
143.10	924.0
145.00	265.0
147.90	130.0
154.90	121.0
156.90	115.0
170.90	103.0
172.20	352.0
174.10	35560.0
175.10	2660.0
176.10	34112.0
177.10	2063.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21