

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046210.D
 Acq On : 09 Dec 2021 11:20
 Operator : SY/MD
 Sample : VU1209WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	92	rVB	138939	153367	16.07%	2.094%
2	1.919	172	180	196	rVB	97419	123496	12.94%	1.686%
3	2.231	276	277	281	rVB2	273	114	0.01%	0.002%
4	2.253	281	284	287	rBV2	367	274	0.03%	0.004%
5	2.353	302	315	317	rBV2	479	525	0.06%	0.007%
6	2.369	317	320	323	rBV	321	257	0.03%	0.004%
7	2.456	340	347	349	rBV2	410	502	0.05%	0.007%
8	2.575	371	384	418	rVB	218058	365622	38.31%	4.993%
9	2.790	448	451	453	rBV2	512	387	0.04%	0.005%
10	2.922	489	492	495	rBV2	277	224	0.02%	0.003%
11	3.044	527	530	531	rBV	458	272	0.03%	0.004%
12	3.305	608	611	615	rVB2	322	233	0.02%	0.003%
13	3.340	615	622	627	rBV2	486	564	0.06%	0.008%
14	3.401	634	641	643	rBV	366	326	0.03%	0.004%
15	3.446	652	655	658	rBV2	489	392	0.04%	0.005%
16	3.488	665	668	671	rBV	328	248	0.03%	0.003%
17	3.584	692	698	703	rBV2	547	589	0.06%	0.008%
18	3.617	705	708	710	rBV	251	152	0.02%	0.002%
19	3.771	753	756	758	rBV2	267	203	0.02%	0.003%
20	3.893	789	794	796	rBV	410	368	0.04%	0.005%
21	3.986	821	823	827	rBV	215	182	0.02%	0.002%
22	4.121	855	865	874	rBV2	464	1118	0.12%	0.015%
23	4.227	895	898	905	rVB	612	544	0.06%	0.007%
24	4.462	965	971	974	rBV2	412	407	0.04%	0.006%
25	4.478	974	976	978	rBV	306	186	0.02%	0.003%
26	4.507	983	985	987	rBV	257	156	0.02%	0.002%
27	4.536	992	994	996	rBV	185	125	0.01%	0.002%
28	4.639	1011	1026	1059	rBV	80969	240017	25.15%	3.277%
29	4.977	1127	1131	1133	rBV2	430	344	0.04%	0.005%
30	5.070	1145	1160	1182	rBV	160279	371896	38.97%	5.078%
31	5.237	1206	1212	1216	rBV2	465	579	0.06%	0.008%
32	5.298	1228	1231	1234	rBV3	346	213	0.02%	0.003%
33	5.353	1245	1248	1250	rBV	425	282	0.03%	0.004%
34	5.430	1269	1272	1277	rVB2	430	303	0.03%	0.004%
35	5.462	1277	1282	1285	rBV	447	363	0.04%	0.005%
36	5.729	1343	1365	1385	rBV2	355690	954289	100.00%	13.031%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046210.D
 Acq On : 09 Dec 2021 11:20
 Operator : SY/MD
 Sample : VU1209WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.086	1473	1476	1482	rBV	373	465	0.05%	0.006%
38	6.253	1513	1528	1547	rBV	248835	468936	49.14%	6.403%
39	6.533	1605	1615	1638	rBV4	4238	10070	1.06%	0.138%
40	6.694	1650	1665	1682	rBV	216257	414409	43.43%	5.659%
41	6.909	1723	1732	1735	rBV2	424	661	0.07%	0.009%
42	7.047	1772	1775	1777	rBV2	482	330	0.03%	0.005%
43	7.186	1811	1818	1821	rBV4	616	866	0.09%	0.012%
44	7.385	1877	1880	1882	rBV2	279	201	0.02%	0.003%
45	7.568	1924	1937	1953	rBV	130221	225264	23.61%	3.076%
46	7.790	2000	2006	2008	rBV2	490	516	0.05%	0.007%
47	7.899	2022	2040	2056	rBV	458236	805042	84.36%	10.993%
48	8.115	2100	2107	2111	rBV2	470	611	0.06%	0.008%
49	8.182	2116	2128	2140	rBV	89431	146992	15.40%	2.007%
50	8.420	2199	2202	2204	rBV	291	234	0.02%	0.003%
51	8.472	2215	2218	2220	rBV	326	240	0.03%	0.003%
52	8.636	2256	2269	2299	rBV	272500	486639	50.99%	6.645%
53	8.857	2335	2338	2343	rBV2	351	301	0.03%	0.004%
54	9.269	2463	2466	2470	rBV2	359	316	0.03%	0.004%
55	9.420	2500	2513	2533	rBV	361003	616476	64.60%	8.418%
56	9.780	2622	2625	2633	rBV2	306	435	0.05%	0.006%
57	9.864	2647	2651	2653	rBV	434	356	0.04%	0.005%
58	9.938	2671	2674	2675	rBV	417	237	0.02%	0.003%
59	9.983	2685	2688	2689	rBV	371	217	0.02%	0.003%
60	10.021	2694	2700	2704	rBV2	337	438	0.05%	0.006%
61	10.147	2736	2739	2742	rBV	331	262	0.03%	0.004%
62	10.562	2864	2868	2872	rBV	416	334	0.03%	0.005%
63	10.671	2898	2902	2912	rVB4	3154	3907	0.41%	0.053%
64	10.758	2917	2929	2947	rVB	316308	499168	52.31%	6.816%
65	11.041	3014	3017	3022	rBV	283	263	0.03%	0.004%
66	11.144	3047	3049	3056	rVB2	881	722	0.08%	0.010%
67	11.256	3081	3084	3089	rBV	389	260	0.03%	0.004%
68	11.285	3091	3093	3097	rVB2	516	307	0.03%	0.004%
69	11.346	3109	3112	3114	rBV	279	176	0.02%	0.002%
70	11.462	3141	3148	3162	rVB5	2261	4348	0.46%	0.059%
71	11.812	3245	3257	3272	rBV	418715	665271	69.71%	9.084%
72	11.915	3285	3289	3291	rBV2	797	644	0.07%	0.009%
73	12.050	3328	3331	3332	rBV	340	204	0.02%	0.003%
74	12.195	3362	3376	3390	rVB	458670	741400	77.69%	10.124%
75	12.333	3414	3419	3423	rBV4	823	820	0.09%	0.011%
76	12.989	3620	3623	3632	rBV	608	735	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046210.D
Acq On : 09 Dec 2021 11:20
Operator : SY/MD
Sample : VU1209WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	13.227	3690	3697	3703	rBV4	1120	1453	0.15%	0.020%
78	13.533	3789	3792	3793	rBV	426	267	0.03%	0.004%
79	13.951	3918	3922	3925	rBV	499	460	0.05%	0.006%
80	14.333	4035	4041	4047	rBV3	1646	2177	0.23%	0.030%
81	14.886	4211	4213	4217	rBV2	526	363	0.04%	0.005%
82	15.195	4306	4309	4311	rBV	475	346	0.04%	0.005%




Sum of corrected areas: 7323258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046210.D
Acq On : 09 Dec 2021 11:20
Operator : SY/MD
Sample : VU1209WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

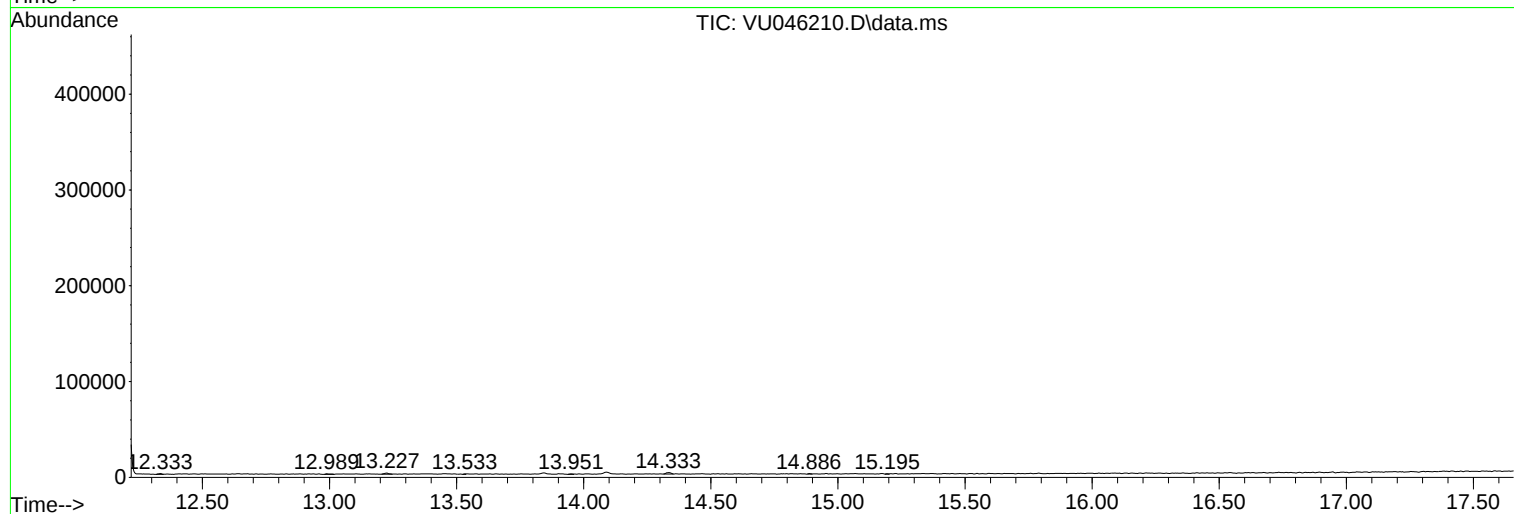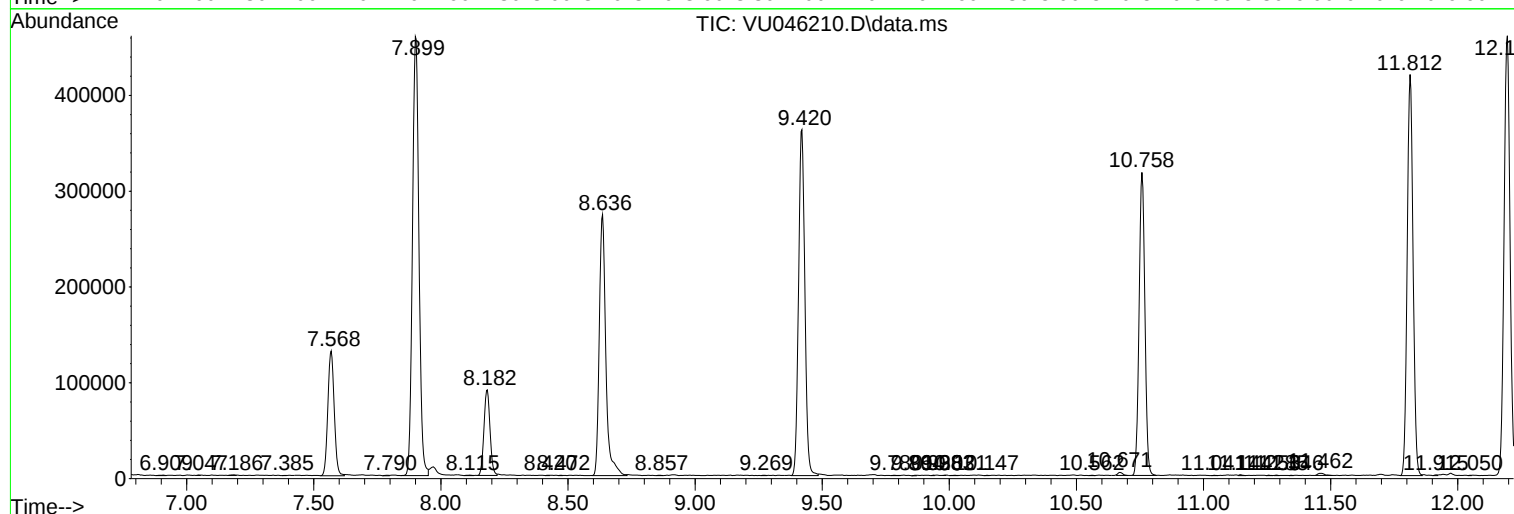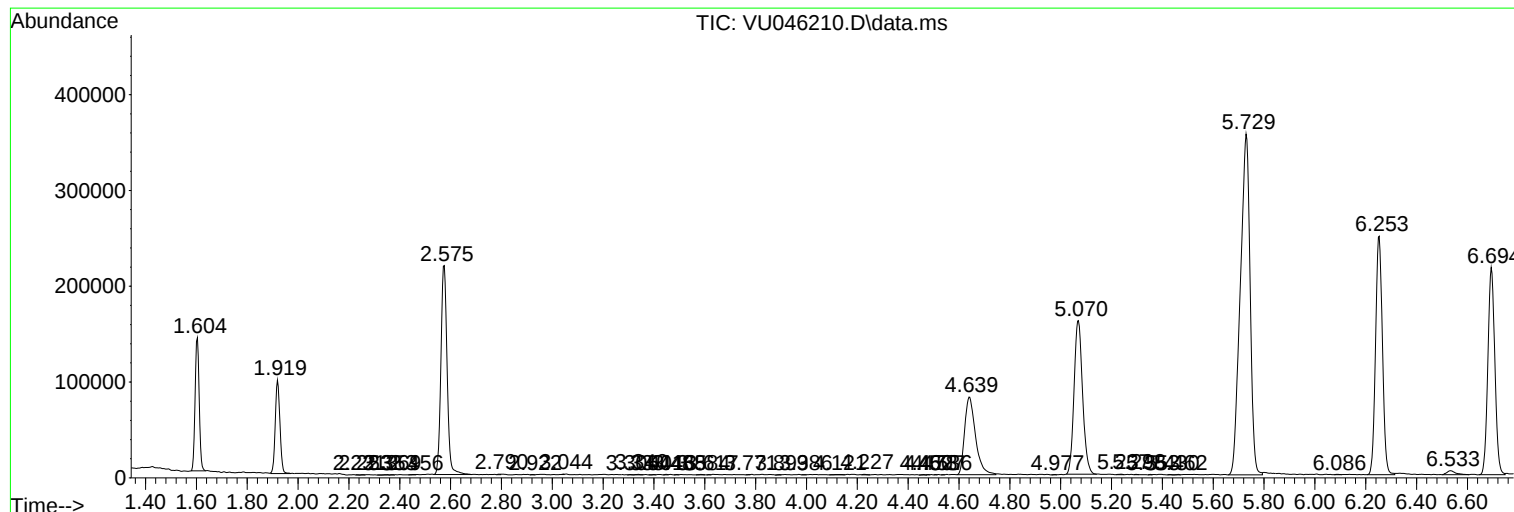

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046210.D
Acq On : 09 Dec 2021 11:20
Operator : SY/MD
Sample : VU1209WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046210.D
Acq On : 09 Dec 2021 11:20
Operator : SY/MD
Sample : VU1209WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc