

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046218.D
 Acq On : 09 Dec 2021 14:24
 Operator : SY/MD
 Sample : M4982-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	96	rVB	127044	140753	16.20%	2.074%
2	1.919	172	180	192	rVB	88308	111070	12.79%	1.637%
3	2.491	355	358	360	rBV2	564	421	0.05%	0.006%
4	2.572	371	383	404	rBV	196355	325718	37.50%	4.799%
5	2.716	424	428	432	rVB2	440	445	0.05%	0.007%
6	2.835	461	465	469	rBV	455	376	0.04%	0.006%
7	2.877	473	478	482	rBV	301	303	0.03%	0.004%
8	2.951	497	501	504	rBV	428	319	0.04%	0.005%
9	3.047	527	531	535	rVB2	669	620	0.07%	0.009%
10	3.186	571	574	577	rBV2	378	303	0.03%	0.004%
11	3.263	594	598	601	rBV	471	369	0.04%	0.005%
12	3.427	643	649	651	rVV2	394	345	0.04%	0.005%
13	3.462	658	660	664	rVB	516	316	0.04%	0.005%
14	3.620	705	709	712	rBV2	298	310	0.04%	0.005%
15	3.681	724	728	738	rVB2	493	636	0.07%	0.009%
16	3.723	738	741	744	rBV2	411	298	0.03%	0.004%
17	3.957	809	814	818	rBV2	310	313	0.04%	0.005%
18	4.022	832	834	842	rVB2	604	685	0.08%	0.010%
19	4.057	842	845	848	rBV	479	418	0.05%	0.006%
20	4.395	946	950	955	rBV	349	371	0.04%	0.005%
21	4.543	991	996	999	rBV2	577	525	0.06%	0.008%
22	4.639	1010	1026	1060	rBV2	70140	212115	24.42%	3.125%
23	5.067	1144	1159	1181	rBB	148438	336849	38.78%	4.963%
24	5.449	1274	1278	1281	rBV	527	400	0.05%	0.006%
25	5.507	1290	1296	1299	rBV2	469	522	0.06%	0.008%
26	5.626	1329	1333	1338	rBV2	377	325	0.04%	0.005%
27	5.729	1343	1365	1385	rBV2	323127	868579	100.00%	12.798%
28	6.182	1503	1506	1510	rVB	480	309	0.04%	0.005%
29	6.250	1511	1527	1544	rBV	245218	462457	53.24%	6.814%
30	6.472	1593	1596	1600	rVB	663	412	0.05%	0.006%
31	6.543	1605	1618	1633	rBV4	15970	31977	3.68%	0.471%
32	6.694	1651	1665	1683	rBV	196944	377234	43.43%	5.558%
33	6.771	1687	1689	1694	rBV3	461	354	0.04%	0.005%
34	6.813	1700	1702	1708	rVB3	738	649	0.07%	0.010%
35	6.954	1742	1746	1749	rBV	440	348	0.04%	0.005%
36	7.038	1769	1772	1777	rBV3	599	594	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046218.D
 Acq On : 09 Dec 2021 14:24
 Operator : SY/MD
 Sample : M4982-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.182	1814	1817	1822	rVB2	457	340	0.04%	0.005%
38	7.227	1827	1831	1837	rBV	551	549	0.06%	0.008%
39	7.295	1848	1852	1857	rVB	353	348	0.04%	0.005%
40	7.327	1858	1862	1865	rBV2	487	417	0.05%	0.006%
41	7.475	1903	1908	1914	rVB	549	673	0.08%	0.010%
42	7.568	1924	1937	1952	rBV	116149	204165	23.51%	3.008%
43	7.690	1971	1975	1981	rBV3	604	692	0.08%	0.010%
44	7.825	2012	2017	2020	rBV	366	415	0.05%	0.006%
45	7.899	2025	2040	2056	rBV	415982	719155	82.80%	10.596%
46	8.079	2093	2096	2103	rVB2	393	313	0.04%	0.005%
47	8.179	2116	2127	2139	rBV	79654	132343	15.24%	1.950%
48	8.478	2210	2220	2228	rVV4	1888	3035	0.35%	0.045%
49	8.632	2256	2268	2297	rBV	242808	432070	49.74%	6.366%
50	9.054	2396	2399	2403	rBV2	344	324	0.04%	0.005%
51	9.295	2466	2474	2477	rBV2	281	431	0.05%	0.006%
52	9.417	2499	2512	2536	rBV	357685	606941	69.88%	8.943%
53	9.687	2591	2596	2599	rBV3	593	687	0.08%	0.010%
54	9.851	2640	2647	2652	rBV	481	638	0.07%	0.009%
55	9.938	2670	2674	2681	rBV2	444	491	0.06%	0.007%
56	10.157	2740	2742	2749	rVB2	401	380	0.04%	0.006%
57	10.250	2767	2771	2779	rBV	513	584	0.07%	0.009%
58	10.668	2895	2901	2910	rBV3	2206	3135	0.36%	0.046%
59	10.758	2917	2929	2948	rVV	281328	450859	51.91%	6.643%
60	10.896	2967	2972	2977	rVB3	1462	1503	0.17%	0.022%
61	11.076	3024	3028	3031	rBV	463	454	0.05%	0.007%
62	11.118	3037	3041	3048	rVB3	471	602	0.07%	0.009%
63	11.462	3142	3148	3156	rVB3	1633	2696	0.31%	0.040%
64	11.529	3166	3169	3173	rVB2	506	400	0.05%	0.006%
65	11.558	3173	3178	3181	rBV2	419	450	0.05%	0.007%
66	11.684	3210	3217	3218	rBV	405	376	0.04%	0.006%
67	11.700	3218	3222	3228	rVB2	901	1023	0.12%	0.015%
68	11.735	3228	3233	3236	rBV	353	310	0.04%	0.005%
69	11.812	3244	3257	3279	rVB	424775	657111	75.65%	9.682%
70	11.947	3293	3299	3301	rBV3	660	737	0.08%	0.011%
71	11.973	3303	3307	3317	rVB4	1318	1613	0.19%	0.024%
72	12.192	3362	3375	3393	rBV	411654	670832	77.23%	9.884%
73	12.298	3404	3408	3411	rBV2	375	354	0.04%	0.005%
74	12.330	3415	3418	3420	rBV	591	361	0.04%	0.005%
75	12.726	3537	3541	3546	rBV	491	583	0.07%	0.009%
76	12.973	3615	3618	3622	rBV	437	351	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046218.D
 Acq On : 09 Dec 2021 14:24
 Operator : SY/MD
 Sample : M4982-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	13.092	3652	3655	3659	rVB	562	439	0.05%	0.006%
78	13.140	3666	3670	3674	rVV	485	410	0.05%	0.006%
79	13.166	3674	3678	3682	rVB2	466	418	0.05%	0.006%
80	13.192	3682	3686	3689	rBV	389	374	0.04%	0.006%
81	13.520	3783	3788	3793	rVB2	467	602	0.07%	0.009%
82	13.558	3798	3800	3806	rVB2	419	307	0.04%	0.005%
83	13.590	3806	3810	3813	rBV	303	300	0.03%	0.004%
84	13.716	3847	3849	3855	rVB2	528	477	0.05%	0.007%
85	13.745	3855	3858	3860	rBV	447	316	0.04%	0.005%
86	14.211	4000	4003	4010	rVB	509	428	0.05%	0.006%
87	14.243	4010	4013	4016	rBV	448	320	0.04%	0.005%
88	14.484	4085	4088	4094	rVB2	498	376	0.04%	0.006%
89	14.774	4175	4178	4181	rBV2	590	416	0.05%	0.006%
90	14.806	4185	4188	4193	rBV2	410	406	0.05%	0.006%
91	14.902	4215	4218	4223	rVB3	662	579	0.07%	0.009%
92	14.944	4223	4231	4232	rBV3	452	606	0.07%	0.009%
93	15.060	4264	4267	4270	rBV2	416	321	0.04%	0.005%
94	15.176	4300	4303	4307	rBV2	538	439	0.05%	0.006%
95	15.208	4311	4313	4320	rVB3	496	415	0.05%	0.006%
96	15.613	4434	4439	4441	rBV	620	583	0.07%	0.009%
97	16.063	4576	4579	4581	rBV	514	341	0.04%	0.005%
98	16.156	4605	4608	4611	rBV3	417	335	0.04%	0.005%
99	16.204	4620	4623	4627	rBV2	515	404	0.05%	0.006%
100	16.475	4704	4707	4712	rBV4	485	495	0.06%	0.007%




Sum of corrected areas: 6786886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046218.D
Acq On : 09 Dec 2021 14:24
Operator : SY/MD
Sample : M4982-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

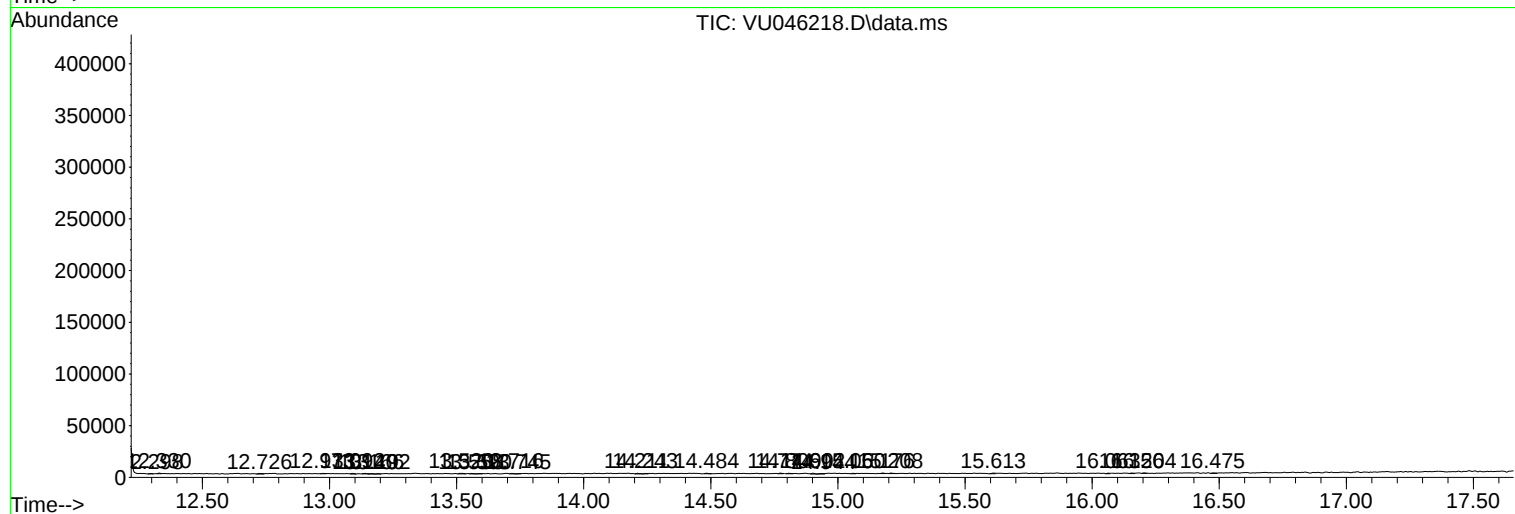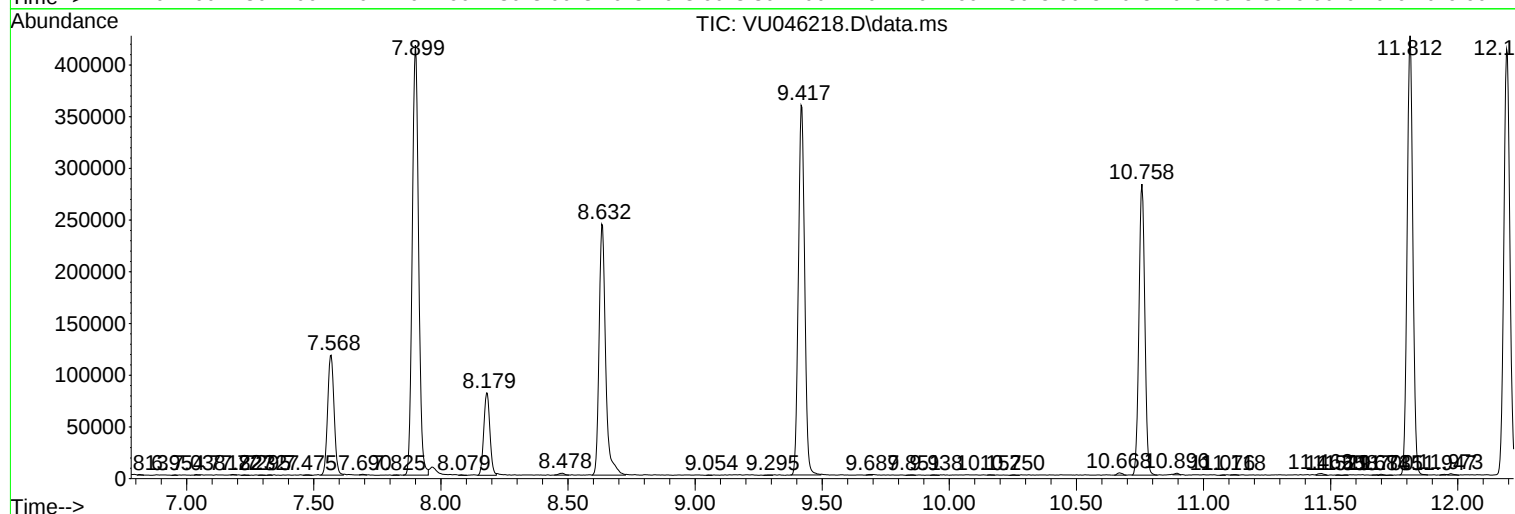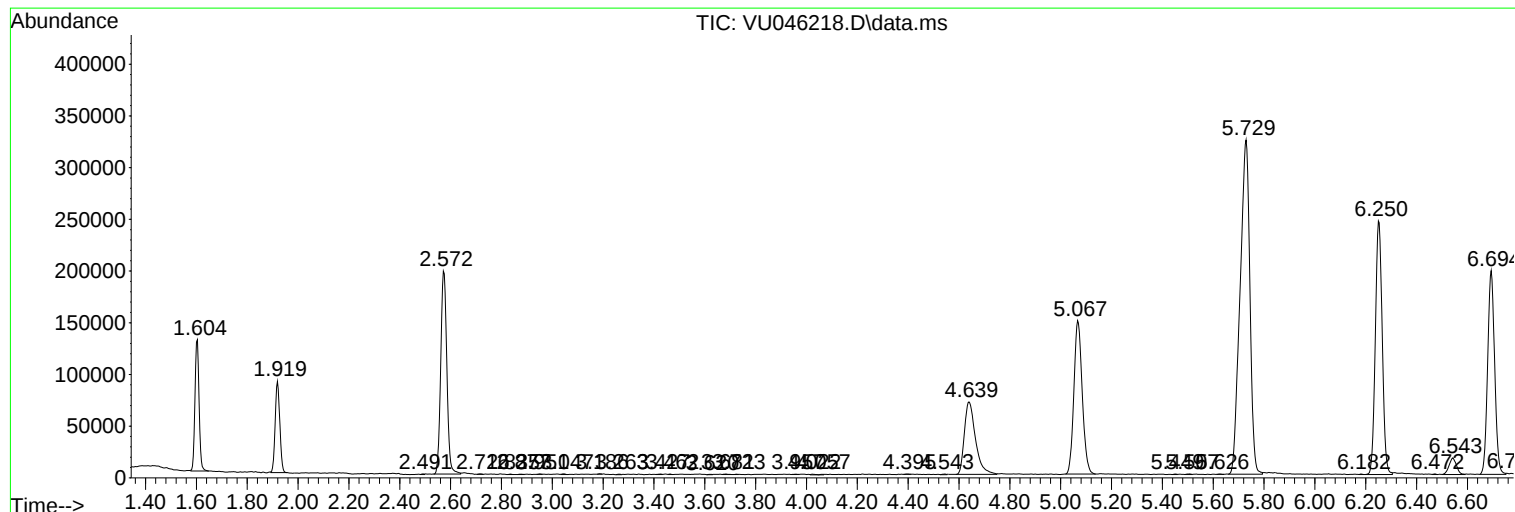

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046218.D
Acq On : 09 Dec 2021 14:24
Operator : SY/MD
Sample : M4982-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046218.D
Acq On : 09 Dec 2021 14:24
Operator : SY/MD
Sample : M4982-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------