

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046219.D
 Acq On : 09 Dec 2021 14:47
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	98	rVB	131267	146037	15.94%	2.126%
2	1.919	172	180	193	rVB	93035	118978	12.98%	1.732%
3	2.202	265	268	271	rBV3	398	262	0.03%	0.004%
4	2.257	278	285	287	rBV2	682	709	0.08%	0.010%
5	2.421	333	336	339	rBV2	505	402	0.04%	0.006%
6	2.523	365	368	370	rBV	390	248	0.03%	0.004%
7	2.572	371	383	400	rBV	207900	343889	37.53%	5.006%
8	2.716	426	428	431	rBV	376	213	0.02%	0.003%
9	2.864	471	474	481	rVB2	433	395	0.04%	0.006%
10	2.896	481	484	486	rBV2	446	332	0.04%	0.005%
11	2.941	495	498	500	rBV	379	259	0.03%	0.004%
12	3.125	552	555	559	rBV	361	290	0.03%	0.004%
13	3.147	559	562	567	rVV	367	352	0.04%	0.005%
14	3.318	612	615	618	rBV	394	233	0.03%	0.003%
15	3.774	754	757	760	rBV	342	230	0.03%	0.003%
16	4.028	833	836	839	rBV2	428	299	0.03%	0.004%
17	4.237	898	901	905	rBV	567	420	0.05%	0.006%
18	4.256	905	907	910	rVV2	360	230	0.03%	0.003%
19	4.392	946	949	952	rBV	428	278	0.03%	0.004%
20	4.433	956	962	965	rBV2	520	572	0.06%	0.008%
21	4.491	977	980	983	rBV	351	246	0.03%	0.004%
22	4.543	991	996	999	rBV2	414	417	0.05%	0.006%
23	4.639	1010	1026	1064	rBV2	75417	230394	25.14%	3.354%
24	4.842	1086	1089	1093	rVB	526	355	0.04%	0.005%
25	5.067	1142	1159	1181	rBV	157162	360072	39.29%	5.241%
26	5.260	1214	1219	1222	rBV2	733	669	0.07%	0.010%
27	5.292	1226	1229	1234	rBV2	426	287	0.03%	0.004%
28	5.324	1235	1239	1244	rVB2	468	401	0.04%	0.006%
29	5.729	1343	1365	1382	rVV2	342753	916399	100.00%	13.339%
30	6.186	1504	1507	1510	rBV	355	226	0.02%	0.003%
31	6.250	1514	1527	1543	rBV	210878	397071	43.33%	5.780%
32	6.494	1600	1603	1605	rBV	413	301	0.03%	0.004%
33	6.543	1605	1618	1633	rVB4	22238	43254	4.72%	0.630%
34	6.694	1650	1665	1682	rBV	207134	400697	43.73%	5.833%
35	6.809	1697	1701	1704	rVB3	695	493	0.05%	0.007%
36	6.986	1753	1756	1759	rVB	400	250	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046219.D
 Acq On : 09 Dec 2021 14:47
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.125	1796	1799	1804	rBV	281	279	0.03%	0.004%
38	7.362	1870	1873	1877	rBV	309	234	0.03%	0.003%
39	7.523	1920	1923	1924	rBV	482	242	0.03%	0.004%
40	7.568	1924	1937	1952	rVV	122856	211123	23.04%	3.073%
41	7.681	1969	1972	1974	rBV2	428	325	0.04%	0.005%
42	7.813	2008	2013	2015	rBV	322	272	0.03%	0.004%
43	7.899	2027	2040	2057	rBV	446885	768150	83.82%	11.181%
44	8.121	2106	2109	2114	rVB	364	315	0.03%	0.005%
45	8.179	2114	2127	2143	rBV	84022	140197	15.30%	2.041%
46	8.276	2155	2157	2160	rBV2	387	250	0.03%	0.004%
47	8.356	2178	2182	2185	rVB2	349	300	0.03%	0.004%
48	8.475	2212	2219	2224	rBV3	1083	1409	0.15%	0.021%
49	8.555	2238	2244	2247	rBV	392	359	0.04%	0.005%
50	8.636	2256	2269	2299	rBV	258198	463445	50.57%	6.746%
51	8.870	2339	2342	2348	rVB2	227	254	0.03%	0.004%
52	8.903	2348	2352	2355	rBV2	455	356	0.04%	0.005%
53	8.922	2355	2358	2364	rBV	334	343	0.04%	0.005%
54	9.041	2392	2395	2399	rVB2	410	268	0.03%	0.004%
55	9.128	2419	2422	2424	rBV2	290	220	0.02%	0.003%
56	9.192	2437	2442	2446	rBV	288	273	0.03%	0.004%
57	9.282	2466	2470	2473	rBV2	302	241	0.03%	0.004%
58	9.346	2486	2490	2494	rVB	423	318	0.03%	0.005%
59	9.417	2499	2512	2544	rBV	318320	530062	57.84%	7.716%
60	9.539	2547	2550	2553	rBV	334	210	0.02%	0.003%
61	9.578	2553	2562	2565	rBV3	435	655	0.07%	0.010%
62	9.626	2574	2577	2580	rBV2	319	222	0.02%	0.003%
63	9.690	2594	2597	2600	rBV3	537	369	0.04%	0.005%
64	9.819	2631	2637	2645	rBV	440	732	0.08%	0.011%
65	9.858	2646	2649	2654	rVV2	367	381	0.04%	0.006%
66	9.938	2666	2674	2678	rBV2	535	826	0.09%	0.012%
67	10.015	2693	2698	2702	rBV2	453	491	0.05%	0.007%
68	10.202	2751	2756	2758	rBV2	412	356	0.04%	0.005%
69	10.414	2818	2822	2825	rVB	652	459	0.05%	0.007%
70	10.443	2825	2831	2833	rBV2	345	340	0.04%	0.005%
71	10.494	2843	2847	2850	rBV	344	316	0.03%	0.005%
72	10.603	2876	2881	2883	rBV2	310	281	0.03%	0.004%
73	10.636	2888	2891	2893	rVV2	404	287	0.03%	0.004%
74	10.671	2896	2902	2913	rVB3	2410	3507	0.38%	0.051%
75	10.758	2916	2929	2948	rVB	300548	479836	52.36%	6.985%
76	10.829	2948	2951	2954	rVB	338	211	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046219.D
 Acq On : 09 Dec 2021 14:47
 Operator : SY/MD
 Sample : M4982-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.243	3076	3080	3088	rBV	372	531	0.06%	0.008%
78	11.353	3111	3114	3116	rBV	358	260	0.03%	0.004%
79	11.404	3127	3130	3133	rBV	438	324	0.04%	0.005%
80	11.459	3140	3147	3154	rBV4	1317	1863	0.20%	0.027%
81	11.652	3204	3207	3210	rBV	345	299	0.03%	0.004%
82	11.697	3215	3221	3222	rBV3	752	741	0.08%	0.011%
83	11.812	3245	3257	3277	rVB	363442	574088	62.65%	8.357%
84	11.893	3277	3282	3286	rBV3	404	459	0.05%	0.007%
85	11.970	3303	3306	3318	rVB3	1595	1747	0.19%	0.025%
86	12.150	3357	3362	3363	rBV3	538	428	0.05%	0.006%
87	12.192	3363	3375	3390	rVV	444506	709177	77.39%	10.323%
88	12.272	3398	3400	3404	rBV2	382	252	0.03%	0.004%
89	12.462	3457	3459	3462	rBV2	348	212	0.02%	0.003%
90	12.706	3531	3535	3539	rBV2	378	360	0.04%	0.005%
91	12.758	3548	3551	3553	rBV2	453	345	0.04%	0.005%
92	12.964	3612	3615	3618	rBV2	469	294	0.03%	0.004%
93	13.198	3685	3688	3690	rBV	329	250	0.03%	0.004%
94	13.275	3709	3712	3713	rBV2	387	221	0.02%	0.003%
95	13.311	3719	3723	3727	rBV2	546	528	0.06%	0.008%
96	13.909	3906	3909	3911	rBV	420	322	0.04%	0.005%
97	13.951	3919	3922	3926	rVB	488	321	0.04%	0.005%
98	14.127	3974	3977	3984	rBV2	399	503	0.05%	0.007%
99	14.417	4060	4067	4071	rBV2	636	867	0.09%	0.013%
100	16.047	4571	4574	4583	rVB2	554	691	0.08%	0.010%




Sum of corrected areas: 6869957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046219.D
Acq On : 09 Dec 2021 14:47
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

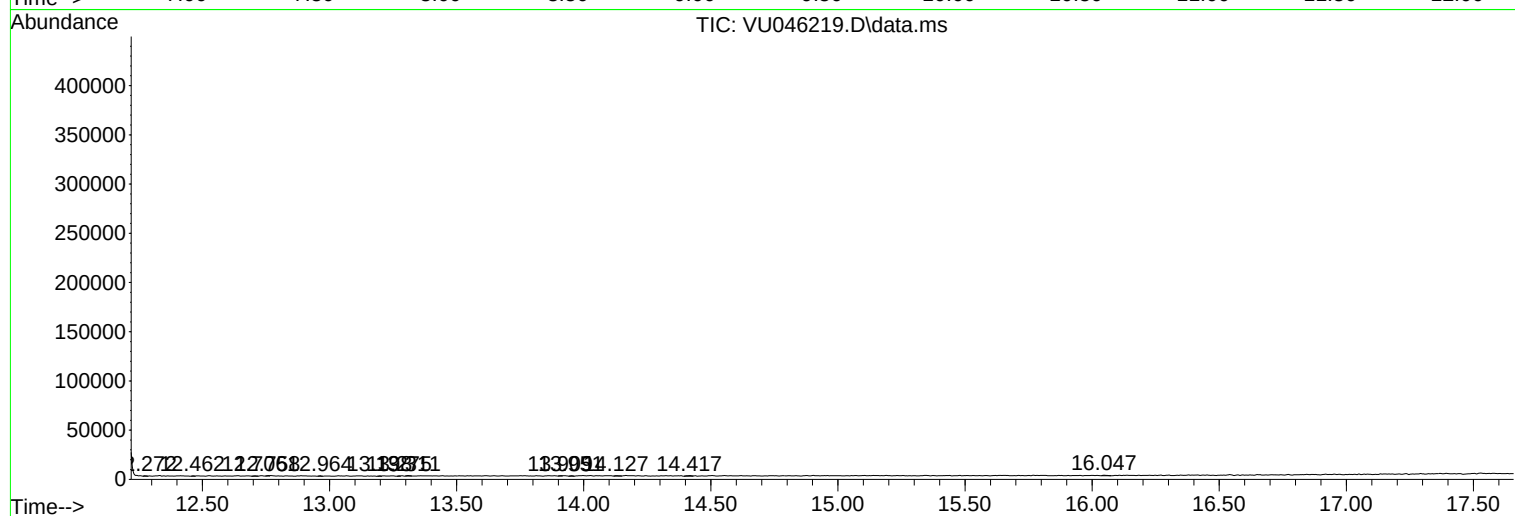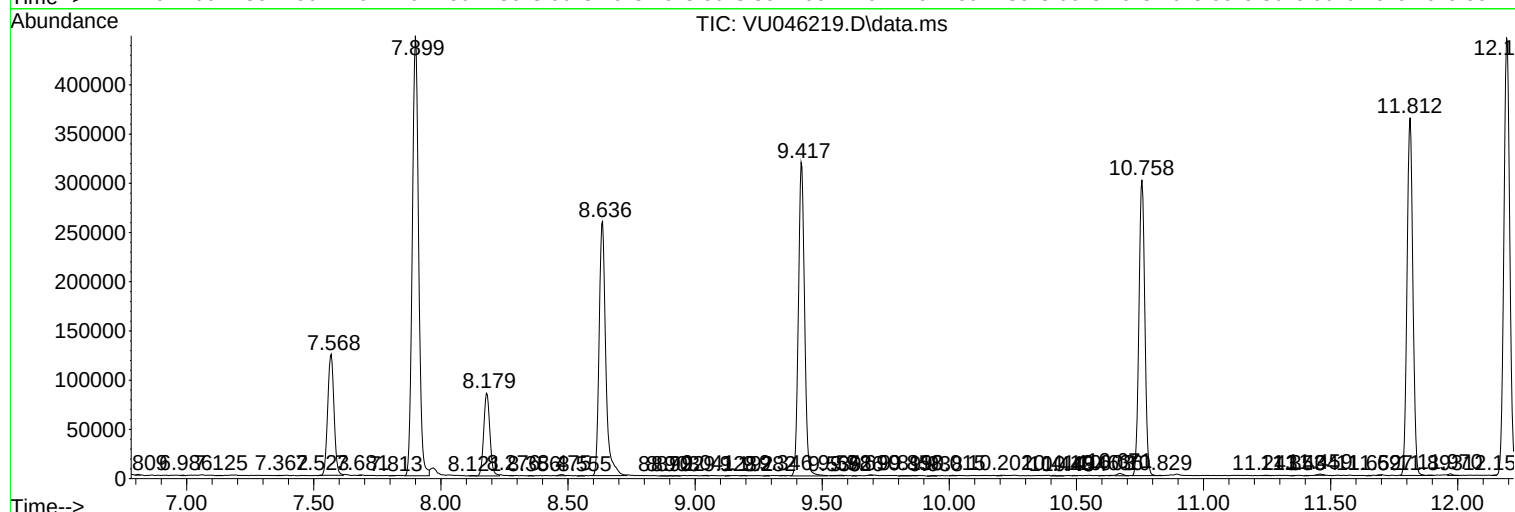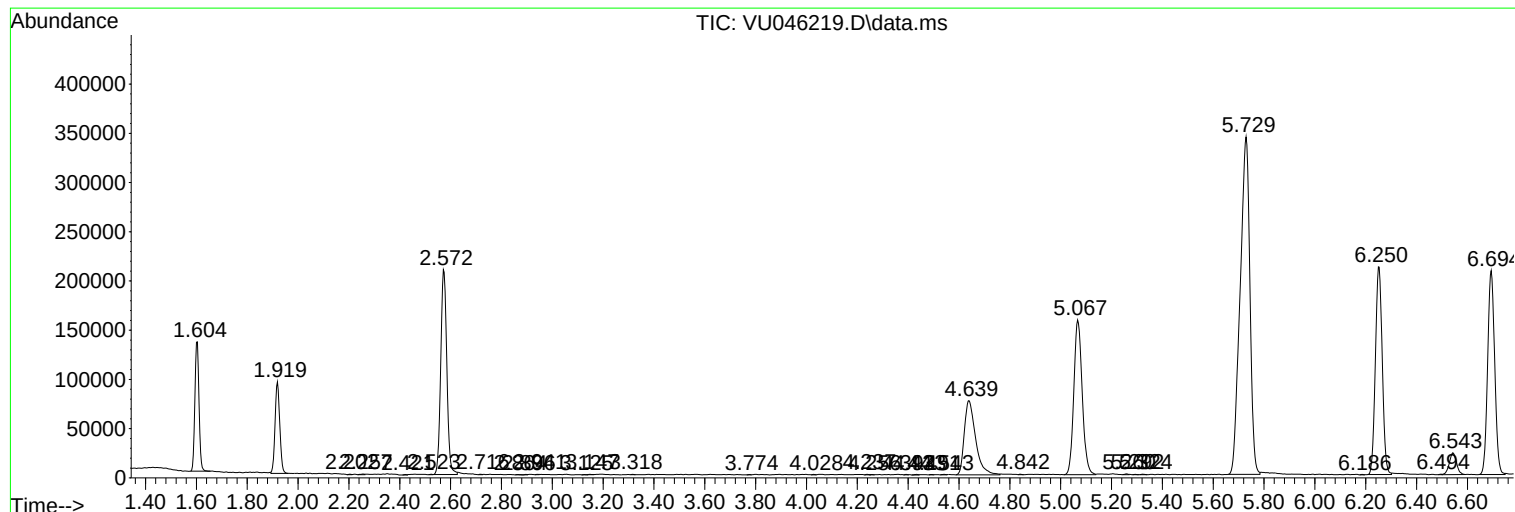

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046219.D
Acq On : 09 Dec 2021 14:47
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046219.D
Acq On : 09 Dec 2021 14:47
Operator : SY/MD
Sample : M4982-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc