

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046225.D
 Acq On : 09 Dec 2021 17:21
 Operator : SY/MD
 Sample : M4983-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5P2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	95	rVB	116054	128513	11.72%	1.591%
2	1.919	171	180	193	rVB	81756	105012	9.58%	1.300%
3	2.231	273	277	279	rBV2	384	271	0.02%	0.003%
4	2.254	279	284	290	rVB3	548	636	0.06%	0.008%
5	2.286	290	294	295	rBV	422	317	0.03%	0.004%
6	2.417	332	335	338	rVB2	418	246	0.02%	0.003%
7	2.437	338	341	343	rBV2	433	280	0.03%	0.003%
8	2.575	371	384	401	rBV2	185676	326932	29.82%	4.048%
9	2.800	449	454	458	rVB4	790	850	0.08%	0.011%
10	3.028	521	525	528	rBV	496	398	0.04%	0.005%
11	3.048	528	531	534	rVB	467	285	0.03%	0.004%
12	3.089	541	544	550	rVB2	440	427	0.04%	0.005%
13	3.231	585	588	594	rBV2	445	423	0.04%	0.005%
14	3.360	620	628	637	rVB2	2422	4189	0.38%	0.052%
15	3.559	686	690	693	rBV2	283	300	0.03%	0.004%
16	3.877	774	789	805	rVB	34504	80945	7.38%	1.002%
17	4.080	850	852	858	rVB	436	386	0.04%	0.005%
18	4.118	858	864	866	rBV	371	431	0.04%	0.005%
19	4.186	882	885	888	rBV2	370	271	0.02%	0.003%
20	4.424	957	959	965	rVB2	385	388	0.04%	0.005%
21	4.450	965	967	973	rVB	354	291	0.03%	0.004%
22	4.482	973	977	981	rBV	335	318	0.03%	0.004%
23	4.659	1011	1032	1064	rVV2	74366	294313	26.84%	3.644%
24	4.993	1131	1136	1139	rVB2	612	502	0.05%	0.006%
25	5.067	1143	1159	1183	rVV	136101	317939	29.00%	3.937%
26	5.160	1183	1188	1196	rBV3	506	992	0.09%	0.012%
27	5.321	1216	1238	1259	rBV	489871	1096375	100.00%	13.575%
28	5.729	1343	1365	1386	rBV2	296797	801546	73.11%	9.925%
29	5.935	1426	1429	1433	rBV3	324	307	0.03%	0.004%
30	6.080	1470	1474	1480	rBV2	433	578	0.05%	0.007%
31	6.250	1510	1527	1546	rBV	231049	433797	39.57%	5.371%
32	6.449	1587	1589	1594	rVB	364	268	0.02%	0.003%
33	6.543	1605	1618	1636	rBV2	88604	168716	15.39%	2.089%
34	6.694	1652	1665	1684	rBV	181815	349245	31.85%	4.324%
35	7.003	1758	1761	1764	rBV	529	431	0.04%	0.005%
36	7.044	1770	1774	1776	rBV	397	309	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046225.D
 Acq On : 09 Dec 2021 17:21
 Operator : SY/MD
 Sample : M4983-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5P2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.121	1794	1798	1802	rBV	351	291	0.03%	0.004%
38	7.157	1806	1809	1812	rBV	454	357	0.03%	0.004%
39	7.179	1812	1816	1820	rBV3	539	559	0.05%	0.007%
40	7.334	1861	1864	1868	rBV2	351	310	0.03%	0.004%
41	7.359	1870	1872	1876	rVB2	407	265	0.02%	0.003%
42	7.388	1876	1881	1884	rBV2	390	443	0.04%	0.005%
43	7.449	1895	1900	1903	rVB	398	296	0.03%	0.004%
44	7.469	1903	1906	1911	rVB2	411	390	0.04%	0.005%
45	7.498	1911	1915	1918	rBV2	478	447	0.04%	0.006%
46	7.568	1918	1937	1957	rBV	109047	190064	17.34%	2.353%
47	7.678	1969	1971	1976	rVB3	444	273	0.02%	0.003%
48	7.900	2027	2040	2057	rBV	377149	658891	60.10%	8.158%
49	8.041	2081	2084	2088	rBV2	388	322	0.03%	0.004%
50	8.179	2113	2127	2143	rBV	77885	136067	12.41%	1.685%
51	8.318	2167	2170	2175	rVB2	330	343	0.03%	0.004%
52	8.350	2175	2180	2182	rBV2	381	371	0.03%	0.005%
53	8.401	2187	2196	2203	rVV5	1157	1627	0.15%	0.020%
54	8.449	2208	2211	2213	rBV	359	245	0.02%	0.003%
55	8.472	2213	2218	2230	rVB3	1442	2256	0.21%	0.028%
56	8.556	2230	2244	2257	rBV	157166	268786	24.52%	3.328%
57	8.636	2257	2269	2297	rVB	235846	422524	38.54%	5.232%
58	8.855	2331	2337	2341	rBV2	565	684	0.06%	0.008%
59	8.967	2370	2372	2382	rVB	465	335	0.03%	0.004%
60	9.102	2412	2414	2422	rVB	396	365	0.03%	0.005%
61	9.150	2425	2429	2435	rBV	389	410	0.04%	0.005%
62	9.417	2500	2512	2534	rBV	342790	569929	51.98%	7.057%
63	9.568	2555	2559	2565	rVB	670	674	0.06%	0.008%
64	9.697	2592	2599	2607	rBV3	969	1453	0.13%	0.018%
65	10.105	2719	2726	2735	rBV4	638	1057	0.10%	0.013%
66	10.192	2749	2753	2756	rBV2	470	378	0.03%	0.005%
67	10.256	2768	2773	2776	rBV2	336	337	0.03%	0.004%
68	10.408	2817	2820	2824	rBV2	277	240	0.02%	0.003%
69	10.584	2872	2875	2878	rVV	421	359	0.03%	0.004%
70	10.600	2878	2880	2884	rVB	371	237	0.02%	0.003%
71	10.671	2896	2902	2907	rVB6	831	1004	0.09%	0.012%
72	10.758	2917	2929	2947	rVB	268562	431207	39.33%	5.339%
73	10.835	2948	2953	2956	rBV2	466	444	0.04%	0.005%
74	10.893	2966	2971	2978	rVB4	1563	2183	0.20%	0.027%
75	11.115	3036	3040	3047	rVB4	996	963	0.09%	0.012%
76	11.260	3083	3085	3089	rVB	498	343	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046225.D
 Acq On : 09 Dec 2021 17:21
 Operator : SY/MD
 Sample : M4983-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5P2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.289	3089	3094	3100	rBV	572	726	0.07%	0.009%
78	11.469	3143	3150	3158	rVB4	2036	3166	0.29%	0.039%
79	11.668	3209	3212	3217	rBV	339	310	0.03%	0.004%
80	11.697	3217	3221	3226	rVV3	668	580	0.05%	0.007%
81	11.745	3233	3236	3238	rBV	375	255	0.02%	0.003%
82	11.813	3244	3257	3277	rBV	389507	619217	56.48%	7.667%
83	11.973	3302	3307	3312	rVB5	953	1199	0.11%	0.015%
84	12.063	3328	3335	3343	rBV5	1892	2934	0.27%	0.036%
85	12.195	3363	3376	3393	rVV	389520	624779	56.99%	7.736%
86	12.260	3393	3396	3402	rVB2	570	503	0.05%	0.006%
87	12.333	3416	3419	3423	rVB3	570	347	0.03%	0.004%
88	12.597	3498	3501	3508	rBV2	520	551	0.05%	0.007%
89	12.764	3549	3553	3566	rVB4	901	1649	0.15%	0.020%
90	12.819	3566	3570	3574	rBV	520	551	0.05%	0.007%
91	13.742	3853	3857	3859	rBV2	455	405	0.04%	0.005%
92	14.038	3946	3949	3951	rBV2	352	243	0.02%	0.003%
93	14.324	4034	4038	4042	rBV2	406	397	0.04%	0.005%
94	14.822	4189	4193	4195	rBV3	420	294	0.03%	0.004%
95	14.877	4206	4210	4213	rBV2	529	416	0.04%	0.005%
96	14.970	4235	4239	4242	rBV	576	475	0.04%	0.006%
97	15.211	4307	4314	4317	rBV2	725	957	0.09%	0.012%
98	15.411	4373	4376	4378	rBV2	417	290	0.03%	0.004%
99	15.620	4438	4441	4446	rVB	495	406	0.04%	0.005%
100	16.237	4629	4633	4636	rBV2	435	415	0.04%	0.005%




Sum of corrected areas: 8076221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046225.D
Acq On : 09 Dec 2021 17:21
Operator : SY/MD
Sample : M4983-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

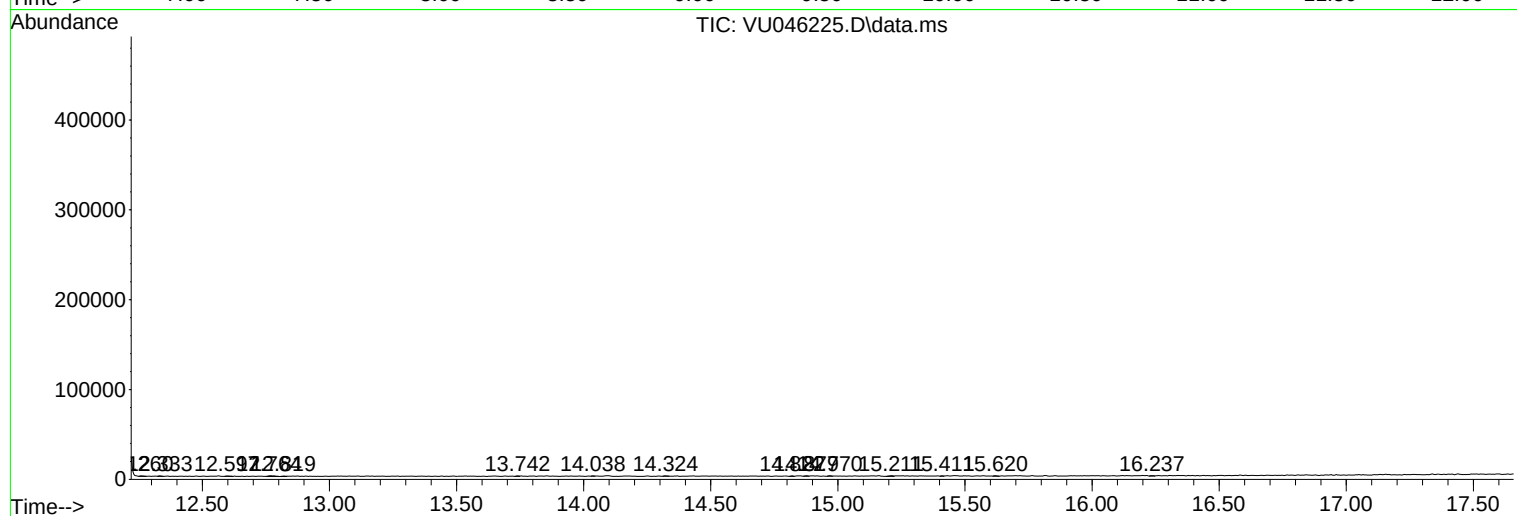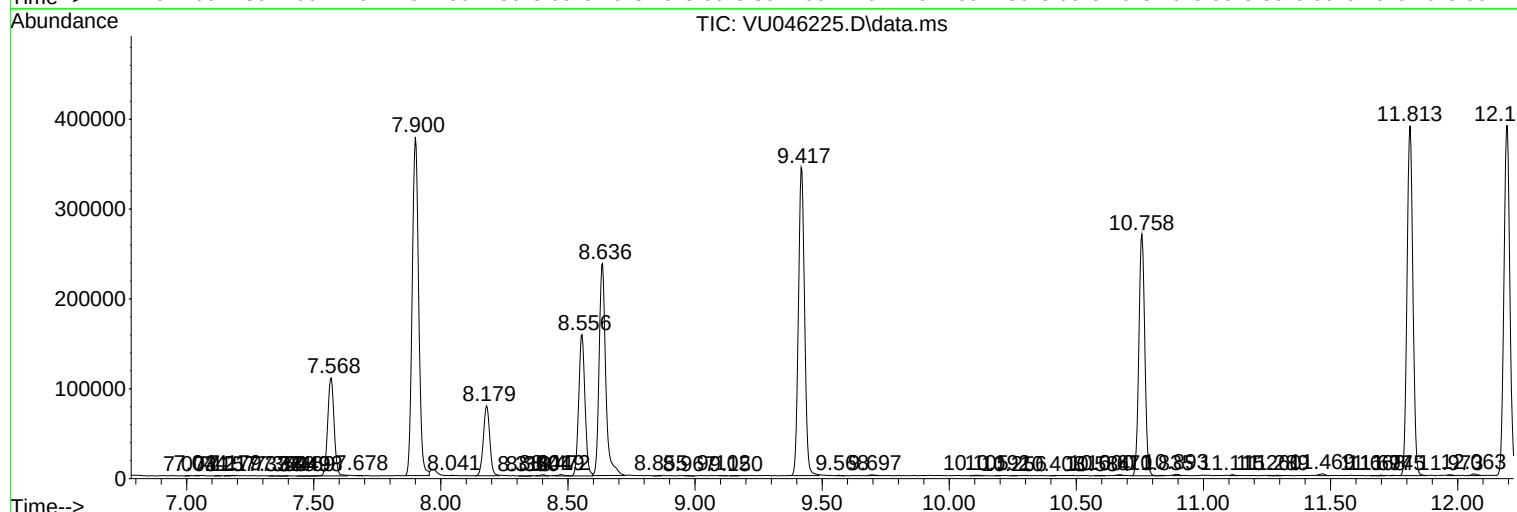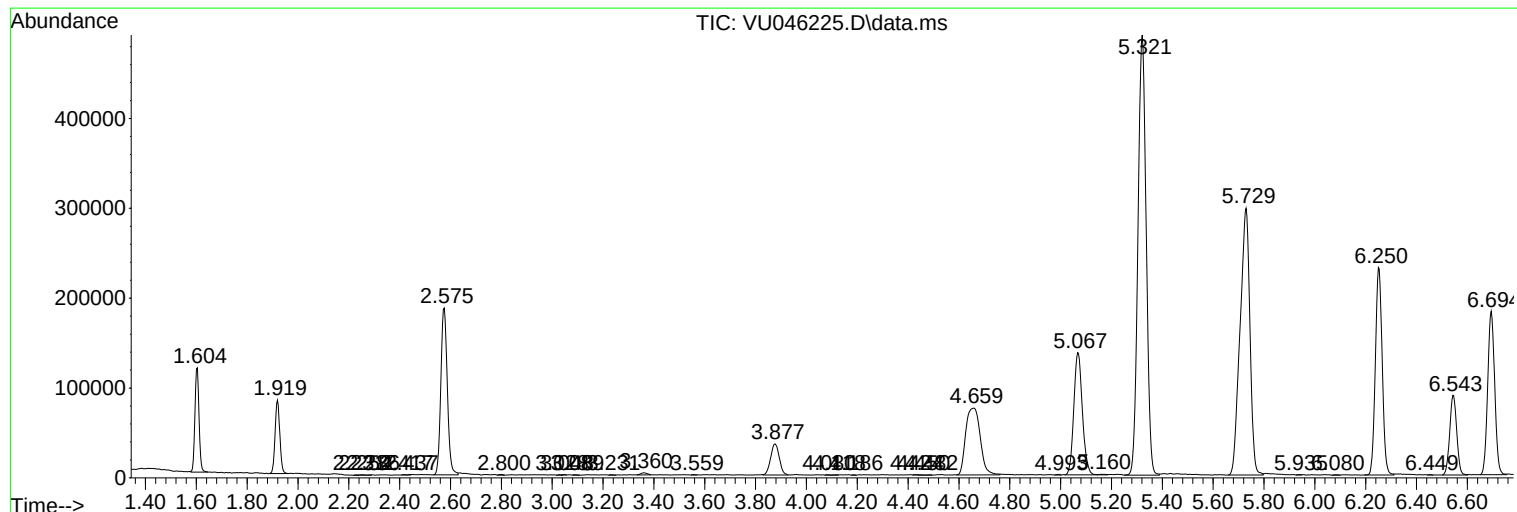

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046225.D
Acq On : 09 Dec 2021 17:21
Operator : SY/MD
Sample : M4983-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046225.D
Acq On : 09 Dec 2021 17:21
Operator : SY/MD
Sample : M4983-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------