

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046229.D
 Acq On : 09 Dec 2021 18:50
 Operator : SY/MD
 Sample : M4983-17
 Misc : 5.4mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	105304	116580	10.91%	1.468%
2	1.919	172	180	194	rVB	76815	98432	9.21%	1.239%
3	2.208	268	270	271	rBB	63	37	0.00%	0.000%
4	2.247	280	282	283	rBV	213	81	0.01%	0.001%
5	2.292	293	296	299	rBV2	354	213	0.02%	0.003%
6	2.372	318	321	323	rBV	376	251	0.02%	0.003%
7	2.478	350	354	356	rBV2	354	301	0.03%	0.004%
8	2.514	360	365	367	rBV2	483	430	0.04%	0.005%
9	2.575	372	384	405	rBV2	176581	310809	29.08%	3.914%
10	2.742	433	436	441	rVB2	472	362	0.03%	0.005%
11	2.890	478	482	486	rBV2	377	345	0.03%	0.004%
12	2.928	491	494	500	rBB	290	284	0.03%	0.004%
13	2.957	500	503	507	rBV2	494	380	0.04%	0.005%
14	3.224	583	586	588	rBV2	327	233	0.02%	0.003%
15	3.359	614	628	641	rBV4	8812	17717	1.66%	0.223%
16	3.411	641	644	647	rBV	490	332	0.03%	0.004%
17	3.462	652	660	666	rBV2	387	684	0.06%	0.009%
18	3.565	690	692	694	rBV	139	77	0.01%	0.001%
19	3.874	773	788	807	rBV	61413	142867	13.37%	1.799%
20	3.999	824	827	829	rBV	350	227	0.02%	0.003%
21	4.231	896	899	901	rBV	428	314	0.03%	0.004%
22	4.308	918	923	925	rBV	358	317	0.03%	0.004%
23	4.391	946	949	951	rBV2	238	165	0.02%	0.002%
24	4.507	982	985	987	rBV	326	206	0.02%	0.003%
25	4.671	1011	1036	1061	rBV2	408711	1068707	100.00%	13.457%
26	4.954	1122	1124	1126	rBV2	420	241	0.02%	0.003%
27	5.067	1144	1159	1182	rBV	130276	304725	28.51%	3.837%
28	5.321	1220	1238	1260	rBV	297747	664880	62.21%	8.372%
29	5.729	1343	1365	1383	rBV2	282781	764671	71.55%	9.628%
30	6.250	1514	1527	1544	rBV	229506	433956	40.61%	5.464%
31	6.542	1606	1618	1632	rBV5	14997	30015	2.81%	0.378%
32	6.694	1651	1665	1681	rBV	174693	336944	31.53%	4.243%
33	7.070	1780	1782	1787	rVB	502	281	0.03%	0.004%
34	7.186	1811	1818	1823	rVB3	961	1120	0.10%	0.014%
35	7.231	1823	1832	1836	rBV	312	539	0.05%	0.007%
36	7.414	1886	1889	1891	rBV	394	300	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046229.D
 Acq On : 09 Dec 2021 18:50
 Operator : SY/MD
 Sample : M4983-17
 Misc : 5.4mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW5P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.449	1897	1900	1905	rBV	361	350	0.03%	0.004%
38	7.568	1925	1937	1963	rVB	103357	178309	16.68%	2.245%
39	7.767	1997	1999	2001	rBV2	298	199	0.02%	0.003%
40	7.812	2009	2013	2018	rVB2	616	605	0.06%	0.008%
41	7.851	2018	2025	2027	rBV	541	629	0.06%	0.008%
42	7.899	2027	2040	2057	rBV	355491	617697	57.80%	7.778%
43	8.115	2104	2107	2110	rBV	451	358	0.03%	0.005%
44	8.179	2116	2127	2145	rBV2	70229	118201	11.06%	1.488%
45	8.475	2212	2219	2229	rBV3	1007	1804	0.17%	0.023%
46	8.555	2233	2244	2257	rBV	58671	98096	9.18%	1.235%
47	8.636	2257	2269	2296	rBV	234382	416515	38.97%	5.245%
48	8.880	2341	2345	2349	rBV	464	349	0.03%	0.004%
49	9.054	2396	2399	2401	rBV	353	253	0.02%	0.003%
50	9.192	2437	2442	2445	rBV2	418	455	0.04%	0.006%
51	9.275	2464	2468	2469	rBV2	366	248	0.02%	0.003%
52	9.308	2474	2478	2482	rBV2	334	350	0.03%	0.004%
53	9.420	2499	2513	2535	rBV	346590	576942	53.99%	7.265%
54	10.362	2803	2806	2809	rBV	372	300	0.03%	0.004%
55	10.468	2835	2839	2845	rBV	536	622	0.06%	0.008%
56	10.510	2845	2852	2855	rBV	515	591	0.06%	0.007%
57	10.555	2863	2866	2868	rBV2	238	150	0.01%	0.002%
58	10.574	2869	2872	2875	rBV2	398	297	0.03%	0.004%
59	10.626	2885	2888	2890	rBV2	363	256	0.02%	0.003%
60	10.758	2917	2929	2949	rVB	258186	417641	39.08%	5.259%
61	10.931	2978	2983	2987	rBV	354	378	0.04%	0.005%
62	11.156	3049	3053	3055	rBV	445	354	0.03%	0.004%
63	11.812	3244	3257	3275	rBV	399039	619441	57.96%	7.800%
64	12.195	3364	3376	3395	rVB	366959	591578	55.35%	7.449%
65	12.549	3480	3486	3488	rBV	483	614	0.06%	0.008%
66	14.494	4089	4091	4094	rBV2	211	127	0.01%	0.002%
67	14.655	4139	4141	4145	rBV2	339	183	0.02%	0.002%




Sum of corrected areas: 7941915

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046229.D
Acq On : 09 Dec 2021 18:50
Operator : SY/MD
Sample : M4983-17
Misc : 5.4mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

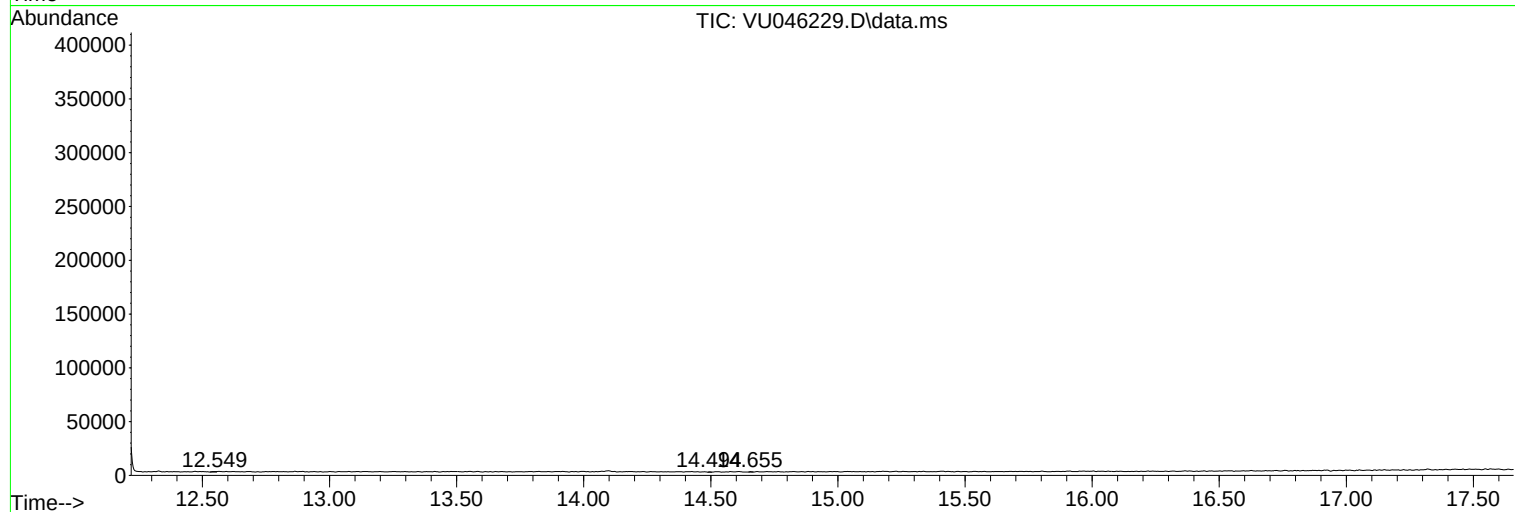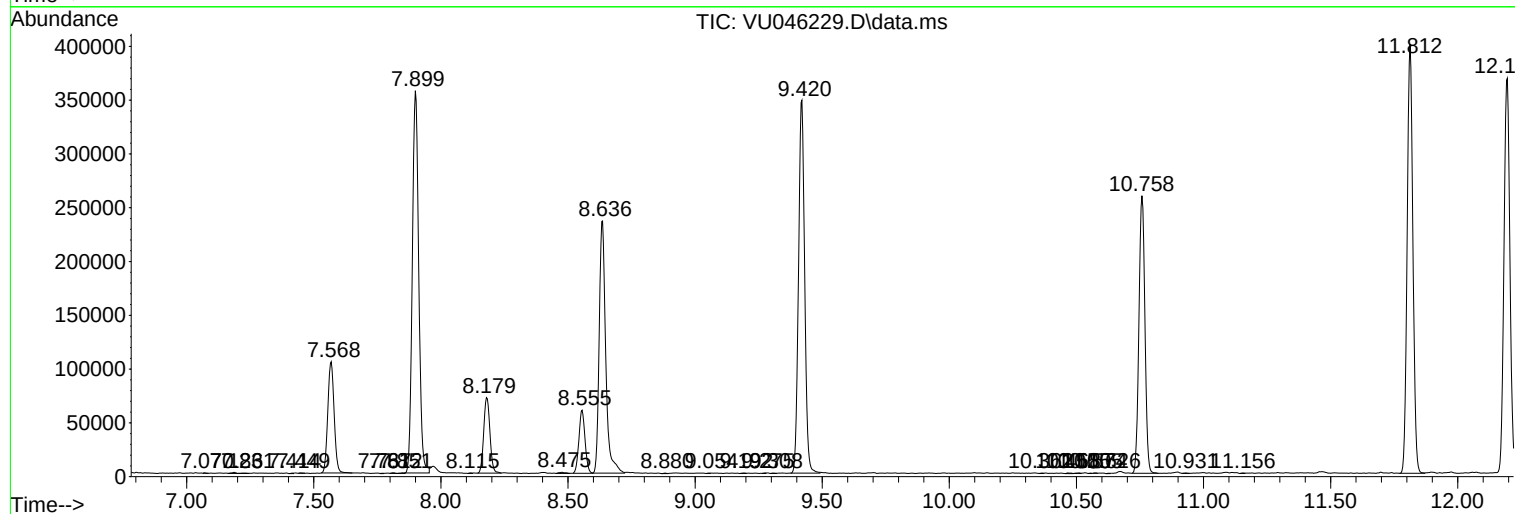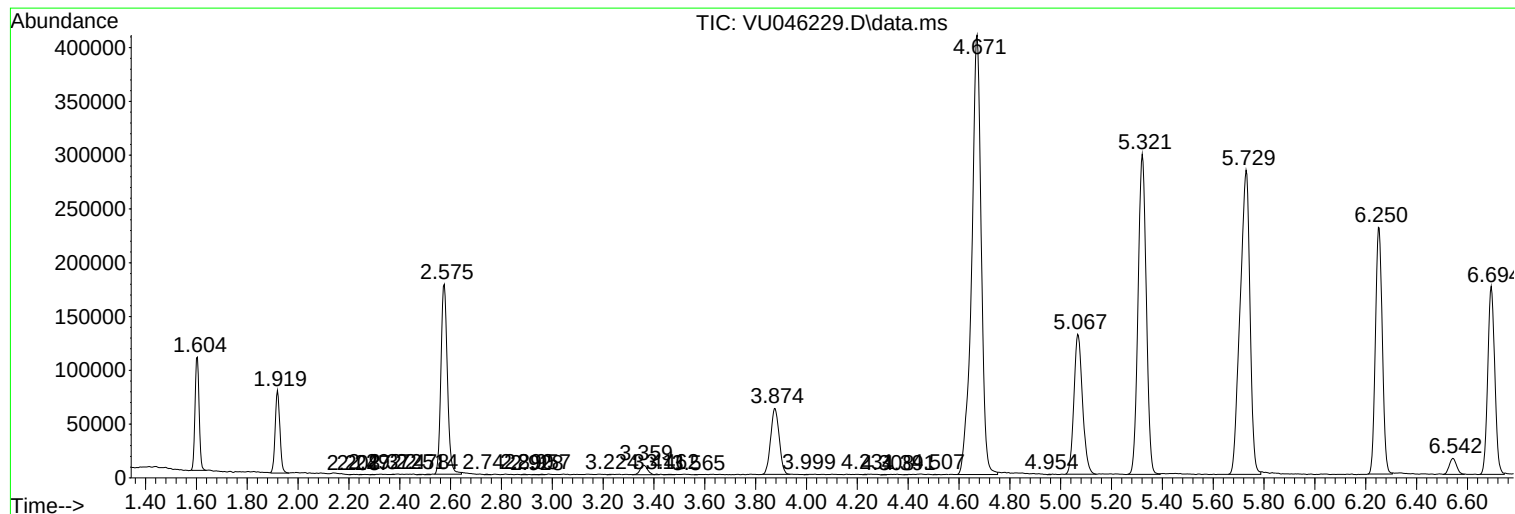

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046229.D
Acq On : 09 Dec 2021 18:50
Operator : SY/MD
Sample : M4983-17
Misc : 5.4mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046229.D
Acq On : 09 Dec 2021 18:50
Operator : SY/MD
Sample : M4983-17
Misc : 5.4mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW5P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc