

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046238.D
 Acq On : 09 Dec 2021 22:26
 Operator : SY/MD
 Sample : M5002-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046238.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	92	rVB	97497	107887	15.51%	1.925%
2	1.919	172	180	192	rVB	71362	90378	12.99%	1.613%
3	2.221	272	274	278	rVB	229	149	0.02%	0.003%
4	2.244	278	281	282	rBV	293	149	0.02%	0.003%
5	2.276	287	291	294	rBV	369	276	0.04%	0.005%
6	2.363	314	318	323	rBV2	517	489	0.07%	0.009%
7	2.421	333	336	340	rBV2	290	283	0.04%	0.005%
8	2.575	371	384	405	rBV	148813	252576	36.31%	4.507%
9	2.848	463	469	472	rBV	530	508	0.07%	0.009%
10	2.938	492	497	499	rBV	376	356	0.05%	0.006%
11	3.022	520	523	526	rBV2	293	221	0.03%	0.004%
12	3.273	597	601	604	rBV	272	275	0.04%	0.005%
13	3.456	655	658	660	rBV2	158	109	0.02%	0.002%
14	3.472	660	663	665	rVV	239	135	0.02%	0.002%
15	3.488	665	668	670	rBV2	267	172	0.02%	0.003%
16	3.584	694	698	700	rBV2	474	399	0.06%	0.007%
17	3.710	733	737	742	rBV2	259	321	0.05%	0.006%
18	3.819	768	771	778	rBV2	252	323	0.05%	0.006%
19	3.855	778	782	784	rBV2	305	268	0.04%	0.005%
20	3.945	807	810	814	rVB2	311	231	0.03%	0.004%
21	4.067	843	848	850	rBV2	316	242	0.03%	0.004%
22	4.192	885	887	890	rBV	289	187	0.03%	0.003%
23	4.388	944	948	951	rBV	386	305	0.04%	0.005%
24	4.485	975	978	982	rBV	334	339	0.05%	0.006%
25	4.546	995	997	1001	rVB	521	312	0.04%	0.006%
26	4.562	1001	1002	1004	rBV	212	116	0.02%	0.002%
27	4.578	1004	1007	1009	rVV	453	322	0.05%	0.006%
28	4.639	1012	1026	1065	rVV	60286	182766	26.28%	3.261%
29	4.874	1096	1099	1103	rBV	398	274	0.04%	0.005%
30	4.980	1128	1132	1133	rBV2	273	168	0.02%	0.003%
31	5.067	1140	1159	1179	rBV	121214	277960	39.96%	4.960%
32	5.391	1254	1260	1262	rBV	395	445	0.06%	0.008%
33	5.546	1305	1308	1310	rBV2	236	160	0.02%	0.003%
34	5.597	1319	1324	1330	rBV	466	720	0.10%	0.013%
35	5.649	1335	1340	1343	rVB2	397	331	0.05%	0.006%
36	5.729	1343	1365	1384	rBV2	259125	695564	100.00%	12.411%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046238.D
 Acq On : 09 Dec 2021 22:26
 Operator : SY/MD
 Sample : M5002-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.253	1514	1528	1548	rBV	214908	402326	57.84%	7.179%
38	6.478	1595	1598	1601	rBV	409	262	0.04%	0.005%
39	6.546	1606	1619	1630	rVB5	22502	43845	6.30%	0.782%
40	6.620	1637	1642	1645	rVB2	281	265	0.04%	0.005%
41	6.642	1645	1649	1651	rBV	333	263	0.04%	0.005%
42	6.694	1651	1665	1681	rBV	158849	305759	43.96%	5.456%
43	6.896	1725	1728	1731	rBV2	462	396	0.06%	0.007%
44	7.086	1784	1787	1790	rBV2	214	133	0.02%	0.002%
45	7.105	1790	1793	1796	rBV2	287	203	0.03%	0.004%
46	7.176	1808	1815	1819	rBV3	596	874	0.13%	0.016%
47	7.250	1834	1838	1841	rBV	325	226	0.03%	0.004%
48	7.305	1850	1855	1857	rBV	427	362	0.05%	0.006%
49	7.388	1879	1881	1888	rBB2	254	258	0.04%	0.005%
50	7.420	1888	1891	1893	rVB2	254	134	0.02%	0.002%
51	7.440	1893	1897	1900	rBV	358	294	0.04%	0.005%
52	7.568	1925	1937	1950	rBV	91598	158007	22.72%	2.819%
53	7.787	2002	2005	2007	rBV	388	282	0.04%	0.005%
54	7.842	2019	2022	2027	rBV	204	143	0.02%	0.003%
55	7.899	2027	2040	2057	rBV	318897	557181	80.10%	9.942%
56	8.179	2116	2127	2145	rBV	62746	105044	15.10%	1.874%
57	8.452	2207	2212	2213	rBV	686	501	0.07%	0.009%
58	8.591	2252	2255	2256	rBV	349	197	0.03%	0.004%
59	8.636	2256	2269	2294	rVV	208777	370816	53.31%	6.617%
60	9.137	2421	2425	2427	rBV	390	289	0.04%	0.005%
61	9.308	2475	2478	2482	rVB2	371	295	0.04%	0.005%
62	9.337	2482	2487	2489	rBV2	332	271	0.04%	0.005%
63	9.420	2499	2513	2533	rBV	324536	538908	77.48%	9.616%
64	9.575	2555	2561	2564	rBV2	621	603	0.09%	0.011%
65	9.780	2620	2625	2630	rBV	492	554	0.08%	0.010%
66	9.813	2630	2635	2639	rBV2	317	345	0.05%	0.006%
67	9.877	2651	2655	2662	rBV	544	741	0.11%	0.013%
68	9.986	2684	2689	2692	rBV2	391	352	0.05%	0.006%
69	10.005	2692	2695	2698	rBV	253	150	0.02%	0.003%
70	10.343	2796	2800	2802	rBV	277	219	0.03%	0.004%
71	10.414	2819	2822	2825	rBV	366	229	0.03%	0.004%
72	10.436	2825	2829	2831	rBV	235	190	0.03%	0.003%
73	10.620	2879	2886	2889	rBV2	587	642	0.09%	0.011%
74	10.668	2898	2901	2908	rVB3	1104	1061	0.15%	0.019%
75	10.758	2916	2929	2947	rVB	237817	381479	54.84%	6.807%
76	10.825	2947	2950	2955	rBV2	265	237	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046238.D
 Acq On : 09 Dec 2021 22:26
 Operator : SY/MD
 Sample : M5002-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	10.951	2985	2989	2991	rBV	351	274	0.04%	0.005%
78	11.041	3014	3017	3019	rVB	223	120	0.02%	0.002%
79	11.057	3019	3022	3024	rBV	376	239	0.03%	0.004%
80	11.140	3045	3048	3050	rBV2	219	117	0.02%	0.002%
81	11.169	3054	3057	3060	rVV	447	257	0.04%	0.005%
82	11.292	3093	3095	3097	rBV	287	173	0.02%	0.003%
83	11.346	3109	3112	3113	rBV	337	196	0.03%	0.003%
84	11.430	3135	3138	3141	rBV	384	287	0.04%	0.005%
85	11.575	3179	3183	3185	rBV	292	246	0.04%	0.004%
86	11.636	3198	3202	3203	rBV	303	218	0.03%	0.004%
87	11.812	3244	3257	3276	rVB	366462	569629	81.89%	10.164%
88	11.973	3304	3307	3311	rVB2	764	507	0.07%	0.009%
89	12.192	3363	3375	3395	rVB	334004	538483	77.42%	9.608%
90	12.356	3423	3426	3429	rBV	383	232	0.03%	0.004%
91	12.648	3514	3517	3518	rBV	298	180	0.03%	0.003%
92	12.906	3594	3597	3600	rBV	470	390	0.06%	0.007%
93	12.964	3612	3615	3617	rBV	274	176	0.03%	0.003%
94	13.269	3706	3710	3715	rBV2	411	522	0.08%	0.009%
95	13.304	3719	3721	3727	rVB	353	313	0.04%	0.006%
96	13.626	3818	3821	3825	rBV	345	263	0.04%	0.005%
97	13.716	3846	3849	3851	rBV2	217	129	0.02%	0.002%
98	14.915	4219	4222	4226	rBV2	370	370	0.05%	0.007%
99	15.034	4254	4259	4265	rBV2	453	608	0.09%	0.011%
100	15.561	4420	4423	4425	rBV2	413	288	0.04%	0.005%




Sum of corrected areas: 5604269

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046238.D
Acq On : 09 Dec 2021 22:26
Operator : SY/MD
Sample : M5002-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

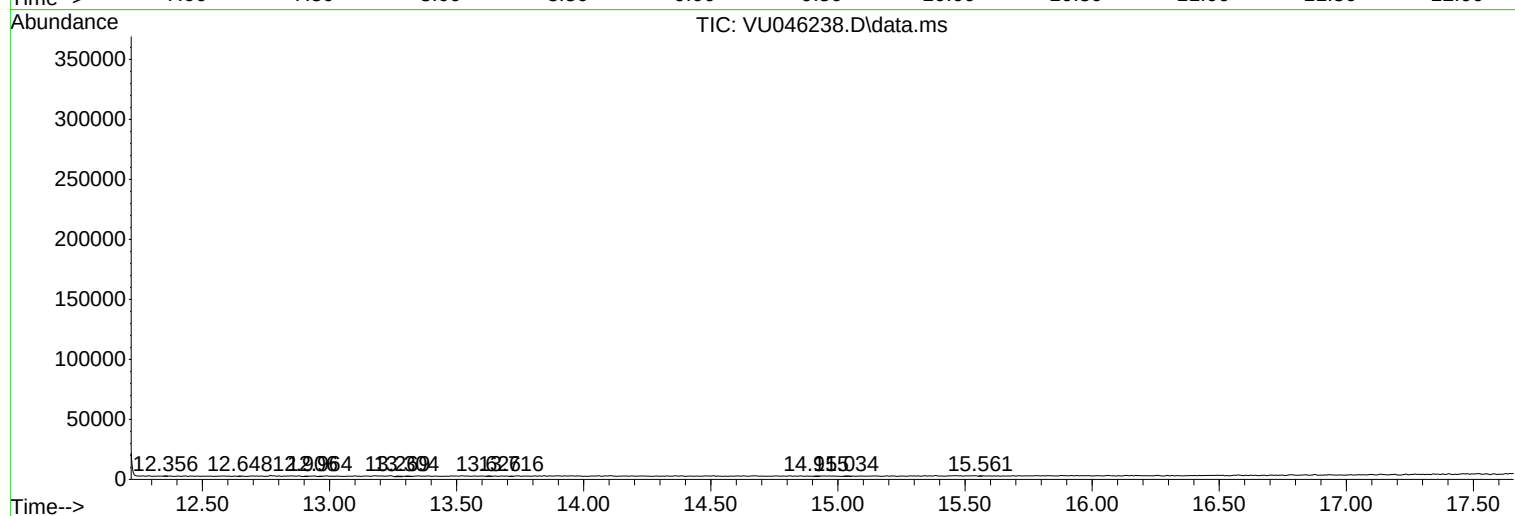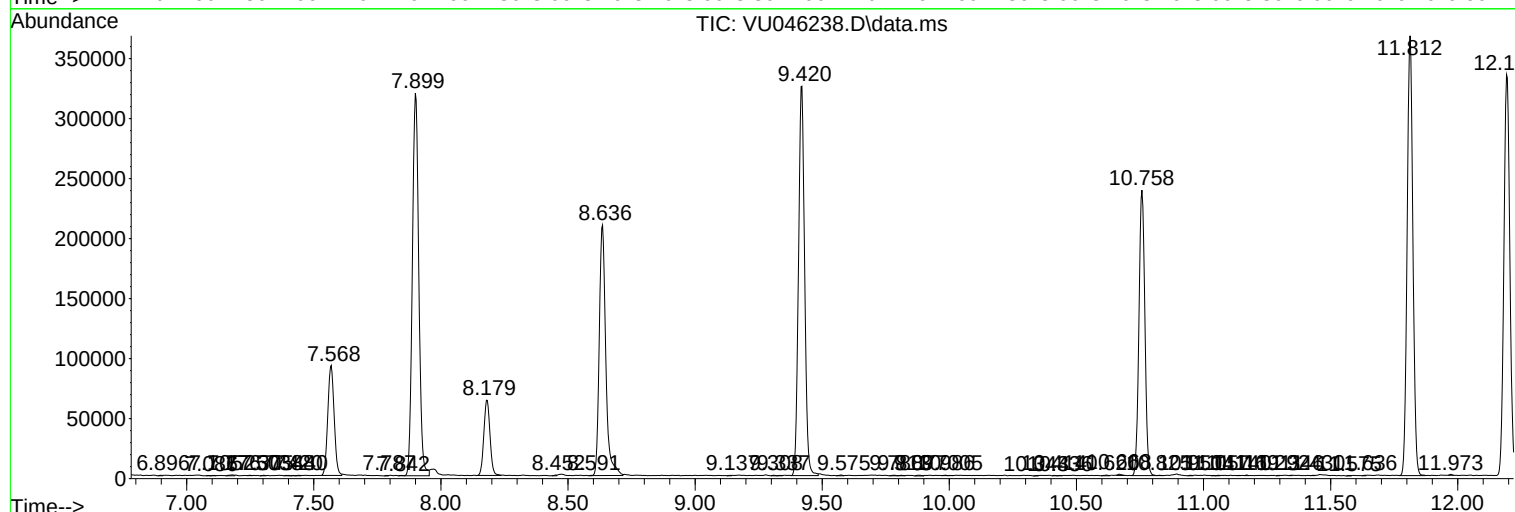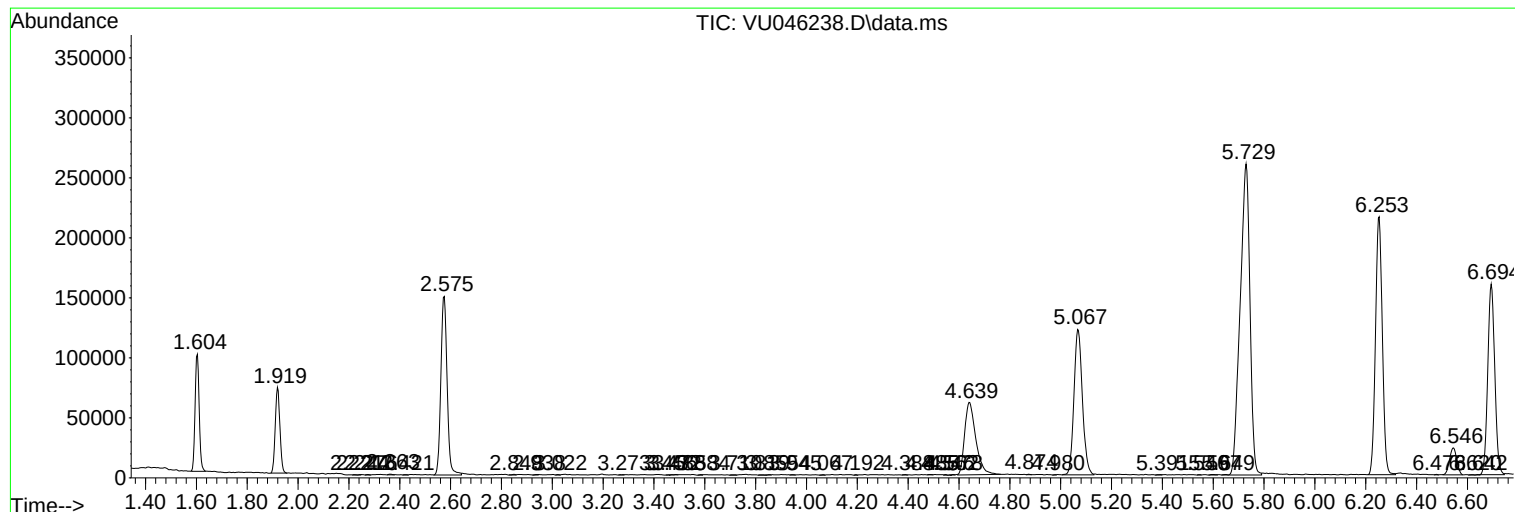

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046238.D
Acq On : 09 Dec 2021 22:26
Operator : SY/MD
Sample : M5002-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046238.D
Acq On : 09 Dec 2021 22:26
Operator : SY/MD
Sample : M5002-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc