

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046240.D
 Acq On : 09 Dec 2021 23:10
 Operator : SY/MD
 Sample : M5002-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	96699	108584	15.58%	1.818%
2	1.919	172	180	191	rBV	71224	89756	12.88%	1.503%
3	2.272	287	290	296	rVB	752	584	0.08%	0.010%
4	2.343	309	312	316	rBV2	417	305	0.04%	0.005%
5	2.379	317	323	327	rVV4	261	366	0.05%	0.006%
6	2.526	362	369	371	rBV2	326	387	0.06%	0.006%
7	2.575	371	384	404	rBV2	155140	264704	37.98%	4.432%
8	2.771	438	445	453	rBV3	458	613	0.09%	0.010%
9	3.044	528	530	537	rVB3	367	456	0.07%	0.008%
10	3.105	546	549	555	rVB2	286	349	0.05%	0.006%
11	3.186	572	574	580	rVV3	382	346	0.05%	0.006%
12	3.333	614	620	623	rBV2	363	365	0.05%	0.006%
13	3.739	743	746	751	rBV2	362	328	0.05%	0.005%
14	3.784	755	760	765	rBV2	356	447	0.06%	0.007%
15	3.864	782	785	788	rBV	425	315	0.05%	0.005%
16	3.922	800	803	809	rVB	364	340	0.05%	0.006%
17	4.134	865	869	873	rBV	412	391	0.06%	0.007%
18	4.411	949	955	958	rVV2	306	333	0.05%	0.006%
19	4.452	964	968	974	rVB	358	416	0.06%	0.007%
20	4.481	974	977	980	rBV	505	410	0.06%	0.007%
21	4.642	1012	1027	1059	rBV	61231	199983	28.69%	3.348%
22	4.909	1107	1110	1116	rVB2	429	365	0.05%	0.006%
23	5.067	1140	1159	1182	rBV	120480	279515	40.10%	4.680%
24	5.221	1203	1207	1214	rVB2	457	419	0.06%	0.007%
25	5.266	1218	1221	1225	rBV2	436	370	0.05%	0.006%
26	5.317	1226	1237	1249	rBV3	3408	7355	1.06%	0.123%
27	5.362	1249	1251	1260	rVB	402	475	0.07%	0.008%
28	5.404	1260	1264	1266	rBV	392	309	0.04%	0.005%
29	5.729	1344	1365	1383	rBV3	258874	697013	100.00%	11.671%
30	5.986	1441	1445	1448	rBV2	402	393	0.06%	0.007%
31	6.092	1471	1478	1481	rBV2	385	508	0.07%	0.009%
32	6.253	1513	1528	1545	rBV	220499	409265	58.72%	6.853%
33	6.546	1605	1619	1634	rBV	178806	337584	48.43%	5.652%
34	6.693	1652	1665	1681	rBV	158503	302902	43.46%	5.072%
35	6.809	1698	1701	1705	rVB4	380	366	0.05%	0.006%
36	6.874	1717	1721	1727	rBV2	384	416	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046240.D
 Acq On : 09 Dec 2021 23:10
 Operator : SY/MD
 Sample : M5002-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.919	1732	1735	1741	rBV	266	298	0.04%	0.005%
38	6.976	1750	1753	1757	rVB	396	347	0.05%	0.006%
39	7.111	1788	1795	1798	rVB	299	344	0.05%	0.006%
40	7.189	1816	1819	1829	rVB3	510	581	0.08%	0.010%
41	7.311	1851	1857	1859	rBV	270	316	0.05%	0.005%
42	7.365	1868	1874	1878	rBV	464	564	0.08%	0.009%
43	7.398	1881	1884	1889	rVB2	467	471	0.07%	0.008%
44	7.436	1889	1896	1898	rBV	448	590	0.08%	0.010%
45	7.568	1924	1937	1952	rVV	93729	159364	22.86%	2.668%
46	7.790	2002	2006	2012	rVB2	603	611	0.09%	0.010%
47	7.899	2023	2040	2057	rBV	318394	552735	79.30%	9.255%
48	8.073	2092	2094	2099	rVB2	549	353	0.05%	0.006%
49	8.179	2114	2127	2144	rBV2	62449	104348	14.97%	1.747%
50	8.282	2156	2159	2163	rBV2	444	343	0.05%	0.006%
51	8.475	2213	2219	2224	rVB2	914	1096	0.16%	0.018%
52	8.636	2254	2269	2294	rBV	207973	370023	53.09%	6.196%
53	8.890	2342	2348	2351	rBV2	281	312	0.04%	0.005%
54	8.909	2351	2354	2359	rVB	347	304	0.04%	0.005%
55	8.935	2359	2362	2365	rBV	595	455	0.07%	0.008%
56	9.018	2385	2388	2391	rVB	468	288	0.04%	0.005%
57	9.108	2413	2416	2423	rVB2	351	394	0.06%	0.007%
58	9.166	2428	2434	2442	rBV	655	1131	0.16%	0.019%
59	9.333	2481	2486	2489	rBV	392	399	0.06%	0.007%
60	9.420	2500	2513	2534	rBV	325749	546488	78.40%	9.150%
61	9.513	2539	2542	2548	rVB3	629	512	0.07%	0.009%
62	9.697	2593	2599	2604	rVB3	617	675	0.10%	0.011%
63	9.726	2604	2608	2611	rBV	429	290	0.04%	0.005%
64	9.861	2646	2650	2653	rBV	321	309	0.04%	0.005%
65	10.028	2698	2702	2707	rBV	460	424	0.06%	0.007%
66	10.057	2707	2711	2715	rBV2	435	337	0.05%	0.006%
67	10.137	2729	2736	2739	rBV2	355	430	0.06%	0.007%
68	10.314	2785	2791	2794	rBV	285	344	0.05%	0.006%
69	10.645	2887	2894	2897	rBV2	379	464	0.07%	0.008%
70	10.671	2898	2902	2912	rVB4	971	1213	0.17%	0.020%
71	10.758	2916	2929	2951	rVB	245215	384888	55.22%	6.444%
72	10.883	2963	2968	2970	rBV2	806	725	0.10%	0.012%
73	11.111	3036	3039	3043	rVB2	444	355	0.05%	0.006%
74	11.311	3096	3101	3104	rBV2	469	457	0.07%	0.008%
75	11.558	3174	3178	3182	rBV2	416	422	0.06%	0.007%
76	11.635	3199	3202	3206	rVB	352	287	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046240.D
 Acq On : 09 Dec 2021 23:10
 Operator : SY/MD
 Sample : M5002-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.745	3232	3236	3238	rBV	429	374	0.05%	0.006%
78	11.812	3244	3257	3277	rVB	374122	579941	83.20%	9.710%
79	11.947	3294	3299	3303	rBV2	897	1005	0.14%	0.017%
80	12.028	3321	3324	3330	rVB2	429	382	0.05%	0.006%
81	12.066	3330	3336	3340	rBV2	473	600	0.09%	0.010%
82	12.195	3362	3376	3393	rBV	341878	541836	77.74%	9.072%
83	12.391	3433	3437	3440	rBV	433	297	0.04%	0.005%
84	12.500	3466	3471	3472	rBV	362	289	0.04%	0.005%
85	12.770	3551	3555	3560	rVB2	450	533	0.08%	0.009%
86	13.311	3719	3723	3726	rVB2	487	399	0.06%	0.007%
87	13.330	3726	3729	3733	rBV2	460	444	0.06%	0.007%
88	13.407	3746	3753	3756	rBV2	310	447	0.06%	0.007%
89	13.529	3787	3791	3795	rBV	422	406	0.06%	0.007%
90	13.745	3855	3858	3861	rBV	395	288	0.04%	0.005%
91	14.458	4077	4080	4084	rVB2	366	316	0.05%	0.005%
92	14.516	4095	4098	4104	rBV2	423	459	0.07%	0.008%
93	14.809	4186	4189	4194	rBV2	471	324	0.05%	0.005%
94	15.240	4320	4323	4328	rVB2	349	333	0.05%	0.006%
95	15.368	4360	4363	4365	rBV2	372	294	0.04%	0.005%
96	15.503	4398	4405	4408	rBV3	413	532	0.08%	0.009%
97	15.523	4408	4411	4414	rBV3	370	362	0.05%	0.006%
98	15.671	4454	4457	4462	rBV3	462	440	0.06%	0.007%
99	16.047	4571	4574	4576	rBV2	483	342	0.05%	0.006%
100	16.220	4624	4628	4630	rBV2	496	440	0.06%	0.007%




Sum of corrected areas: 5972403

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046240.D
Acq On : 09 Dec 2021 23:10
Operator : SY/MD
Sample : M5002-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

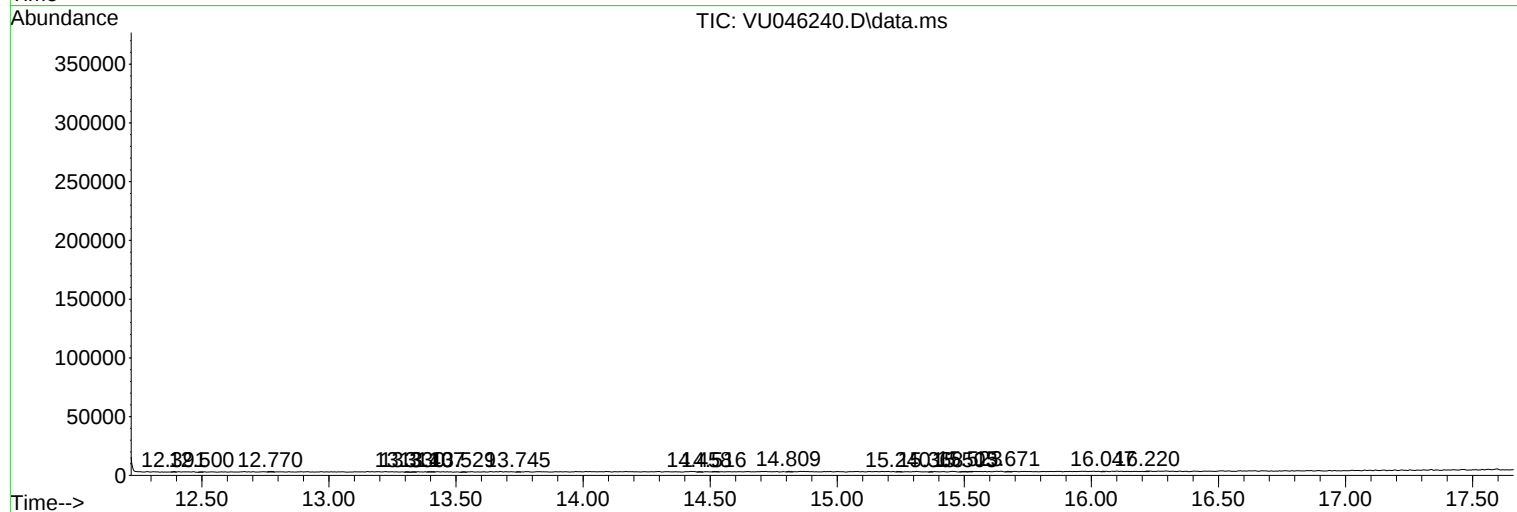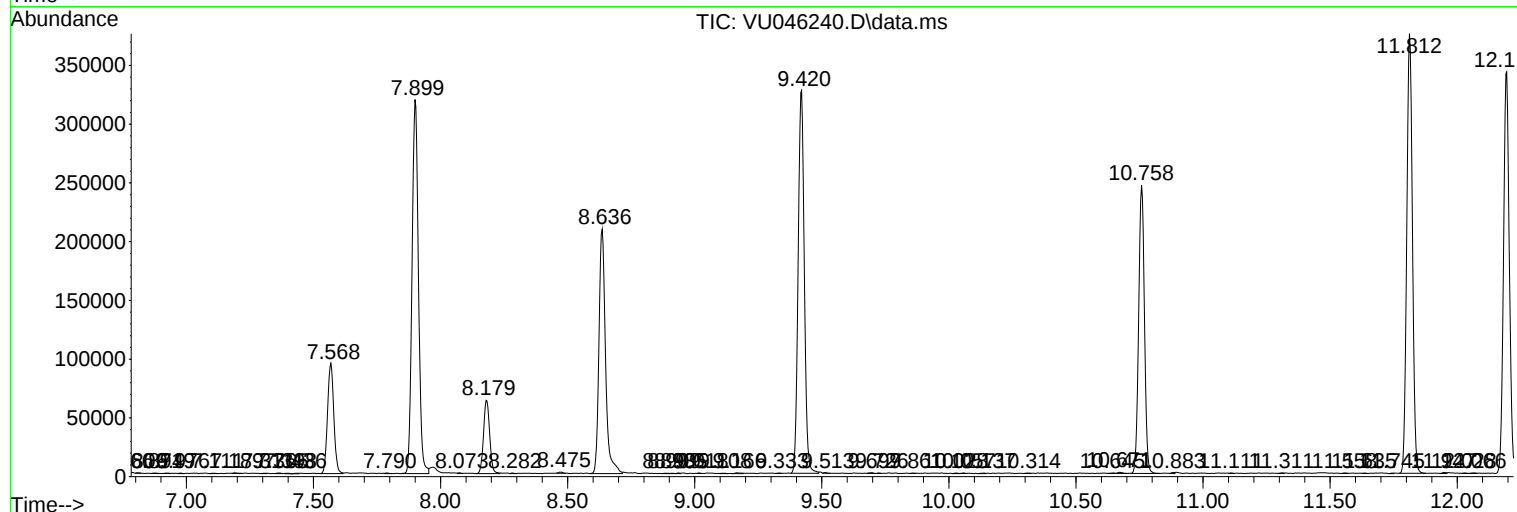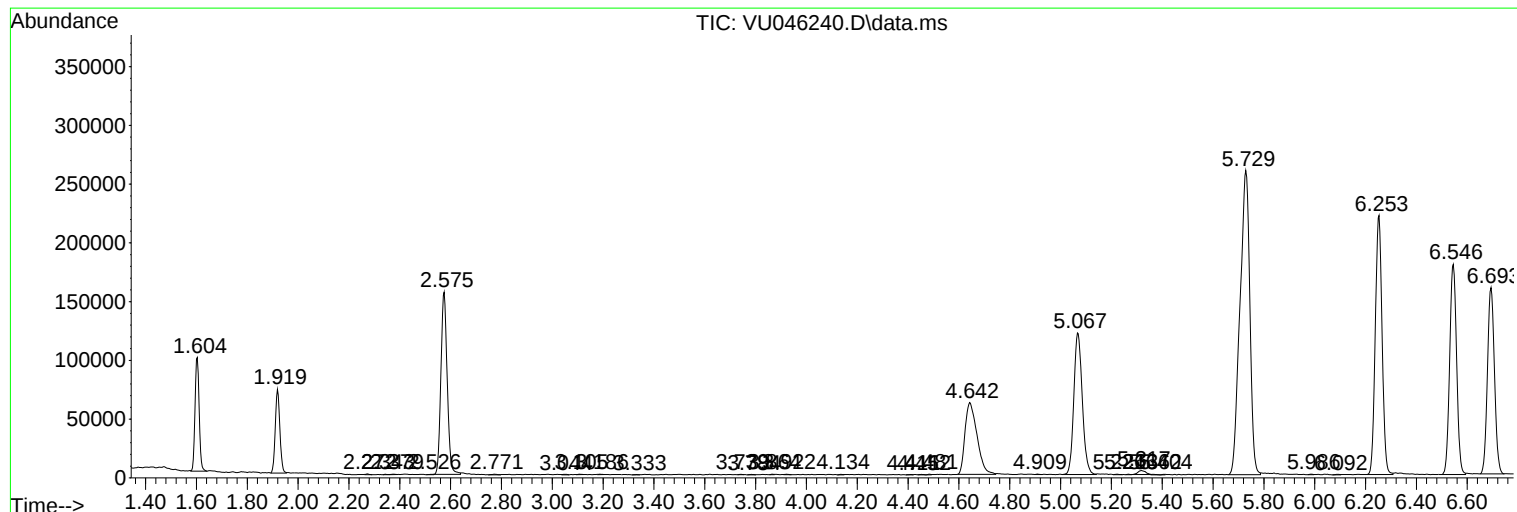

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046240.D
Acq On : 09 Dec 2021 23:10
Operator : SY/MD
Sample : M5002-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046240.D
Acq On : 09 Dec 2021 23:10
Operator : SY/MD
Sample : M5002-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc