

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046241.D
 Acq On : 09 Dec 2021 23:33
 Operator : SY/MD
 Sample : M5002-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	97	rVB	97945	109392	15.47%	1.939%
2	1.919	172	180	192	rVB	72118	91176	12.90%	1.616%
3	2.215	270	272	276	rBV2	225	213	0.03%	0.004%
4	2.260	283	286	288	rBV	244	173	0.02%	0.003%
5	2.334	307	309	312	rBV2	309	174	0.02%	0.003%
6	2.572	372	383	411	rBV	151267	254280	35.96%	4.508%
7	2.784	446	449	457	rVB2	474	573	0.08%	0.010%
8	2.819	457	460	462	rBV	194	145	0.02%	0.003%
9	3.083	539	542	544	rBV	159	91	0.01%	0.002%
10	3.099	544	547	548	rBV	256	149	0.02%	0.003%
11	3.176	566	571	572	rBV	366	281	0.04%	0.005%
12	3.343	621	623	625	rVB	274	113	0.02%	0.002%
13	3.459	655	659	662	rBV	314	289	0.04%	0.005%
14	3.642	713	716	719	rVB	502	347	0.05%	0.006%
15	3.662	719	722	724	rBV	258	152	0.02%	0.003%
16	3.681	724	728	730	rBV2	315	252	0.04%	0.004%
17	3.726	739	742	744	rBV	247	162	0.02%	0.003%
18	3.755	748	751	754	rVB	238	139	0.02%	0.002%
19	3.819	768	771	775	rVB	398	298	0.04%	0.005%
20	3.842	775	778	780	rBV	295	154	0.02%	0.003%
21	3.893	791	794	798	rBV	281	231	0.03%	0.004%
22	4.054	841	844	851	rBV	348	344	0.05%	0.006%
23	4.215	892	894	897	rVB	388	223	0.03%	0.004%
24	4.498	979	982	987	rBV2	386	342	0.05%	0.006%
25	4.639	1010	1026	1062	rBV	65080	186690	26.40%	3.310%
26	5.067	1143	1159	1182	rBV	123964	286472	40.52%	5.079%
27	5.282	1223	1226	1227	rBV2	368	187	0.03%	0.003%
28	5.337	1240	1243	1244	rBV2	113	57	0.01%	0.001%
29	5.385	1256	1258	1260	rBV	269	133	0.02%	0.002%
30	5.462	1278	1282	1287	rBV2	326	385	0.05%	0.007%
31	5.729	1343	1365	1383	rBV2	262437	707042	100.00%	12.535%
32	5.960	1434	1437	1439	rBV2	284	165	0.02%	0.003%
33	6.038	1457	1461	1464	rBV	503	467	0.07%	0.008%
34	6.250	1514	1527	1544	rBV	216501	406061	57.43%	7.199%
35	6.497	1602	1604	1605	rBV	265	114	0.02%	0.002%
36	6.533	1605	1615	1628	rVV8	4307	9258	1.31%	0.164%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046241.D
 Acq On : 09 Dec 2021 23:33
 Operator : SY/MD
 Sample : M5002-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.694	1651	1665	1682	rBV	165769	314987	44.55%	5.584%
38	6.880	1721	1723	1726	rBV2	287	163	0.02%	0.003%
39	7.279	1845	1847	1850	rBV	222	130	0.02%	0.002%
40	7.298	1850	1853	1855	rBV2	297	195	0.03%	0.003%
41	7.452	1894	1901	1903	rBV2	412	489	0.07%	0.009%
42	7.568	1923	1937	1956	rBV	93287	161091	22.78%	2.856%
43	7.899	2026	2040	2057	rBV	326106	569362	80.53%	10.094%
44	8.092	2097	2100	2102	rBV	177	114	0.02%	0.002%
45	8.179	2116	2127	2147	rBV	63997	107909	15.26%	1.913%
46	8.398	2192	2195	2198	rBV	339	255	0.04%	0.005%
47	8.546	2239	2241	2244	rBV	127	81	0.01%	0.001%
48	8.636	2256	2269	2297	rBV	213300	376583	53.26%	6.676%
49	8.915	2353	2356	2359	rBV	383	303	0.04%	0.005%
50	8.986	2375	2378	2384	rBV2	375	245	0.03%	0.004%
51	9.288	2469	2472	2474	rBV	256	138	0.02%	0.002%
52	9.417	2500	2512	2533	rBV	325463	541570	76.60%	9.601%
53	9.819	2634	2637	2642	rBV	420	430	0.06%	0.008%
54	10.002	2691	2694	2695	rBV	239	153	0.02%	0.003%
55	10.025	2698	2701	2708	rVV2	393	435	0.06%	0.008%
56	10.163	2741	2744	2746	rBV2	545	342	0.05%	0.006%
57	10.607	2878	2882	2888	rBV	407	522	0.07%	0.009%
58	10.758	2917	2929	2944	rBV	245329	387891	54.86%	6.877%
59	11.372	3117	3120	3121	rBV2	298	170	0.02%	0.003%
60	11.526	3165	3168	3171	rBV	357	247	0.03%	0.004%
61	11.726	3228	3230	3232	rBV	305	184	0.03%	0.003%
62	11.812	3245	3257	3280	rVB	364683	571547	80.84%	10.133%
63	12.195	3363	3376	3390	rBV	335506	546842	77.34%	9.695%
64	13.134	3665	3668	3671	rBV2	457	321	0.05%	0.006%
65	13.549	3793	3797	3803	rBV	669	798	0.11%	0.014%
66	14.214	3999	4004	4005	rBV	505	418	0.06%	0.007%




Sum of corrected areas: 5640639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046241.D
Acq On : 09 Dec 2021 23:33
Operator : SY/MD
Sample : M5002-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

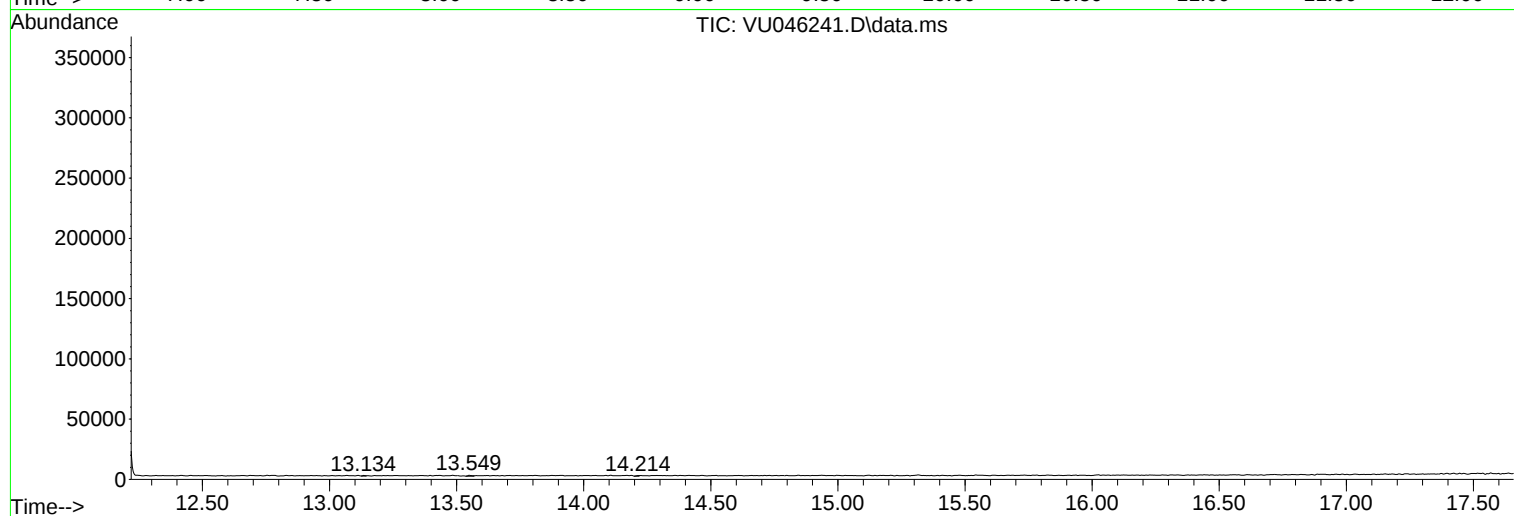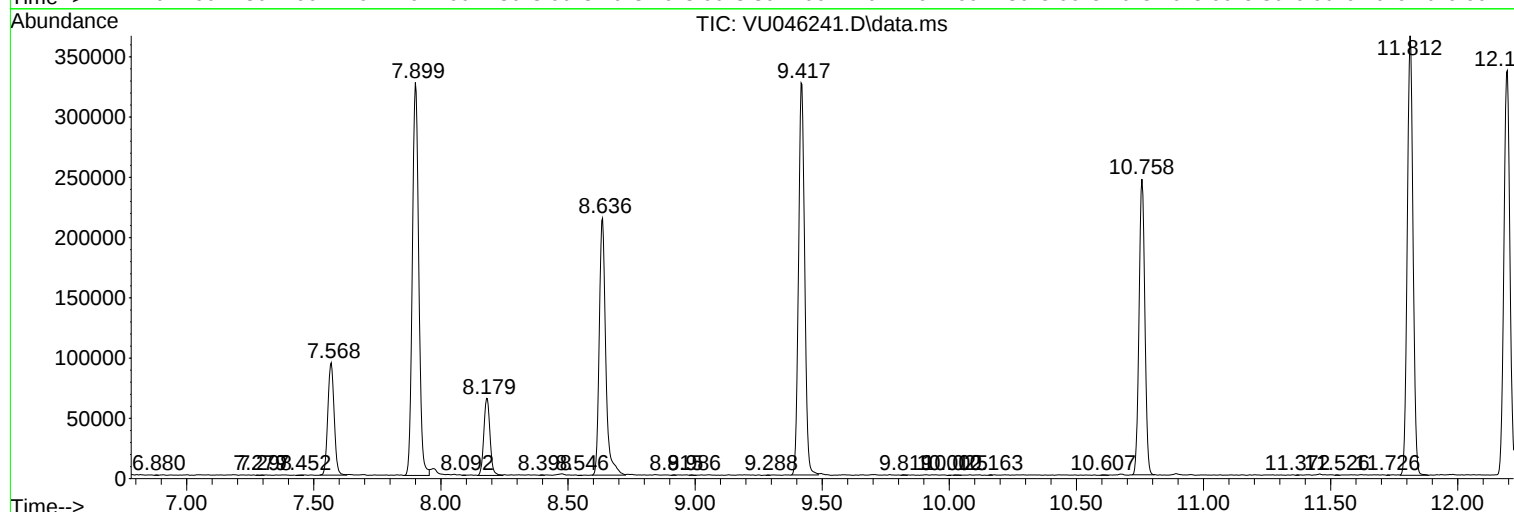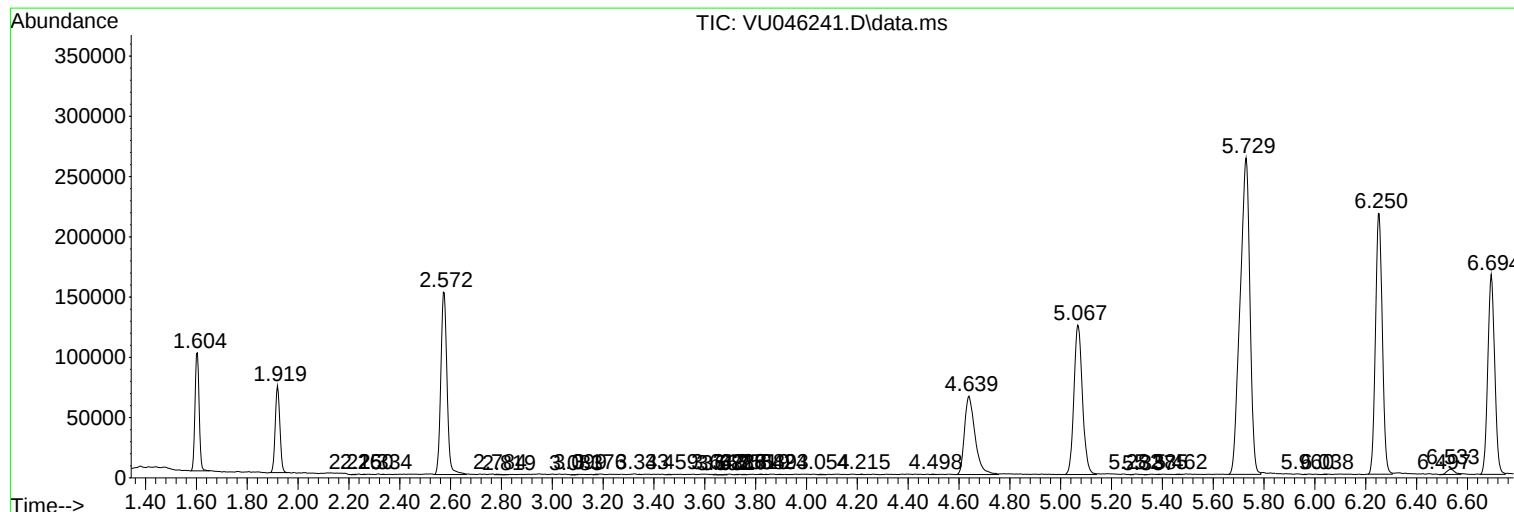

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046241.D
Acq On : 09 Dec 2021 23:33
Operator : SY/MD
Sample : M5002-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046241.D
Acq On : 09 Dec 2021 23:33
Operator : SY/MD
Sample : M5002-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc