

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046242.D
 Acq On : 09 Dec 2021 23:55
 Operator : SY/MD
 Sample : M5002-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	92	rVB	95588	106482	15.29%	1.935%
2	1.919	172	180	191	rBV	70374	89182	12.80%	1.620%
3	2.327	304	307	309	rBV	408	273	0.04%	0.005%
4	2.353	311	315	317	rVV	299	280	0.04%	0.005%
5	2.424	334	337	342	rBV2	319	315	0.05%	0.006%
6	2.572	372	383	400	rBV	149478	247977	35.60%	4.505%
7	2.742	431	436	437	rBV	344	275	0.04%	0.005%
8	3.047	527	531	532	rVB	228	134	0.02%	0.002%
9	3.057	532	534	539	rBV	219	159	0.02%	0.003%
10	3.086	539	543	546	rBV2	303	311	0.04%	0.006%
11	3.224	584	586	588	rBV2	78	36	0.01%	0.001%
12	3.247	588	593	595	rBV2	192	212	0.03%	0.004%
13	3.385	629	636	640	rBV	344	437	0.06%	0.008%
14	3.404	640	642	644	rBV	185	103	0.01%	0.002%
15	3.523	672	679	683	rVB	625	795	0.11%	0.014%
16	3.549	683	687	689	rBV	246	206	0.03%	0.004%
17	3.684	726	729	733	rVB	223	149	0.02%	0.003%
18	3.793	759	763	770	rBV	516	474	0.07%	0.009%
19	3.829	771	774	779	rBV	235	201	0.03%	0.004%
20	3.941	802	809	811	rBV2	536	585	0.08%	0.011%
21	4.073	847	850	855	rBV	376	375	0.05%	0.007%
22	4.118	861	864	870	rBV	297	317	0.05%	0.006%
23	4.147	870	873	877	rBV2	315	248	0.04%	0.005%
24	4.198	882	889	895	rBV2	404	668	0.10%	0.012%
25	4.362	933	940	942	rBV	258	285	0.04%	0.005%
26	4.475	972	975	978	rBV	301	226	0.03%	0.004%
27	4.639	1010	1026	1050	rBV	61375	177732	25.52%	3.229%
28	4.928	1113	1116	1121	rBV2	297	242	0.03%	0.004%
29	5.067	1142	1159	1184	rBV2	121491	279047	40.07%	5.070%
30	5.153	1184	1186	1189	rBV	281	157	0.02%	0.003%
31	5.198	1198	1200	1202	rBV2	411	228	0.03%	0.004%
32	5.321	1235	1238	1241	rBV	201	167	0.02%	0.003%
33	5.369	1250	1253	1254	rBV	225	137	0.02%	0.002%
34	5.417	1265	1268	1270	rBV2	190	96	0.01%	0.002%
35	5.433	1270	1273	1275	rBV2	250	127	0.02%	0.002%
36	5.459	1279	1281	1282	rBV	119	44	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046242.D
 Acq On : 09 Dec 2021 23:55
 Operator : SY/MD
 Sample : M5002-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.472	1282	1285	1289	rBV	305	246	0.04%	0.004%
38	5.546	1304	1308	1314	rBV2	237	271	0.04%	0.005%
39	5.571	1314	1316	1319	rVB	202	91	0.01%	0.002%
40	5.597	1321	1324	1326	rBV	225	141	0.02%	0.003%
41	5.610	1326	1328	1331	rVB	266	133	0.02%	0.002%
42	5.629	1331	1334	1337	rBV2	256	217	0.03%	0.004%
43	5.729	1344	1365	1387	rBV2	258887	696479	100.00%	12.653%
44	5.996	1445	1448	1449	rBV2	318	165	0.02%	0.003%
45	6.095	1476	1479	1480	rBV2	201	106	0.02%	0.002%
46	6.192	1505	1509	1510	rBV2	319	237	0.03%	0.004%
47	6.253	1514	1528	1544	rVV	208816	392228	56.32%	7.126%
48	6.472	1594	1596	1601	rVB2	529	340	0.05%	0.006%
49	6.694	1651	1665	1684	rBV	158469	307521	44.15%	5.587%
50	6.864	1716	1718	1720	rBV2	274	170	0.02%	0.003%
51	6.996	1754	1759	1766	rBV	497	710	0.10%	0.013%
52	7.028	1766	1769	1772	rBV	401	299	0.04%	0.005%
53	7.163	1806	1811	1814	rBV	636	653	0.09%	0.012%
54	7.211	1824	1826	1828	rBV	365	240	0.03%	0.004%
55	7.333	1859	1864	1866	rBV	285	287	0.04%	0.005%
56	7.375	1875	1877	1881	rBV2	281	183	0.03%	0.003%
57	7.449	1895	1900	1903	rBV	305	259	0.04%	0.005%
58	7.468	1903	1906	1910	rVB	242	179	0.03%	0.003%
59	7.491	1910	1913	1916	rBV	343	292	0.04%	0.005%
60	7.568	1925	1937	1950	rBV	91573	155498	22.33%	2.825%
61	7.751	1991	1994	1998	rBV2	199	210	0.03%	0.004%
62	7.800	2006	2009	2011	rBV	304	168	0.02%	0.003%
63	7.899	2026	2040	2056	rBV	318633	553869	79.52%	10.063%
64	8.115	2103	2107	2108	rBV	305	215	0.03%	0.004%
65	8.179	2115	2127	2144	rBV	62371	104371	14.99%	1.896%
66	8.391	2190	2193	2195	rBV2	274	183	0.03%	0.003%
67	8.439	2205	2208	2210	rBV	278	155	0.02%	0.003%
68	8.468	2210	2217	2218	rBV	876	947	0.14%	0.017%
69	8.581	2246	2252	2255	rBV2	212	214	0.03%	0.004%
70	8.636	2255	2269	2294	rBV	205857	365989	52.55%	6.649%
71	8.832	2327	2330	2332	rBV	211	137	0.02%	0.002%
72	8.899	2348	2351	2352	rBV	228	138	0.02%	0.003%
73	8.938	2360	2363	2365	rBV	355	238	0.03%	0.004%
74	9.282	2467	2470	2472	rBV	315	215	0.03%	0.004%
75	9.420	2500	2513	2538	rBV	316547	527615	75.75%	9.586%
76	9.619	2572	2575	2579	rBV	409	295	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046242.D
 Acq On : 09 Dec 2021 23:55
 Operator : SY/MD
 Sample : M5002-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	9.677	2590	2593	2594	rBV	210	129	0.02%	0.002%
78	9.867	2649	2652	2660	rVB	505	625	0.09%	0.011%
79	9.902	2660	2663	2665	rBV2	272	205	0.03%	0.004%
80	10.632	2886	2890	2896	rBV	491	592	0.08%	0.011%
81	10.661	2896	2899	2900	rBV	787	403	0.06%	0.007%
82	10.758	2917	2929	2947	rBV	238785	381030	54.71%	6.922%
83	11.340	3104	3110	3113	rBV2	298	351	0.05%	0.006%
84	11.369	3116	3119	3123	rBV	404	275	0.04%	0.005%
85	11.394	3123	3127	3129	rBV2	519	457	0.07%	0.008%
86	11.459	3141	3147	3149	rBV2	649	607	0.09%	0.011%
87	11.648	3204	3206	3208	rBV	281	129	0.02%	0.002%
88	11.812	3245	3257	3278	rBV	359046	557507	80.05%	10.129%
89	11.906	3283	3286	3288	rBV2	325	214	0.03%	0.004%
90	11.944	3295	3298	3300	rBV2	534	345	0.05%	0.006%
91	12.195	3364	3376	3395	rBV	334330	538270	77.28%	9.779%
92	12.542	3481	3484	3488	rBV2	333	337	0.05%	0.006%
93	12.655	3516	3519	3522	rBV	311	253	0.04%	0.005%
94	13.031	3631	3636	3639	rBV2	475	535	0.08%	0.010%
95	13.108	3658	3660	3663	rBV	399	208	0.03%	0.004%
96	13.423	3755	3758	3760	rBV2	380	241	0.03%	0.004%
97	14.420	4065	4068	4073	rVB	597	395	0.06%	0.007%
98	14.446	4073	4076	4082	rBV2	523	594	0.09%	0.011%




Sum of corrected areas: 5504288

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046242.D
Acq On : 09 Dec 2021 23:55
Operator : SY/MD
Sample : M5002-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

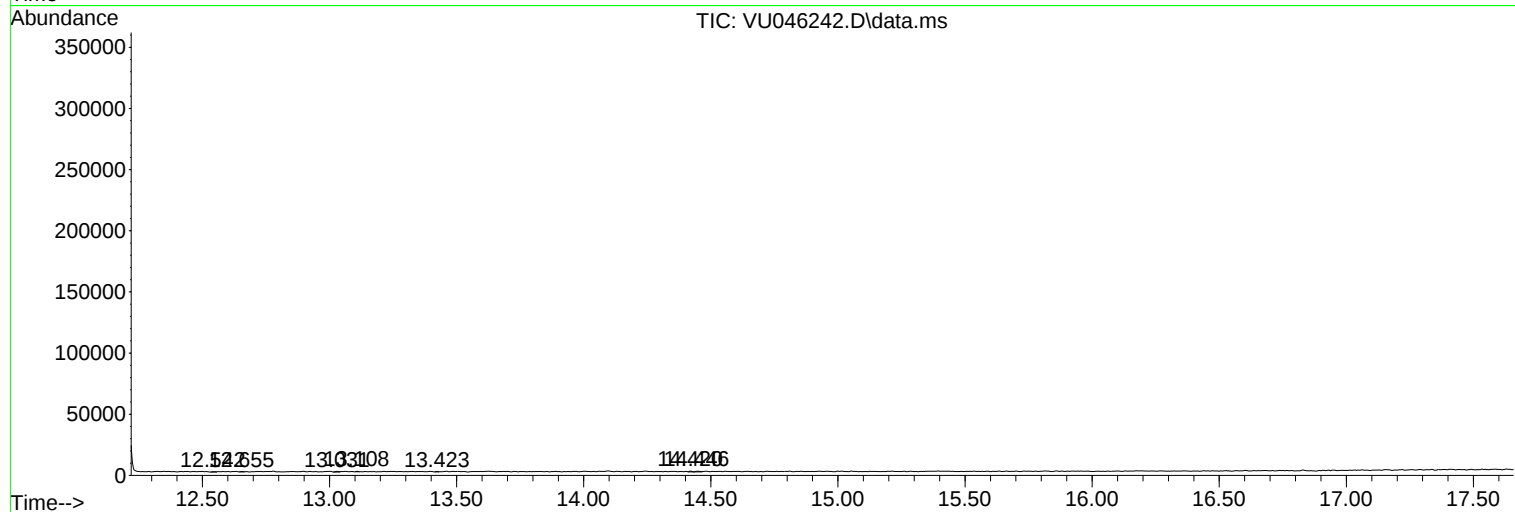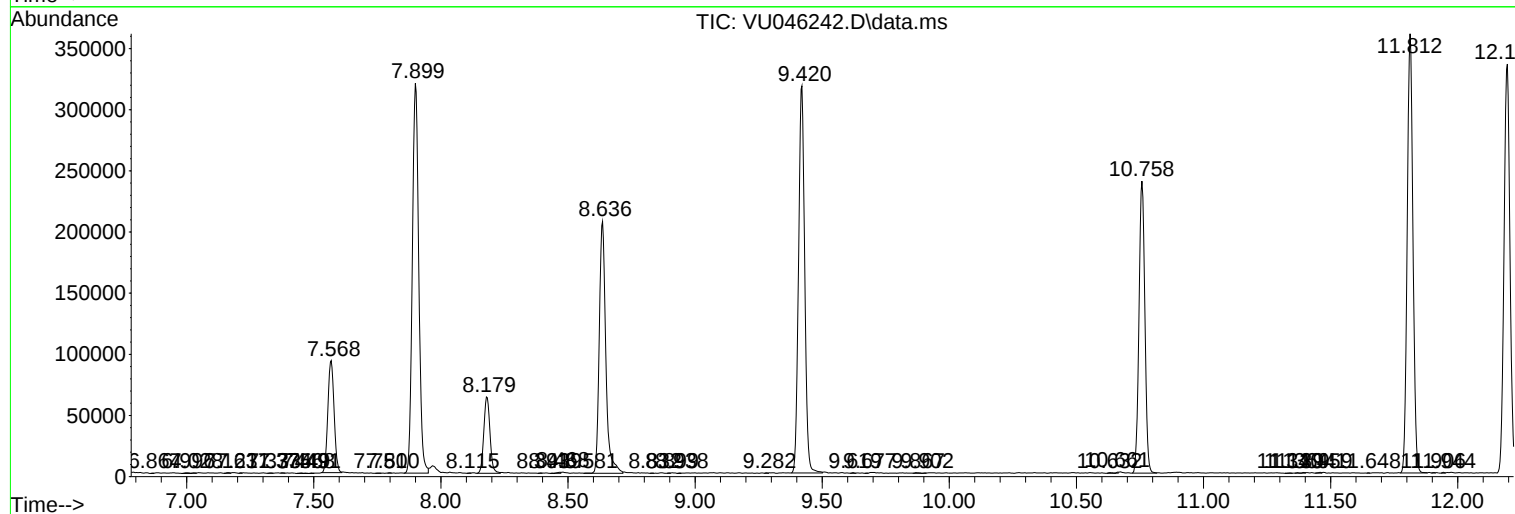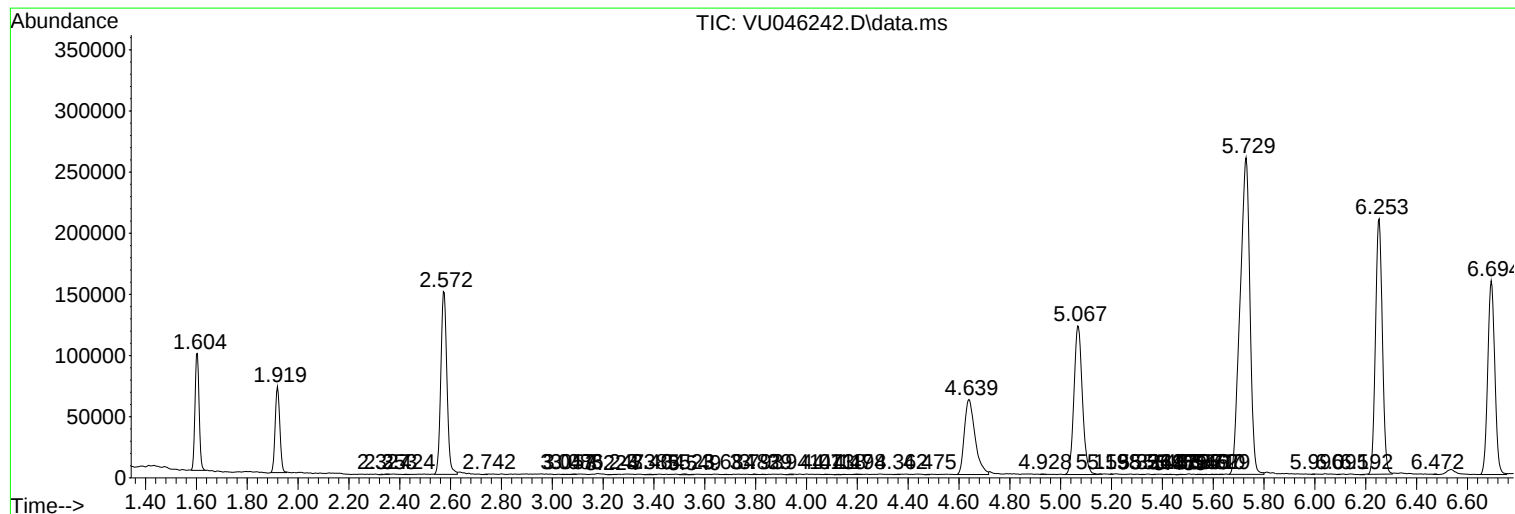

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046242.D
Acq On : 09 Dec 2021 23:55
Operator : SY/MD
Sample : M5002-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046242.D
Acq On : 09 Dec 2021 23:55
Operator : SY/MD
Sample : M5002-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc