

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046243.D
 Acq On : 10 Dec 2021 00:18
 Operator : SY/MD
 Sample : M5002-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	99	rVB	95133	107501	15.71%	1.967%
2	1.919	172	180	191	rVB	70545	88194	12.89%	1.614%
3	2.404	329	331	333	rBV	311	154	0.02%	0.003%
4	2.571	372	383	405	rBV	146867	245512	35.88%	4.492%
5	2.803	448	455	457	rBV	515	559	0.08%	0.010%
6	2.848	466	469	471	rBV	436	301	0.04%	0.006%
7	2.887	478	481	482	rBV	271	168	0.02%	0.003%
8	3.115	549	552	554	rBV	301	206	0.03%	0.004%
9	3.350	622	625	627	rBV	377	234	0.03%	0.004%
10	3.449	654	656	659	rVB2	312	163	0.02%	0.003%
11	3.475	659	664	668	rBV	348	414	0.06%	0.008%
12	3.571	690	694	697	rBV2	262	276	0.04%	0.005%
13	3.639	712	715	718	rBV	354	202	0.03%	0.004%
14	3.739	743	746	750	rVB2	304	202	0.03%	0.004%
15	3.761	750	753	757	rBV	386	318	0.05%	0.006%
16	3.832	772	775	777	rBV	273	181	0.03%	0.003%
17	3.915	797	801	803	rBV	419	350	0.05%	0.006%
18	4.083	850	853	856	rBV	279	220	0.03%	0.004%
19	4.192	885	887	890	rBV2	322	251	0.04%	0.005%
20	4.308	918	923	929	rBV2	441	549	0.08%	0.010%
21	4.382	944	946	948	rBV2	175	81	0.01%	0.001%
22	4.639	1012	1026	1054	rBV	58359	175103	25.59%	3.204%
23	4.970	1126	1129	1132	rBV	280	202	0.03%	0.004%
24	5.067	1143	1159	1183	rBV	121749	277513	40.56%	5.077%
25	5.253	1214	1217	1218	rBV2	323	180	0.03%	0.003%
26	5.472	1282	1285	1287	rBV2	211	160	0.02%	0.003%
27	5.523	1299	1301	1302	rBV	89	41	0.01%	0.001%
28	5.549	1306	1309	1310	rBV	215	134	0.02%	0.002%
29	5.597	1322	1324	1326	rBV	229	145	0.02%	0.003%
30	5.629	1331	1334	1336	rBV	360	208	0.03%	0.004%
31	5.729	1344	1365	1384	rBV2	251881	684216	100.00%	12.518%
32	6.153	1494	1497	1498	rBV	326	197	0.03%	0.004%
33	6.250	1514	1527	1546	rBV	210770	395122	57.75%	7.229%
34	6.491	1599	1602	1603	rBV2	170	95	0.01%	0.002%
35	6.536	1607	1616	1624	rVV3	3018	5867	0.86%	0.107%
36	6.616	1639	1641	1647	rVB	343	232	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046243.D
 Acq On : 10 Dec 2021 00:18
 Operator : SY/MD
 Sample : M5002-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.694	1651	1665	1685	rVV	159043	302706	44.24%	5.538%
38	6.848	1710	1713	1719	rBV	319	267	0.04%	0.005%
39	6.909	1729	1732	1734	rBV	364	203	0.03%	0.004%
40	7.002	1757	1761	1769	rBV	408	523	0.08%	0.010%
41	7.073	1780	1783	1786	rBV	395	275	0.04%	0.005%
42	7.218	1824	1828	1833	rBV	395	511	0.07%	0.009%
43	7.568	1925	1937	1952	rBV	88681	154282	22.55%	2.823%
44	7.777	1996	2002	2005	rBV2	482	576	0.08%	0.011%
45	7.899	2027	2040	2057	rBV	313859	548754	80.20%	10.040%
46	8.121	2105	2109	2111	rBV2	360	279	0.04%	0.005%
47	8.179	2116	2127	2148	rVB	61469	103324	15.10%	1.890%
48	8.446	2198	2210	2213	rBV2	551	1108	0.16%	0.020%
49	8.636	2257	2269	2294	rBV	207255	363878	53.18%	6.657%
50	9.012	2383	2386	2388	rBV	271	153	0.02%	0.003%
51	9.417	2500	2512	2530	rBV	317309	527556	77.10%	9.652%
52	9.591	2563	2566	2569	rBV	265	205	0.03%	0.004%
53	9.812	2632	2635	2638	rBV	457	336	0.05%	0.006%
54	10.008	2692	2696	2699	rBV2	393	344	0.05%	0.006%
55	10.105	2720	2726	2728	rBV	311	349	0.05%	0.006%
56	10.250	2768	2771	2772	rBV	335	179	0.03%	0.003%
57	10.343	2798	2800	2802	rBV2	229	137	0.02%	0.003%
58	10.398	2814	2817	2822	rBV	302	325	0.05%	0.006%
59	10.500	2846	2849	2852	rBV2	406	296	0.04%	0.005%
60	10.706	2910	2913	2915	rBV	288	173	0.03%	0.003%
61	10.758	2917	2929	2946	rVB	238702	379999	55.54%	6.952%
62	10.947	2985	2988	2990	rBV2	275	203	0.03%	0.004%
63	10.986	2996	3000	3004	rBV2	403	404	0.06%	0.007%
64	11.060	3021	3023	3026	rBV	291	192	0.03%	0.004%
65	11.201	3062	3067	3070	rBV2	399	457	0.07%	0.008%
66	11.356	3112	3115	3121	rVB2	451	377	0.06%	0.007%
67	11.452	3140	3145	3148	rBV3	737	814	0.12%	0.015%
68	11.812	3245	3257	3275	rVV	356150	553253	80.86%	10.122%
69	11.893	3279	3282	3285	rBV2	319	245	0.04%	0.004%
70	12.195	3363	3376	3396	rVB	333164	533086	77.91%	9.753%
71	12.629	3508	3511	3514	rBV	301	222	0.03%	0.004%
72	12.864	3578	3584	3586	rBV	276	304	0.04%	0.006%
73	12.954	3609	3612	3616	rBV2	252	181	0.03%	0.003%
74	13.066	3644	3647	3651	rBV2	354	275	0.04%	0.005%
75	13.105	3656	3659	3665	rBV2	234	203	0.03%	0.004%
76	13.169	3676	3679	3684	rVB2	526	348	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046243.D
Acq On : 10 Dec 2021 00:18
Operator : SY/MD
Sample : M5002-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	13.243	3699	3702	3705	rBV	374	334	0.05%	0.006%
78	13.471	3771	3773	3774	rBV	218	104	0.02%	0.002%
79	13.497	3778	3781	3786	rVB	414	285	0.04%	0.005%
80	13.610	3813	3816	3817	rBV	266	148	0.02%	0.003%
81	14.317	4029	4036	4040	rBV	648	1026	0.15%	0.019%
82	15.568	4422	4425	4428	rBV	681	593	0.09%	0.011%
83	15.610	4435	4438	4442	rBV	647	616	0.09%	0.011%




Sum of corrected areas: 5465859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046243.D
Acq On : 10 Dec 2021 00:18
Operator : SY/MD
Sample : M5002-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

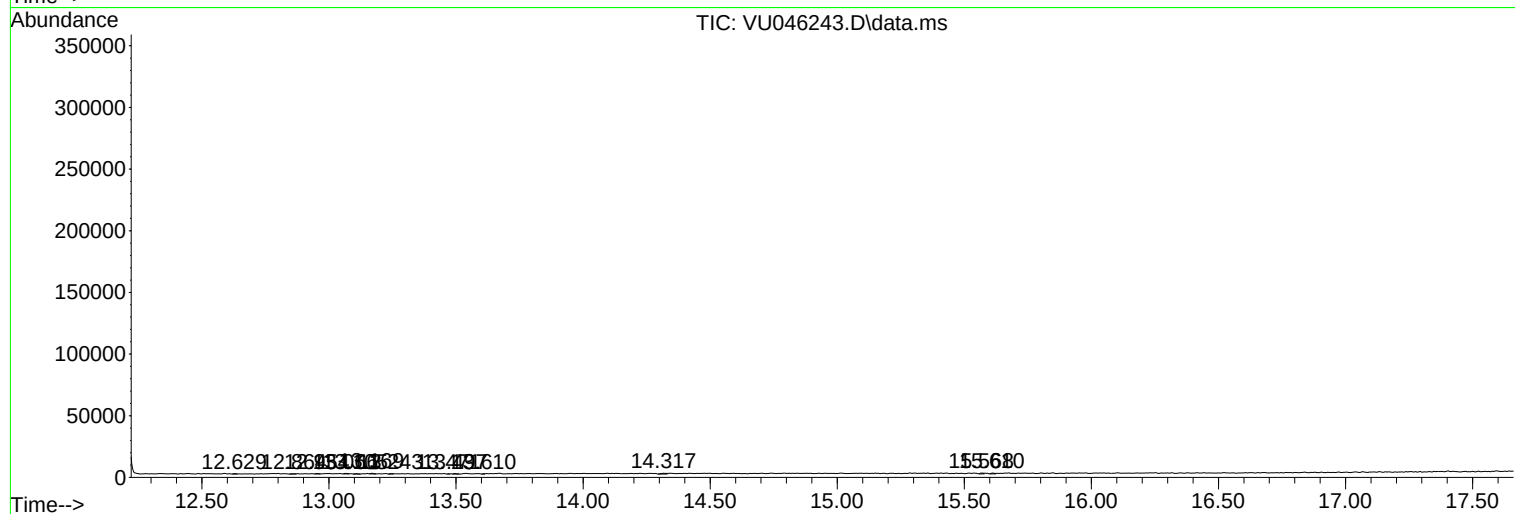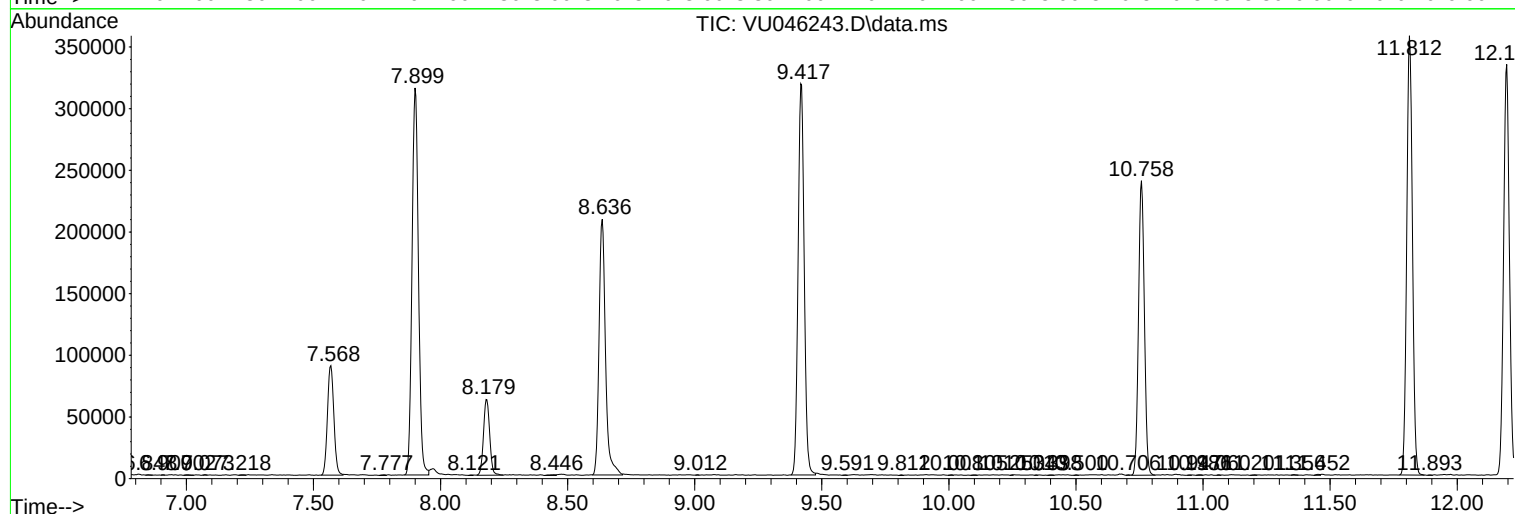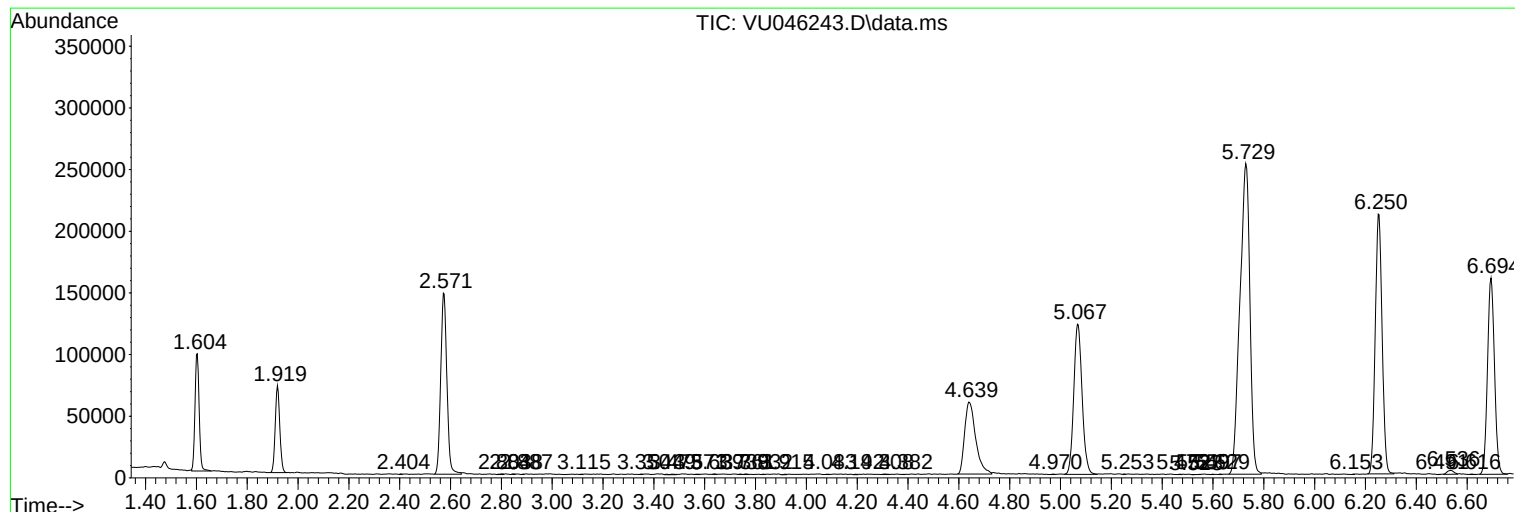

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046243.D
Acq On : 10 Dec 2021 00:18
Operator : SY/MD
Sample : M5002-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046243.D
Acq On : 10 Dec 2021 00:18
Operator : SY/MD
Sample : M5002-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc