

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046246.D
 Acq On : 10 Dec 2021 01:25
 Operator : SY/MD
 Sample : M4982-11
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	99	rVB	93415	106694	15.67%	1.982%
2	1.919	172	180	193	rVB	69733	88572	13.01%	1.645%
3	2.224	273	275	279	rVB	340	160	0.02%	0.003%
4	2.247	279	282	284	rBV	300	153	0.02%	0.003%
5	2.298	295	298	304	rBV2	460	513	0.08%	0.010%
6	2.520	364	367	369	rBV2	289	170	0.02%	0.003%
7	2.572	372	383	407	rVV	144114	240588	35.35%	4.469%
8	2.774	443	446	450	rBV2	400	376	0.06%	0.007%
9	2.842	463	467	470	rBV	174	143	0.02%	0.003%
10	2.874	473	477	481	rBV2	299	373	0.05%	0.007%
11	3.051	529	532	537	rVB2	285	233	0.03%	0.004%
12	3.121	550	554	558	rBV	446	374	0.05%	0.007%
13	3.173	567	570	573	rBV3	305	276	0.04%	0.005%
14	3.340	618	622	627	rBV2	412	471	0.07%	0.009%
15	3.388	634	637	640	rBV	322	188	0.03%	0.003%
16	3.404	640	642	645	rBV2	247	120	0.02%	0.002%
17	3.504	667	673	676	rBV	284	329	0.05%	0.006%
18	3.594	698	701	706	rVB2	220	133	0.02%	0.002%
19	3.642	712	716	721	rVB	608	598	0.09%	0.011%
20	3.671	721	725	727	rBV	334	249	0.04%	0.005%
21	3.723	738	741	742	rBV	234	131	0.02%	0.002%
22	3.845	777	779	781	rBV	97	53	0.01%	0.001%
23	3.861	781	784	787	rVV	224	153	0.02%	0.003%
24	3.887	787	792	795	rBV	327	292	0.04%	0.005%
25	3.945	807	810	813	rBV2	245	164	0.02%	0.003%
26	3.993	822	825	828	rBV	201	154	0.02%	0.003%
27	4.031	833	837	839	rBV	307	250	0.04%	0.005%
28	4.125	863	866	871	rVB	393	330	0.05%	0.006%
29	4.256	904	907	914	rBV	336	343	0.05%	0.006%
30	4.311	921	924	927	rVB2	285	187	0.03%	0.003%
31	4.340	927	933	935	rBV	460	505	0.07%	0.009%
32	4.639	1013	1026	1061	rVB	59583	175445	25.78%	3.259%
33	4.948	1117	1122	1126	rBV	524	555	0.08%	0.010%
34	5.067	1144	1159	1181	rBV	117565	273797	40.22%	5.086%
35	5.292	1222	1229	1232	rBV	517	575	0.08%	0.011%
36	5.433	1269	1273	1276	rBV2	464	420	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046246.D
 Acq On : 10 Dec 2021 01:25
 Operator : SY/MD
 Sample : M4982-11
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.729	1342	1365	1384	rBV2	252363	680666	100.00%	12.643%
38	6.253	1514	1528	1544	rBV	202722	381193	56.00%	7.081%
39	6.533	1607	1615	1626	rBV5	3517	6604	0.97%	0.123%
40	6.694	1651	1665	1686	rBV	154901	299783	44.04%	5.568%
41	7.430	1891	1894	1900	rBV	390	384	0.06%	0.007%
42	7.498	1912	1915	1920	rBV	443	360	0.05%	0.007%
43	7.568	1924	1937	1952	rBV	88334	153220	22.51%	2.846%
44	7.681	1970	1972	1976	rBV3	427	312	0.05%	0.006%
45	7.899	2027	2040	2058	rBV	312877	537684	78.99%	9.988%
46	8.131	2109	2112	2116	rBV	410	383	0.06%	0.007%
47	8.179	2116	2127	2144	rVV	61821	101823	14.96%	1.891%
48	8.266	2152	2154	2157	rBV	269	171	0.03%	0.003%
49	8.636	2254	2269	2297	rBV	206605	367166	53.94%	6.820%
50	9.012	2382	2386	2390	rBV	489	554	0.08%	0.010%
51	9.144	2422	2427	2430	rBV	636	578	0.08%	0.011%
52	9.372	2495	2498	2500	rBV	306	215	0.03%	0.004%
53	9.417	2500	2512	2532	rVV	309858	514363	75.57%	9.554%
54	9.976	2680	2686	2689	rBV2	398	431	0.06%	0.008%
55	10.597	2876	2879	2882	rBV2	384	273	0.04%	0.005%
56	10.758	2917	2929	2946	rVB	237302	377679	55.49%	7.015%
57	11.031	3010	3014	3018	rBV	412	422	0.06%	0.008%
58	11.308	3096	3100	3103	rBV2	513	480	0.07%	0.009%
59	11.812	3244	3257	3279	rBV	340980	538334	79.09%	10.000%
60	12.105	3341	3348	3351	rBV2	497	670	0.10%	0.012%
61	12.195	3363	3376	3390	rBV	326813	525005	77.13%	9.752%
62	13.555	3796	3799	3803	rBV2	456	423	0.06%	0.008%
63	14.944	4228	4231	4234	rBV	511	315	0.05%	0.006%




Sum of corrected areas: 5383558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046246.D
Acq On : 10 Dec 2021 01:25
Operator : SY/MD
Sample : M4982-11
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

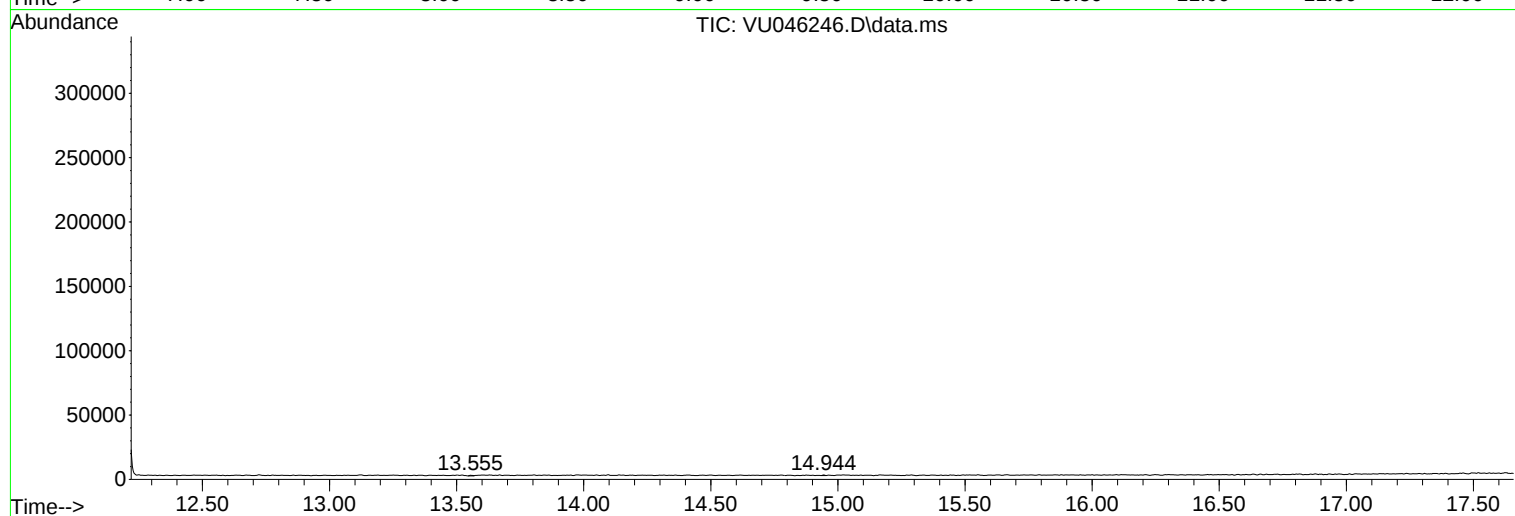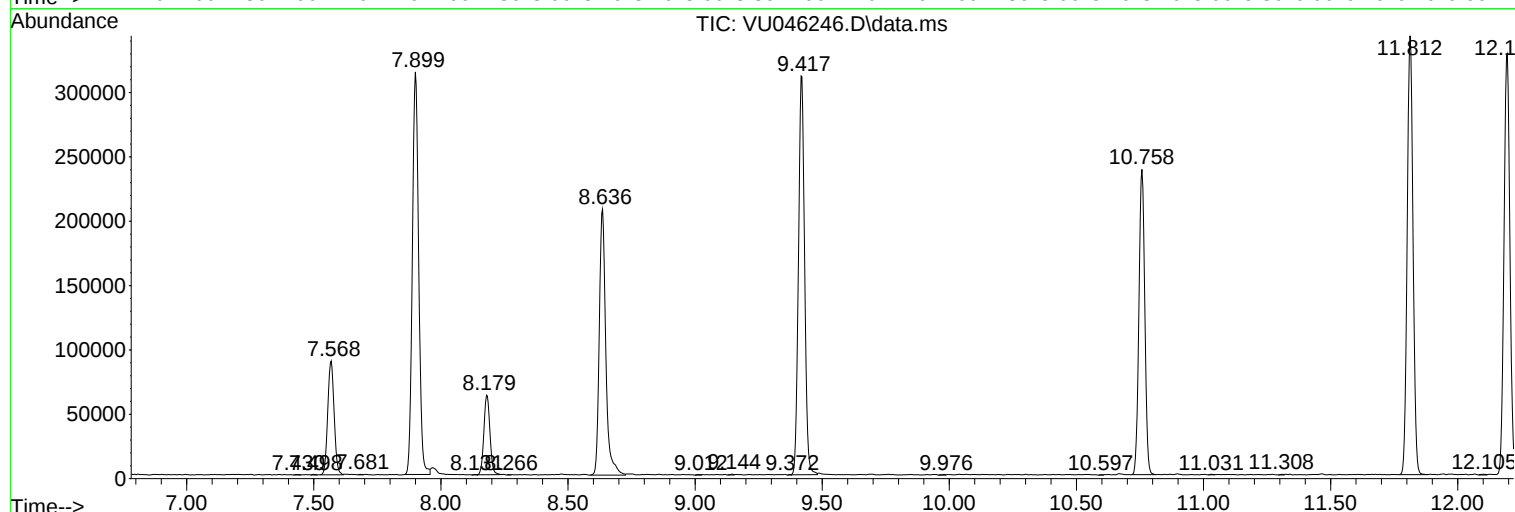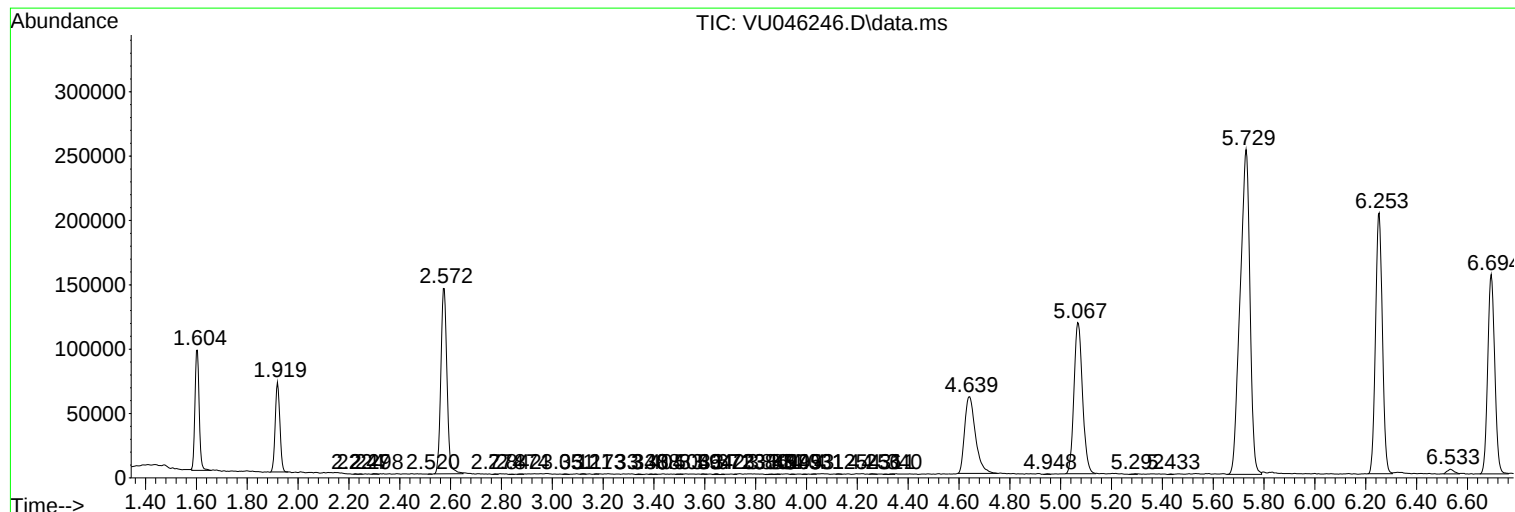

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046246.D
Acq On : 10 Dec 2021 01:25
Operator : SY/MD
Sample : M4982-11
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046246.D
Acq On : 10 Dec 2021 01:25
Operator : SY/MD
Sample : M4982-11
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc