

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046247.D
 Acq On : 10 Dec 2021 01:47
 Operator : SY/MD
 Sample : M4982-12
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046247.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	93072	102333	15.04%	1.873%
2	1.919	171	180	190	rBV	68692	87292	12.83%	1.598%
3	2.305	296	300	304	rBV3	339	304	0.04%	0.006%
4	2.379	320	323	330	rVB2	641	775	0.11%	0.014%
5	2.417	330	335	338	rBV2	438	452	0.07%	0.008%
6	2.501	357	361	366	rVB	584	440	0.06%	0.008%
7	2.530	366	370	372	rBV	501	410	0.06%	0.008%
8	2.575	372	384	404	rBV	144984	242239	35.61%	4.434%
9	2.678	413	416	419	rVB2	586	432	0.06%	0.008%
10	2.774	443	446	451	rBV2	363	374	0.05%	0.007%
11	2.806	452	456	461	rVB3	471	454	0.07%	0.008%
12	2.858	467	472	475	rBV2	355	375	0.06%	0.007%
13	2.874	475	477	483	rVB2	274	287	0.04%	0.005%
14	2.912	483	489	494	rVB2	511	613	0.09%	0.011%
15	3.440	649	653	658	rVB	415	375	0.06%	0.007%
16	3.472	659	663	666	rBV	414	333	0.05%	0.006%
17	3.649	712	718	721	rBV	354	316	0.05%	0.006%
18	3.764	751	754	759	rVB2	374	366	0.05%	0.007%
19	3.806	759	767	770	rBV	333	345	0.05%	0.006%
20	3.999	820	827	830	rBV2	294	334	0.05%	0.006%
21	4.070	846	849	856	rVB	436	507	0.07%	0.009%
22	4.105	856	860	864	rBV2	544	528	0.08%	0.010%
23	4.186	880	885	887	rBV2	523	463	0.07%	0.008%
24	4.491	977	980	984	rVB	503	361	0.05%	0.007%
25	4.578	1005	1007	1011	rBV2	368	367	0.05%	0.007%
26	4.639	1011	1026	1051	rBV	59923	173301	25.48%	3.172%
27	4.867	1092	1097	1100	rBV2	452	532	0.08%	0.010%
28	4.957	1120	1125	1130	rVB2	333	376	0.06%	0.007%
29	5.067	1142	1159	1184	rBV	117788	275020	40.43%	5.034%
30	5.289	1224	1228	1231	rVB2	422	310	0.05%	0.006%
31	5.314	1231	1236	1239	rBV2	394	456	0.07%	0.008%
32	5.398	1258	1262	1268	rVB2	322	384	0.06%	0.007%
33	5.629	1330	1334	1339	rVB	380	427	0.06%	0.008%
34	5.729	1339	1365	1385	rBV2	250933	680264	100.00%	12.451%
35	5.838	1397	1399	1403	rBV4	513	313	0.05%	0.006%
36	6.015	1451	1454	1459	rVB	575	511	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046247.D
 Acq On : 10 Dec 2021 01:47
 Operator : SY/MD
 Sample : M4982-12
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.051	1459	1465	1469	rBV2	459	549	0.08%	0.010%
38	6.179	1502	1505	1511	rVB	524	397	0.06%	0.007%
39	6.253	1511	1528	1547	rBV	203946	388058	57.05%	7.103%
40	6.542	1603	1618	1634	rBV5	32956	64513	9.48%	1.181%
41	6.694	1651	1665	1682	rBV	156573	300927	44.24%	5.508%
42	6.948	1739	1744	1748	rVV2	342	305	0.04%	0.006%
43	7.067	1777	1781	1784	rBV	353	340	0.05%	0.006%
44	7.186	1813	1818	1823	rVB2	609	638	0.09%	0.012%
45	7.276	1843	1846	1850	rBV2	319	358	0.05%	0.007%
46	7.395	1880	1883	1890	rBV2	344	393	0.06%	0.007%
47	7.504	1908	1917	1922	rBV	482	775	0.11%	0.014%
48	7.568	1922	1937	1952	rBV	86754	151726	22.30%	2.777%
49	7.694	1972	1976	1980	rVB3	442	371	0.05%	0.007%
50	7.806	2005	2011	2014	rBV2	615	611	0.09%	0.011%
51	7.899	2027	2040	2058	rBV	310902	540601	79.47%	9.895%
52	8.179	2116	2127	2141	rVV	60834	99655	14.65%	1.824%
53	8.346	2174	2179	2182	rBV	447	428	0.06%	0.008%
54	8.369	2182	2186	2190	rBV	337	313	0.05%	0.006%
55	8.478	2215	2220	2221	rBV2	349	313	0.05%	0.006%
56	8.636	2256	2269	2297	rBV	200710	356005	52.33%	6.516%
57	8.854	2333	2337	2341	rBV	394	356	0.05%	0.007%
58	9.417	2499	2512	2539	rBV	313135	521552	76.67%	9.546%
59	9.607	2567	2571	2577	rVB2	459	429	0.06%	0.008%
60	9.645	2577	2583	2592	rVB	632	977	0.14%	0.018%
61	9.690	2592	2597	2603	rBV3	734	1027	0.15%	0.019%
62	10.044	2704	2707	2713	rBV	445	542	0.08%	0.010%
63	10.073	2713	2716	2724	rVB2	372	470	0.07%	0.009%
64	10.372	2805	2809	2813	rBV2	336	337	0.05%	0.006%
65	10.581	2870	2874	2880	rVB	603	587	0.09%	0.011%
66	10.758	2916	2929	2948	rVB	234564	375972	55.27%	6.882%
67	10.896	2965	2972	2975	rBV3	433	516	0.08%	0.009%
68	10.941	2983	2986	2993	rBV2	346	384	0.06%	0.007%
69	11.195	3062	3065	3068	rBV	391	346	0.05%	0.006%
70	11.288	3090	3094	3099	rBV2	505	572	0.08%	0.010%
71	11.443	3136	3142	3145	rBV	616	585	0.09%	0.011%
72	11.468	3145	3150	3156	rVB3	714	830	0.12%	0.015%
73	11.652	3204	3207	3210	rBV2	465	333	0.05%	0.006%
74	11.812	3245	3257	3277	rBV	348123	542686	79.78%	9.933%
75	12.057	3328	3333	3336	rBV	424	344	0.05%	0.006%
76	12.195	3363	3376	3393	rBV	325017	524351	77.08%	9.598%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046247.D
 Acq On : 10 Dec 2021 01:47
 Operator : SY/MD
 Sample : M4982-12
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.262	3394	3397	3406	rVB3	596	660	0.10%	0.012%
78	12.311	3408	3412	3416	rVB2	440	317	0.05%	0.006%
79	12.385	3429	3435	3438	rBV2	280	300	0.04%	0.005%
80	12.529	3478	3480	3488	rVB2	276	344	0.05%	0.006%
81	12.584	3494	3497	3503	rBV	406	366	0.05%	0.007%
82	12.639	3510	3514	3517	rBV	417	324	0.05%	0.006%
83	12.838	3574	3576	3580	rVB2	451	304	0.04%	0.006%
84	12.870	3583	3586	3589	rBV	379	294	0.04%	0.005%
85	12.989	3620	3623	3629	rVB	464	408	0.06%	0.007%
86	13.057	3640	3644	3649	rVB	457	423	0.06%	0.008%
87	13.253	3701	3705	3709	rBV	368	341	0.05%	0.006%
88	13.687	3836	3840	3846	rBV2	530	509	0.07%	0.009%
89	13.944	3917	3920	3924	rVB	417	304	0.04%	0.006%
90	13.967	3924	3927	3930	rBV	424	397	0.06%	0.007%
91	14.275	4020	4023	4028	rVB	434	343	0.05%	0.006%
92	14.372	4049	4053	4059	rBV2	366	499	0.07%	0.009%
93	14.999	4245	4248	4251	rBV2	472	389	0.06%	0.007%
94	15.066	4265	4269	4272	rBV	550	407	0.06%	0.007%
95	15.397	4368	4372	4375	rVB2	624	438	0.06%	0.008%
96	15.423	4375	4380	4382	rBV2	427	434	0.06%	0.008%
97	15.793	4492	4495	4501	rVB3	478	369	0.05%	0.007%
98	16.349	4665	4668	4671	rBV2	562	416	0.06%	0.008%
99	16.973	4859	4862	4869	rBV4	594	623	0.09%	0.011%
100	17.050	4882	4886	4889	rBV4	702	700	0.10%	0.013%




Sum of corrected areas: 5463350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046247.D
Acq On : 10 Dec 2021 01:47
Operator : SY/MD
Sample : M4982-12
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

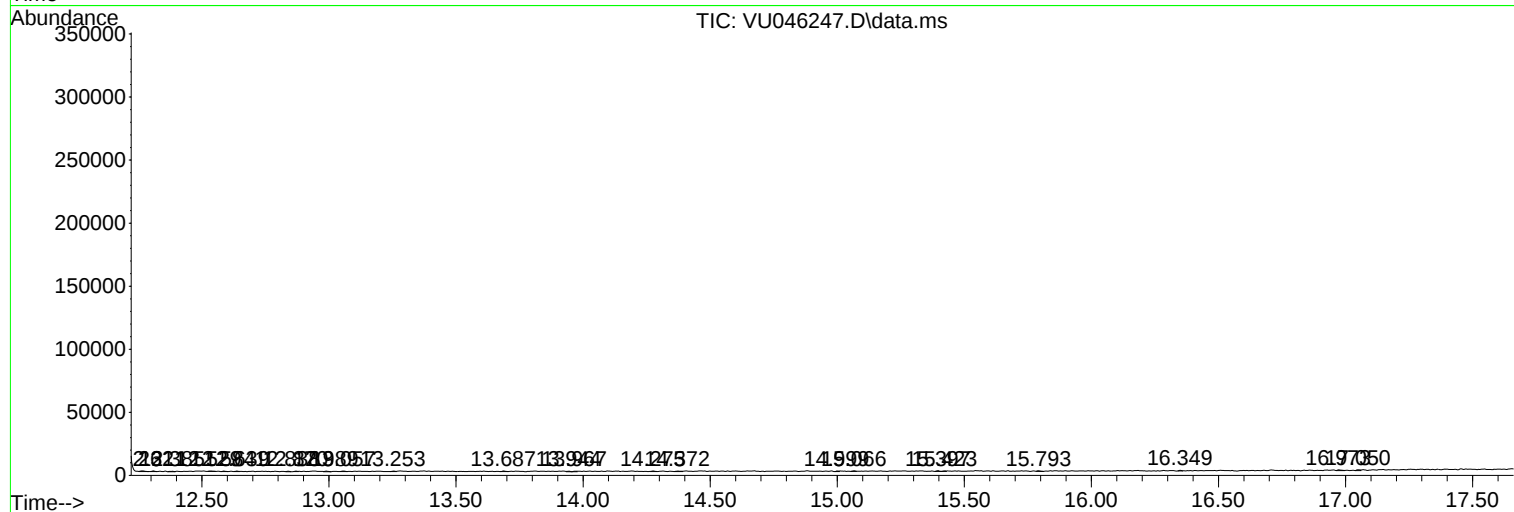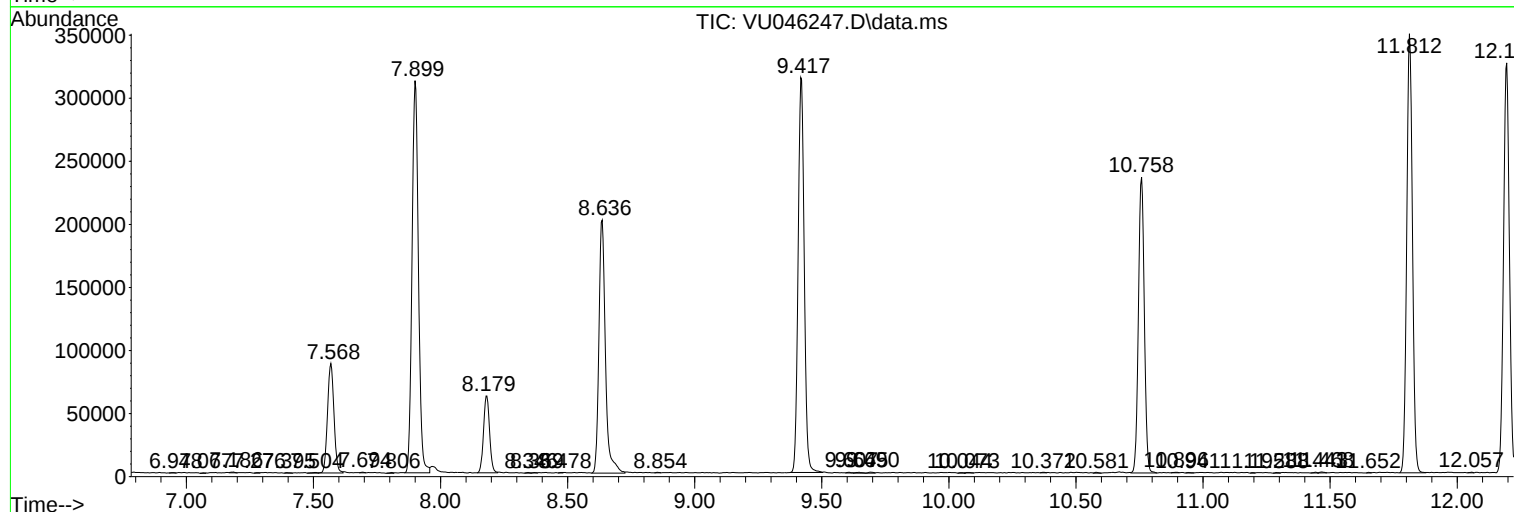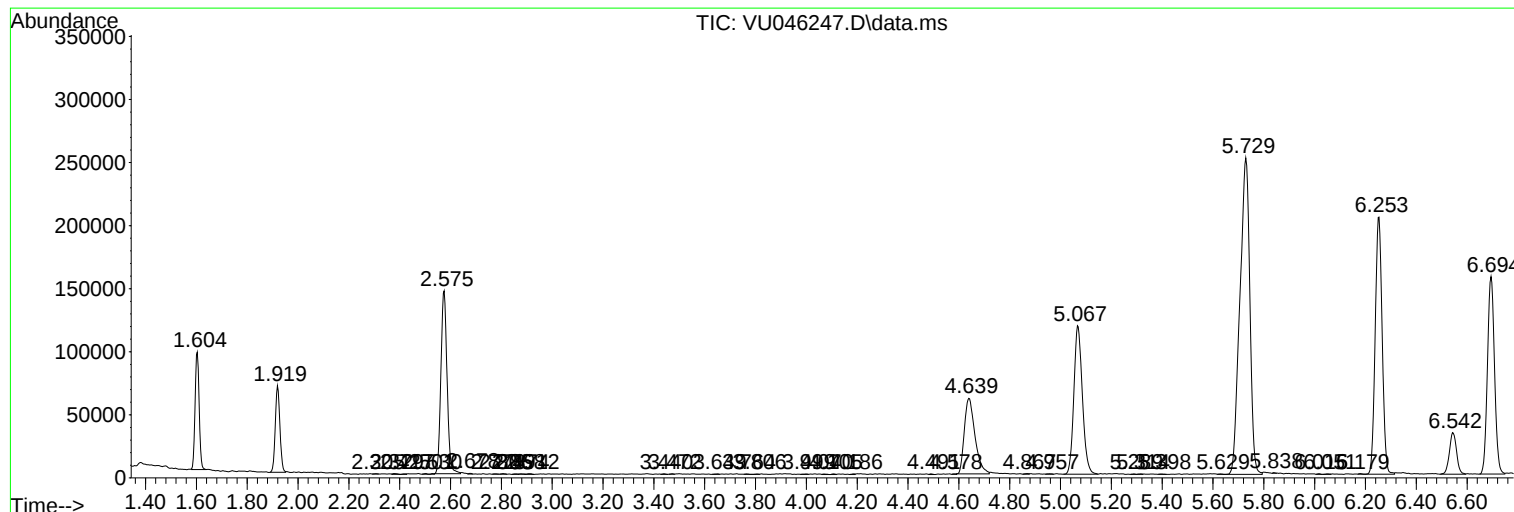

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046247.D
Acq On : 10 Dec 2021 01:47
Operator : SY/MD
Sample : M4982-12
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046247.D
Acq On : 10 Dec 2021 01:47
Operator : SY/MD
Sample : M4982-12
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------