

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046248.D
 Acq On : 10 Dec 2021 02:09
 Operator : SY/MD
 Sample : M4982-13
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	99	rVB	90632	102835	15.63%	1.964%
2	1.919	172	180	192	rVB	67756	86845	13.20%	1.659%
3	2.224	273	275	278	rBV2	451	269	0.04%	0.005%
4	2.273	287	290	295	rBV2	604	508	0.08%	0.010%
5	2.572	372	383	409	rBV	139435	233711	35.52%	4.463%
6	2.745	434	437	442	rVB2	509	513	0.08%	0.010%
7	2.957	500	503	506	rBV3	361	261	0.04%	0.005%
8	2.973	506	508	514	rVV2	367	274	0.04%	0.005%
9	3.019	519	522	525	rBV	434	318	0.05%	0.006%
10	3.305	608	611	615	rBV	381	316	0.05%	0.006%
11	3.530	678	681	683	rBV2	257	169	0.03%	0.003%
12	3.610	703	706	711	rBV	373	344	0.05%	0.007%
13	3.710	734	737	743	rBV	341	407	0.06%	0.008%
14	3.761	747	753	757	rVV	449	539	0.08%	0.010%
15	3.784	757	760	763	rBV	319	207	0.03%	0.004%
16	3.909	794	799	801	rBV	439	389	0.06%	0.007%
17	3.973	816	819	823	rBV2	242	209	0.03%	0.004%
18	4.057	841	845	847	rBV	487	343	0.05%	0.007%
19	4.147	869	873	877	rVB2	466	446	0.07%	0.009%
20	4.176	877	882	884	rBV2	262	213	0.03%	0.004%
21	4.256	904	907	909	rBV	140	100	0.02%	0.002%
22	4.276	909	913	918	rVB	504	438	0.07%	0.008%
23	4.301	918	921	923	rBV2	260	154	0.02%	0.003%
24	4.350	930	936	939	rBV	358	485	0.07%	0.009%
25	4.404	949	953	957	rBV	449	399	0.06%	0.008%
26	4.469	970	973	977	rVB2	290	194	0.03%	0.004%
27	4.491	977	980	981	rBV	198	106	0.02%	0.002%
28	4.639	1010	1026	1061	rBV	58000	169871	25.82%	3.244%
29	4.874	1096	1099	1102	rBV2	363	231	0.04%	0.004%
30	4.912	1109	1111	1113	rBV	220	141	0.02%	0.003%
31	5.067	1143	1159	1180	rBV	114644	269523	40.96%	5.147%
32	5.337	1240	1243	1248	rBV2	292	260	0.04%	0.005%
33	5.398	1259	1262	1264	rBV2	275	182	0.03%	0.003%
34	5.475	1284	1286	1290	rBV2	197	160	0.02%	0.003%
35	5.504	1290	1295	1298	rBV	603	569	0.09%	0.011%
36	5.610	1325	1328	1330	rBV2	153	92	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046248.D
 Acq On : 10 Dec 2021 02:09
 Operator : SY/MD
 Sample : M4982-13
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	5.729	1344	1365	1384	rBV2	242458	657995	100.00%	12.566%
38	5.996	1446	1448	1449	rBV2	168	71	0.01%	0.001%
39	6.025	1455	1457	1459	rBV	233	138	0.02%	0.003%
40	6.153	1491	1497	1500	rBV	457	501	0.08%	0.010%
41	6.253	1511	1528	1545	rBV	200358	377468	57.37%	7.209%
42	6.491	1599	1602	1605	rBV2	317	255	0.04%	0.005%
43	6.530	1605	1614	1630	rVV2	4366	8773	1.33%	0.168%
44	6.613	1637	1640	1642	rBV	278	148	0.02%	0.003%
45	6.645	1647	1650	1651	rBV	218	124	0.02%	0.002%
46	6.694	1651	1665	1683	rBV	151761	293948	44.67%	5.614%
47	6.986	1753	1756	1757	rBV	233	125	0.02%	0.002%
48	7.092	1786	1789	1792	rBV	268	202	0.03%	0.004%
49	7.153	1805	1808	1810	rBV	277	164	0.02%	0.003%
50	7.182	1810	1817	1819	rBV2	389	518	0.08%	0.010%
51	7.237	1827	1834	1835	rBV2	143	156	0.02%	0.003%
52	7.256	1835	1840	1844	rBV	424	471	0.07%	0.009%
53	7.468	1902	1906	1911	rVB	275	231	0.04%	0.004%
54	7.491	1911	1913	1916	rVB	291	155	0.02%	0.003%
55	7.514	1916	1920	1922	rBV	435	352	0.05%	0.007%
56	7.568	1925	1937	1951	rVB	84339	146116	22.21%	2.790%
57	7.774	1998	2001	2002	rBV	306	154	0.02%	0.003%
58	7.829	2011	2018	2024	rBV2	607	862	0.13%	0.016%
59	7.899	2027	2040	2058	rBV	304326	523911	79.62%	10.005%
60	8.182	2116	2128	2146	rBV2	58313	98127	14.91%	1.874%
61	8.472	2210	2218	2224	rBV3	818	1581	0.24%	0.030%
62	8.584	2249	2253	2255	rBV2	440	346	0.05%	0.007%
63	8.636	2258	2269	2294	rVV	190994	339500	51.60%	6.484%
64	8.822	2322	2327	2331	rBV	382	420	0.06%	0.008%
65	8.922	2353	2358	2361	rBV2	334	339	0.05%	0.006%
66	9.038	2391	2394	2396	rBV2	145	100	0.02%	0.002%
67	9.343	2486	2489	2491	rBV	328	229	0.03%	0.004%
68	9.420	2500	2513	2542	rBV	298521	507159	77.08%	9.685%
69	9.857	2646	2649	2651	rBV	299	195	0.03%	0.004%
70	9.890	2656	2659	2661	rBV	321	180	0.03%	0.003%
71	9.938	2671	2674	2675	rBV2	373	222	0.03%	0.004%
72	10.099	2721	2724	2727	rBV	481	346	0.05%	0.007%
73	10.218	2758	2761	2762	rBV	232	155	0.02%	0.003%
74	10.317	2790	2792	2796	rBV	293	178	0.03%	0.003%
75	10.616	2882	2885	2887	rBV	319	181	0.03%	0.003%
76	10.632	2887	2890	2892	rBV	370	209	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046248.D
 Acq On : 10 Dec 2021 02:09
 Operator : SY/MD
 Sample : M4982-13
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M

Title : VOC Analysis

77	10.758	2917	2929	2949	rVB	231051	364835	55.45%	6.967%
78	10.954	2987	2990	2994	rVB2	523	364	0.06%	0.007%
79	11.092	3029	3033	3035	rBV	447	372	0.06%	0.007%
80	11.388	3119	3125	3127	rBV	373	357	0.05%	0.007%
81	11.812	3244	3257	3274	rBV	334107	523355	79.54%	9.995%
82	11.973	3304	3307	3311	rBV2	573	367	0.06%	0.007%
83	12.195	3363	3376	3397	rVB	319955	510459	77.58%	9.748%
84	13.018	3629	3632	3638	rBV2	573	681	0.10%	0.013%
85	13.973	3925	3929	3935	rBV	543	729	0.11%	0.014%
86	14.838	4194	4198	4201	rBV	617	465	0.07%	0.009%




Sum of corrected areas: 5236310

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046248.D
Acq On : 10 Dec 2021 02:09
Operator : SY/MD
Sample : M4982-13
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

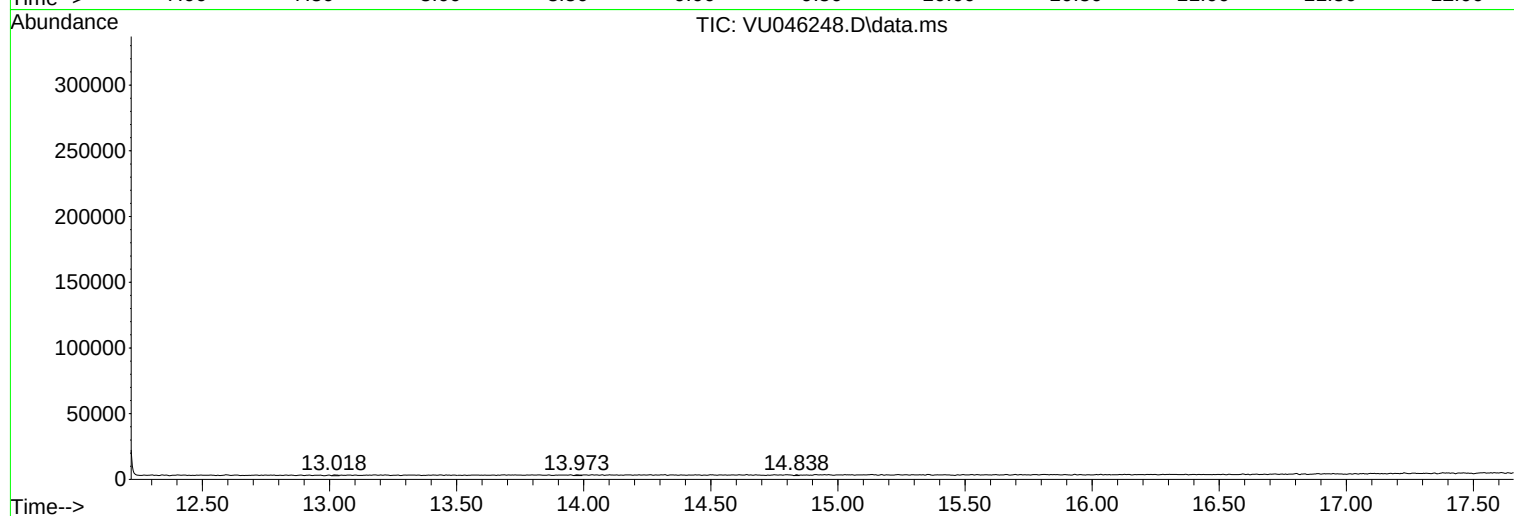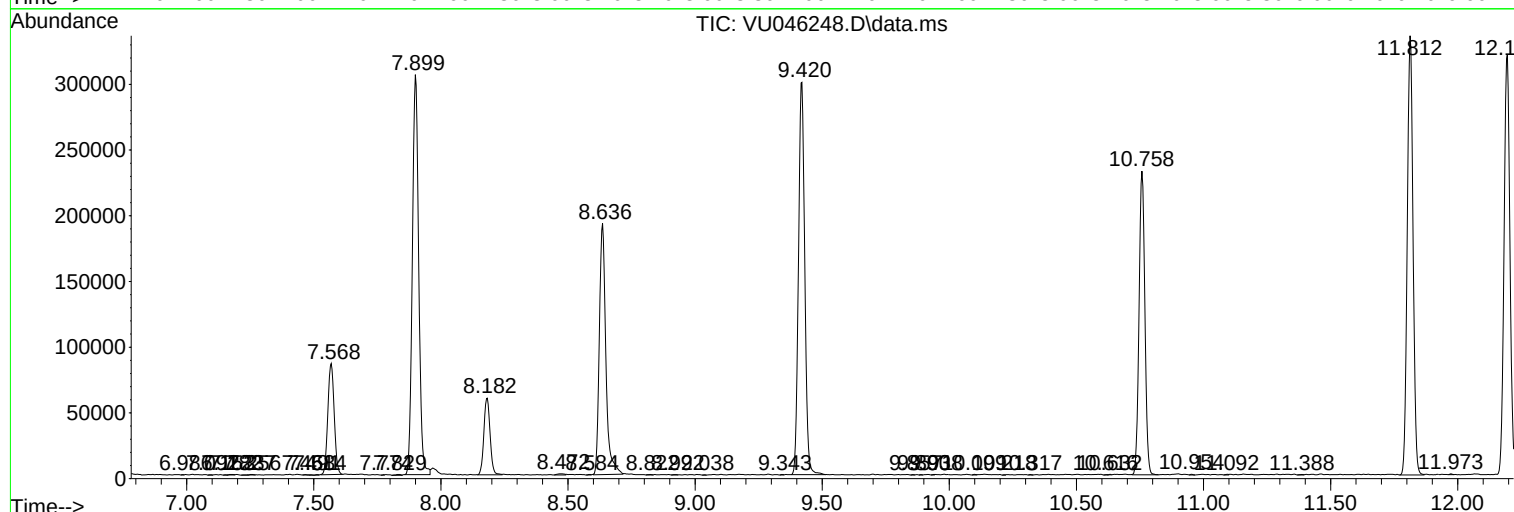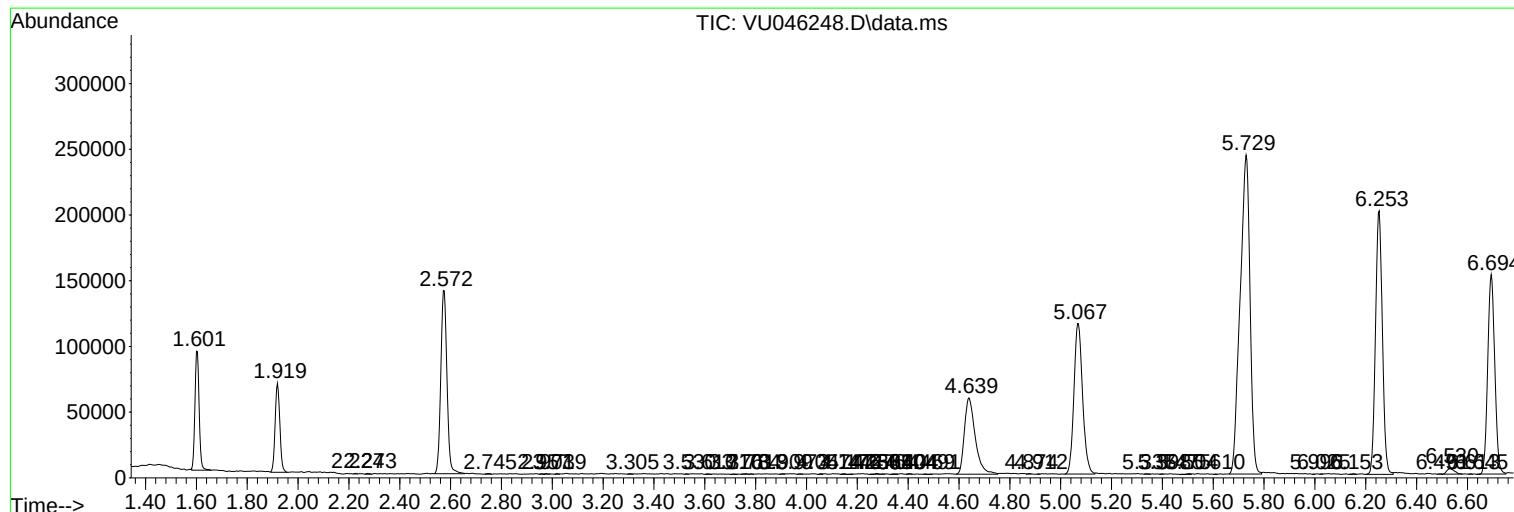

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046248.D
Acq On : 10 Dec 2021 02:09
Operator : SY/MD
Sample : M4982-13
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046248.D
Acq On : 10 Dec 2021 02:09
Operator : SY/MD
Sample : M4982-13
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc