

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046250.D
 Acq On : 10 Dec 2021 02:54
 Operator : SY/MD
 Sample : M4982-15
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	91	rVB	91382	99982	15.34%	1.929%
2	1.919	172	180	196	rVB	67099	85956	13.19%	1.658%
3	2.356	313	316	318	rBV3	565	345	0.05%	0.007%
4	2.420	333	336	338	rBV	314	189	0.03%	0.004%
5	2.437	338	341	344	rVB	403	203	0.03%	0.004%
6	2.514	361	365	366	rBV	269	186	0.03%	0.004%
7	2.575	371	384	407	rVV2	142260	249894	38.34%	4.821%
8	2.787	448	450	452	rBV2	208	106	0.02%	0.002%
9	3.047	528	531	534	rBV	262	133	0.02%	0.003%
10	3.096	542	546	550	rBV	335	335	0.05%	0.006%
11	3.182	570	573	577	rBV2	544	576	0.09%	0.011%
12	3.244	588	592	595	rBV	428	344	0.05%	0.007%
13	3.285	598	605	611	rBV2	307	476	0.07%	0.009%
14	3.507	671	674	676	rBV2	226	146	0.02%	0.003%
15	3.973	816	819	822	rBV	408	310	0.05%	0.006%
16	4.012	827	831	835	rBV2	375	337	0.05%	0.007%
17	4.080	847	852	857	rVB	325	360	0.06%	0.007%
18	4.317	922	926	929	rBV	474	449	0.07%	0.009%
19	4.446	963	966	968	rBV	264	153	0.02%	0.003%
20	4.491	977	980	982	rBV	453	294	0.05%	0.006%
21	4.639	1010	1026	1056	rBV	58735	185134	28.40%	3.571%
22	5.067	1143	1159	1183	rBV2	114216	267594	41.06%	5.162%
23	5.250	1213	1216	1217	rBV	286	137	0.02%	0.003%
24	5.491	1289	1291	1293	rBV	236	153	0.02%	0.003%
25	5.729	1343	1365	1383	rBV2	241376	651781	100.00%	12.573%
26	6.044	1457	1463	1465	rBV2	495	541	0.08%	0.010%
27	6.160	1497	1499	1501	rBV	277	187	0.03%	0.004%
28	6.253	1514	1528	1543	rBV	195099	362491	55.62%	6.993%
29	6.533	1606	1615	1630	rVB5	4023	8059	1.24%	0.155%
30	6.613	1635	1640	1647	rBV	633	898	0.14%	0.017%
31	6.694	1650	1665	1681	rBV	150790	289938	44.48%	5.593%
32	6.932	1736	1739	1741	rBV	185	97	0.01%	0.002%
33	6.944	1741	1743	1748	rVB2	264	221	0.03%	0.004%
34	6.977	1748	1753	1757	rBV	277	305	0.05%	0.006%
35	7.002	1757	1761	1764	rBV2	309	308	0.05%	0.006%
36	7.041	1770	1773	1775	rBV2	385	203	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046250.D
 Acq On : 10 Dec 2021 02:54
 Operator : SY/MD
 Sample : M4982-15
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.131	1798	1801	1805	rBV	387	331	0.05%	0.006%
38	7.256	1837	1840	1844	rBV	301	249	0.04%	0.005%
39	7.276	1844	1846	1851	rVV2	228	165	0.03%	0.003%
40	7.314	1855	1858	1864	rBV2	467	391	0.06%	0.008%
41	7.395	1879	1883	1885	rBV2	186	137	0.02%	0.003%
42	7.414	1885	1889	1893	rBV2	447	445	0.07%	0.009%
43	7.507	1912	1918	1922	rBV	361	446	0.07%	0.009%
44	7.568	1925	1937	1954	rVV	84467	145686	22.35%	2.810%
45	7.674	1967	1970	1971	rBV	285	177	0.03%	0.003%
46	7.726	1983	1986	1991	rBV2	251	227	0.03%	0.004%
47	7.758	1991	1996	1999	rBV2	368	377	0.06%	0.007%
48	7.790	2003	2006	2009	rBV2	352	230	0.04%	0.004%
49	7.813	2009	2013	2015	rBV	368	291	0.04%	0.006%
50	7.851	2022	2025	2027	rBV	245	151	0.02%	0.003%
51	7.899	2027	2040	2057	rBV	298801	516401	79.23%	9.962%
52	8.182	2116	2128	2148	rBV	57734	97057	14.89%	1.872%
53	8.401	2193	2196	2200	rVB3	404	295	0.05%	0.006%
54	8.465	2209	2216	2217	rBV2	589	624	0.10%	0.012%
55	8.636	2257	2269	2294	rBV	192610	343359	52.68%	6.624%
56	8.835	2328	2331	2334	rBV	433	261	0.04%	0.005%
57	9.025	2388	2390	2393	rBV	209	112	0.02%	0.002%
58	9.108	2413	2416	2421	rVB2	490	347	0.05%	0.007%
59	9.304	2473	2477	2480	rBV	366	277	0.04%	0.005%
60	9.420	2499	2513	2541	rBV	297707	494222	75.83%	9.534%
61	9.677	2590	2593	2595	rBV2	348	208	0.03%	0.004%
62	9.845	2642	2645	2646	rBV	206	115	0.02%	0.002%
63	9.906	2659	2664	2666	rBV	566	549	0.08%	0.011%
64	10.452	2830	2834	2836	rBV2	421	415	0.06%	0.008%
65	10.603	2878	2881	2883	rBV	342	219	0.03%	0.004%
66	10.671	2896	2902	2906	rBV3	917	984	0.15%	0.019%
67	10.758	2917	2929	2947	rVB	227905	360461	55.30%	6.954%
68	10.957	2985	2991	2993	rBV	281	329	0.05%	0.006%
69	11.044	3016	3018	3021	rVB	323	175	0.03%	0.003%
70	11.343	3108	3111	3114	rBV2	370	250	0.04%	0.005%
71	11.362	3114	3117	3125	rVB2	439	446	0.07%	0.009%
72	11.401	3126	3129	3132	rBV	300	261	0.04%	0.005%
73	11.812	3245	3257	3277	rBV	322490	506483	77.71%	9.770%
74	11.976	3305	3308	3312	rVB	536	396	0.06%	0.008%
75	12.195	3363	3376	3395	rBV	311053	501219	76.90%	9.669%
76	13.787	3868	3871	3874	rBV	338	256	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046250.D
Acq On : 10 Dec 2021 02:54
Operator : SY/MD
Sample : M4982-15
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Title : VOC Analysis




Sum of corrected areas: 5183845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046250.D
Acq On : 10 Dec 2021 02:54
Operator : SY/MD
Sample : M4982-15
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COCT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

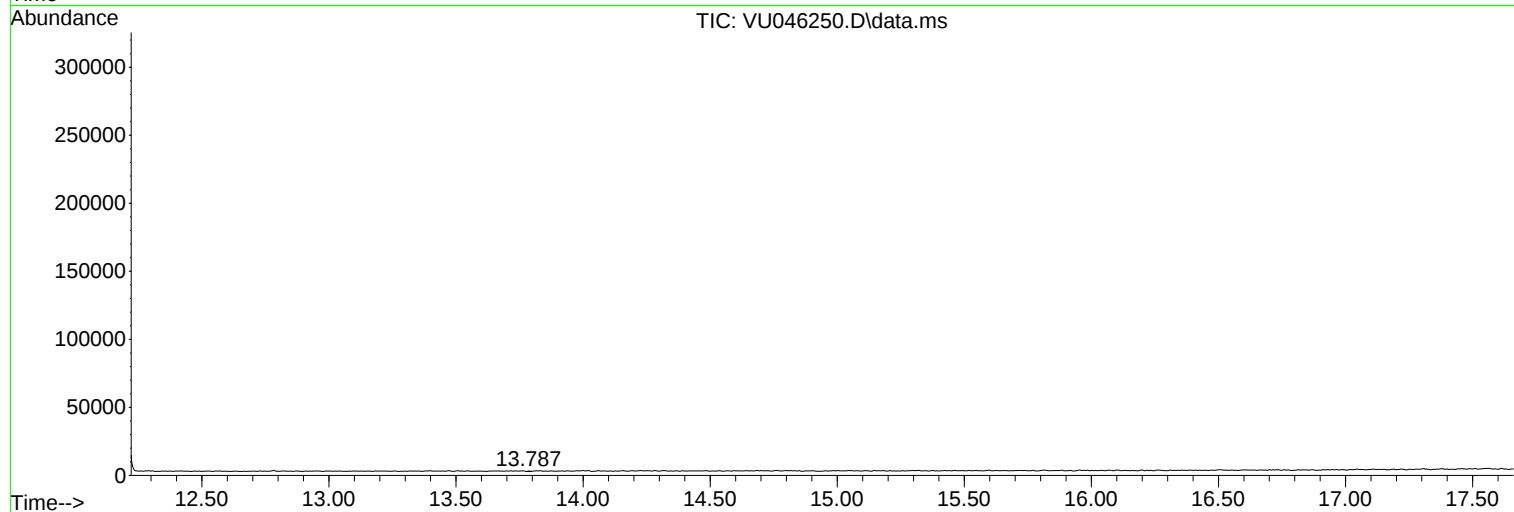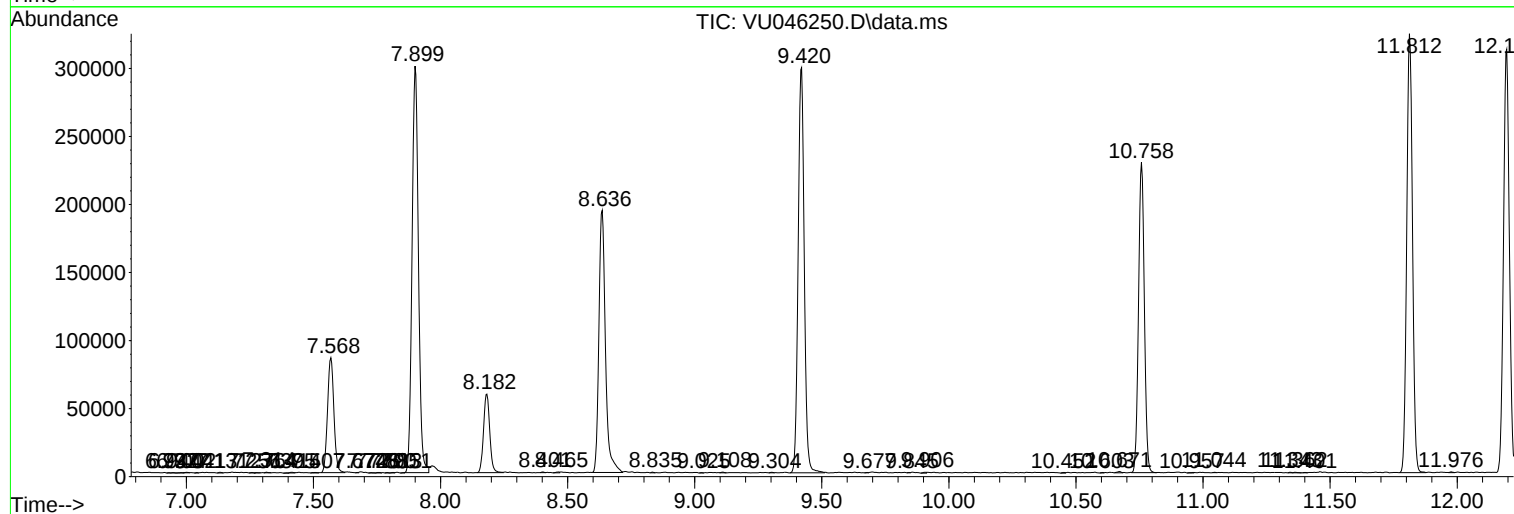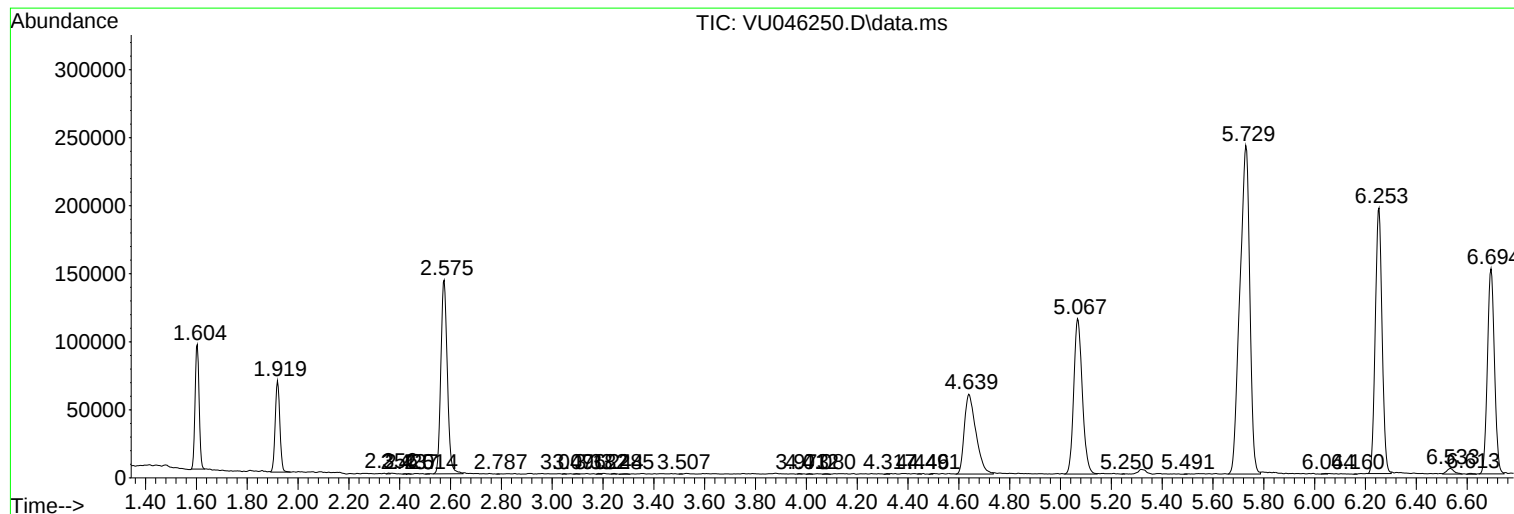

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046250.D
Acq On : 10 Dec 2021 02:54
Operator : SY/MD
Sample : M4982-15
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046250.D
Acq On : 10 Dec 2021 02:54
Operator : SY/MD
Sample : M4982-15
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc