

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046251.D
 Acq On : 10 Dec 2021 03:16
 Operator : SY/MD
 Sample : M4982-16
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	90678	100342	15.43%	1.810%
2	1.919	172	180	191	rVB	67450	84502	12.99%	1.524%
3	2.465	347	350	354	rBV2	372	397	0.06%	0.007%
4	2.575	372	384	399	rBV2	144738	246921	37.96%	4.453%
5	2.848	464	469	473	rVV2	357	402	0.06%	0.007%
6	3.131	554	557	566	rBV	322	365	0.06%	0.007%
7	3.244	587	592	594	rBV2	432	326	0.05%	0.006%
8	3.305	606	611	615	rBV2	389	383	0.06%	0.007%
9	3.941	805	809	811	rBV	520	351	0.05%	0.006%
10	4.131	862	868	873	rBV	277	341	0.05%	0.006%
11	4.195	883	888	892	rBV	453	518	0.08%	0.009%
12	4.250	902	905	911	rVB	344	371	0.06%	0.007%
13	4.321	923	927	930	rBV2	424	304	0.05%	0.005%
14	4.382	943	946	951	rVB	478	410	0.06%	0.007%
15	4.475	972	975	980	rVB	566	411	0.06%	0.007%
16	4.507	980	985	988	rBV2	407	407	0.06%	0.007%
17	4.568	1000	1004	1007	rBV	451	436	0.07%	0.008%
18	4.642	1012	1027	1056	rBV	57012	185538	28.52%	3.346%
19	5.067	1141	1159	1182	rBV2	113774	265883	40.88%	4.795%
20	5.179	1191	1194	1196	rBV	492	295	0.05%	0.005%
21	5.224	1204	1208	1210	rBV2	391	295	0.05%	0.005%
22	5.317	1227	1237	1238	rBV4	3549	4103	0.63%	0.074%
23	5.404	1261	1264	1267	rBV	435	333	0.05%	0.006%
24	5.462	1278	1282	1284	rBV2	348	333	0.05%	0.006%
25	5.559	1306	1312	1315	rBV	322	298	0.05%	0.005%
26	5.613	1324	1329	1332	rBV2	368	307	0.05%	0.006%
27	5.636	1332	1336	1342	rBV2	247	359	0.06%	0.006%
28	5.729	1344	1365	1383	rBV2	241166	650460	100.00%	11.732%
29	6.253	1514	1528	1548	rVV	189849	360169	55.37%	6.496%
30	6.388	1567	1570	1572	rBV	404	300	0.05%	0.005%
31	6.465	1591	1594	1601	rVB2	378	372	0.06%	0.007%
32	6.546	1605	1619	1634	rBV	201972	377294	58.00%	6.805%
33	6.694	1651	1665	1681	rBV	149486	286712	44.08%	5.171%
34	6.845	1709	1712	1718	rBV	455	376	0.06%	0.007%
35	6.896	1725	1728	1732	rVB2	505	390	0.06%	0.007%
36	6.931	1732	1739	1743	rBV2	337	521	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046251.D
 Acq On : 10 Dec 2021 03:16
 Operator : SY/MD
 Sample : M4982-16
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.976	1750	1753	1758	rVB	376	345	0.05%	0.006%
38	7.112	1789	1795	1799	rBV2	423	447	0.07%	0.008%
39	7.182	1813	1817	1822	rVV	420	421	0.06%	0.008%
40	7.497	1908	1915	1918	rBV2	391	457	0.07%	0.008%
41	7.568	1924	1937	1952	rBV	83075	143831	22.11%	2.594%
42	7.716	1979	1983	1987	rBV	377	356	0.05%	0.006%
43	7.790	2003	2006	2009	rVB	484	289	0.04%	0.005%
44	7.812	2009	2013	2015	rBV2	441	301	0.05%	0.005%
45	7.899	2024	2040	2056	rBV	292332	513002	78.87%	9.253%
46	8.179	2110	2127	2141	rBV	57382	95512	14.68%	1.723%
47	8.308	2161	2167	2169	rBV	301	350	0.05%	0.006%
48	8.443	2201	2209	2212	rBV	389	463	0.07%	0.008%
49	8.468	2212	2217	2219	rBV2	756	592	0.09%	0.011%
50	8.636	2254	2269	2297	rBV	194790	344991	53.04%	6.222%
51	8.822	2322	2327	2332	rBV2	456	510	0.08%	0.009%
52	8.928	2351	2360	2363	rBV2	448	624	0.10%	0.011%
53	8.996	2371	2381	2385	rBV	432	639	0.10%	0.012%
54	9.121	2415	2420	2423	rBV	332	291	0.04%	0.005%
55	9.263	2460	2464	2469	rVB2	437	373	0.06%	0.007%
56	9.375	2494	2499	2500	rBV	371	294	0.05%	0.005%
57	9.420	2500	2513	2536	rBV	288343	485806	74.69%	8.762%
58	9.693	2594	2598	2603	rVB3	360	435	0.07%	0.008%
59	9.716	2603	2605	2612	rVB2	319	313	0.05%	0.006%
60	9.751	2612	2616	2620	rBV	572	484	0.07%	0.009%
61	9.793	2625	2629	2631	rBV	444	357	0.05%	0.006%
62	9.873	2652	2654	2659	rVB	389	319	0.05%	0.006%
63	10.047	2705	2708	2714	rVB2	344	317	0.05%	0.006%
64	10.140	2732	2737	2742	rBV	396	371	0.06%	0.007%
65	10.246	2765	2770	2773	rBV	345	326	0.05%	0.006%
66	10.369	2804	2808	2812	rVB2	523	517	0.08%	0.009%
67	10.398	2812	2817	2819	rBV	560	496	0.08%	0.009%
68	10.446	2829	2832	2837	rVB2	347	326	0.05%	0.006%
69	10.478	2837	2842	2846	rBV	542	444	0.07%	0.008%
70	10.517	2848	2854	2857	rBV	424	447	0.07%	0.008%
71	10.574	2869	2872	2875	rBV	543	361	0.06%	0.007%
72	10.671	2897	2902	2908	rVB2	895	945	0.15%	0.017%
73	10.758	2917	2929	2946	rVB	224720	361825	55.63%	6.526%
74	10.854	2951	2959	2962	rBV2	554	873	0.13%	0.016%
75	10.893	2965	2971	2976	rBV3	693	998	0.15%	0.018%
76	10.992	2998	3002	3011	rVB	546	630	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046251.D
 Acq On : 10 Dec 2021 03:16
 Operator : SY/MD
 Sample : M4982-16
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.041	3011	3017	3020	rBV	371	415	0.06%	0.007%
78	11.060	3020	3023	3028	rBV2	282	334	0.05%	0.006%
79	11.279	3087	3091	3097	rBV	357	378	0.06%	0.007%
80	11.375	3117	3121	3124	rBV	403	333	0.05%	0.006%
81	11.471	3146	3151	3158	rBV3	478	595	0.09%	0.011%
82	11.700	3217	3222	3226	rBV2	676	714	0.11%	0.013%
83	11.812	3245	3257	3271	rBV	315226	499795	76.84%	9.014%
84	11.893	3278	3282	3286	rBV	430	403	0.06%	0.007%
85	11.976	3306	3308	3313	rVB3	513	371	0.06%	0.007%
86	12.037	3322	3327	3330	rBV2	461	436	0.07%	0.008%
87	12.102	3342	3347	3350	rBV	592	439	0.07%	0.008%
88	12.195	3363	3376	3393	rVB	315609	501842	77.15%	9.051%
89	12.381	3428	3434	3439	rBV	715	743	0.11%	0.013%
90	12.819	3567	3570	3576	rVB2	413	412	0.06%	0.007%
91	13.414	3748	3755	3759	rBV2	359	457	0.07%	0.008%
92	13.484	3773	3777	3782	rBV2	465	501	0.08%	0.009%
93	13.555	3797	3799	3806	rVB2	481	478	0.07%	0.009%
94	13.603	3807	3814	3817	rBV2	361	516	0.08%	0.009%
95	13.909	3905	3909	3916	rVB	539	557	0.09%	0.010%
96	14.034	3945	3948	3953	rBV2	364	326	0.05%	0.006%
97	14.822	4190	4193	4195	rBV	475	291	0.04%	0.005%
98	15.008	4246	4251	4258	rBV	598	869	0.13%	0.016%
99	15.494	4399	4402	4407	rBV3	367	382	0.06%	0.007%
100	16.098	4588	4590	4598	rVB3	619	658	0.10%	0.012%




Sum of corrected areas: 5544448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046251.D
Acq On : 10 Dec 2021 03:16
Operator : SY/MD
Sample : M4982-16
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

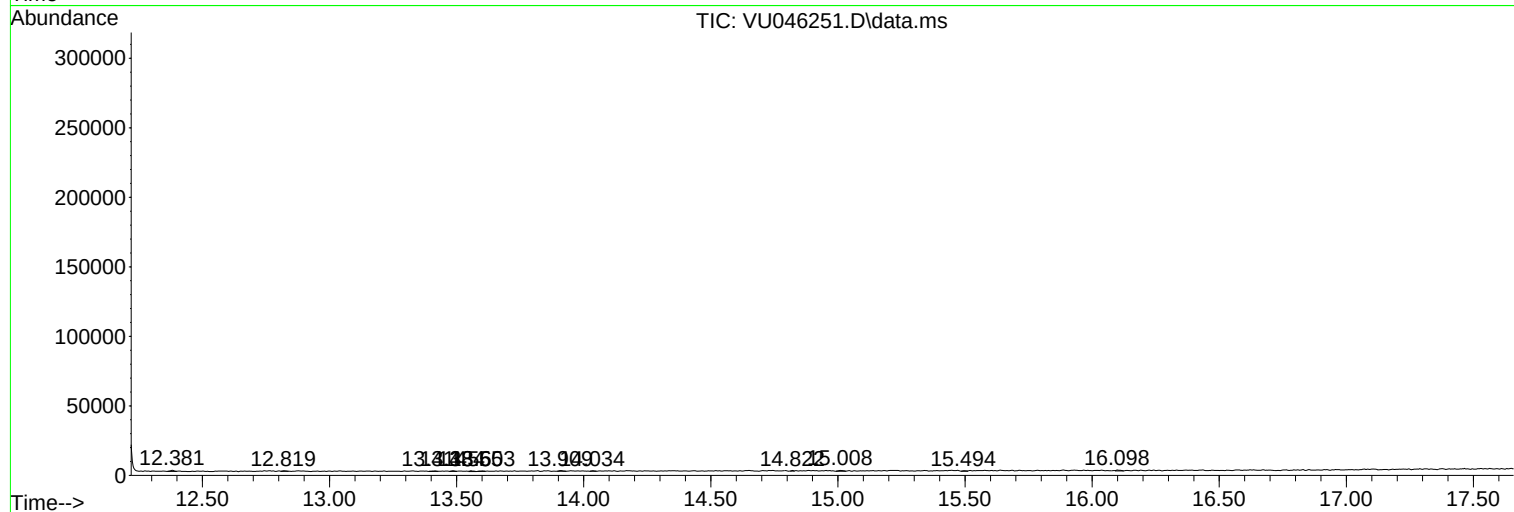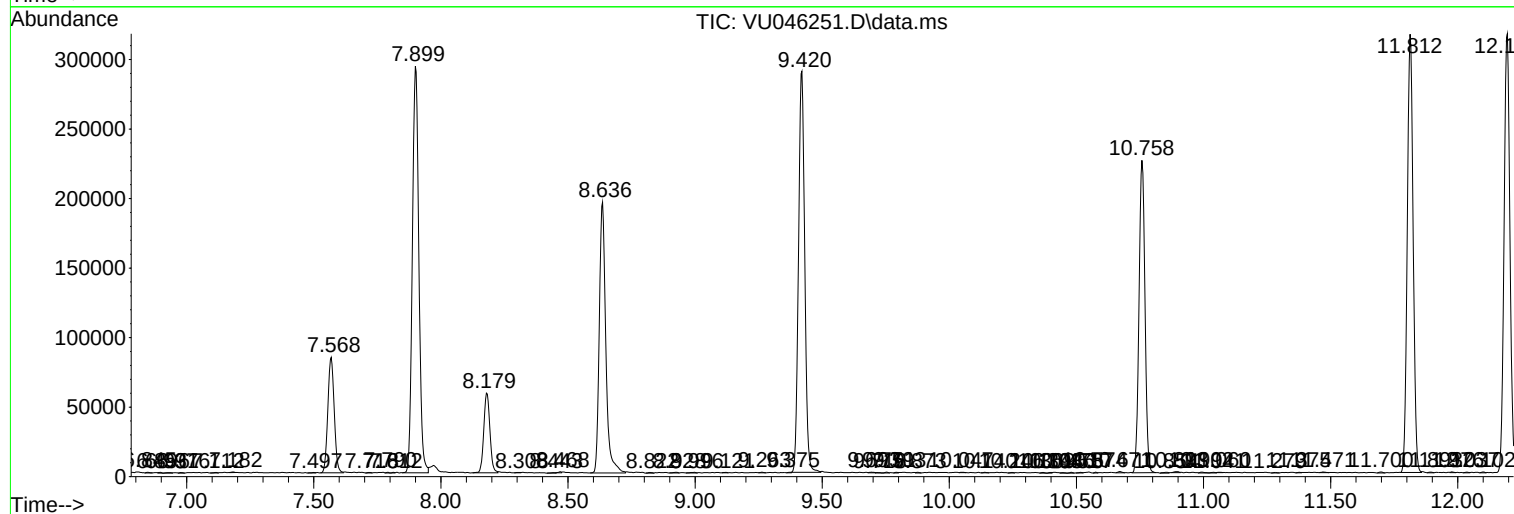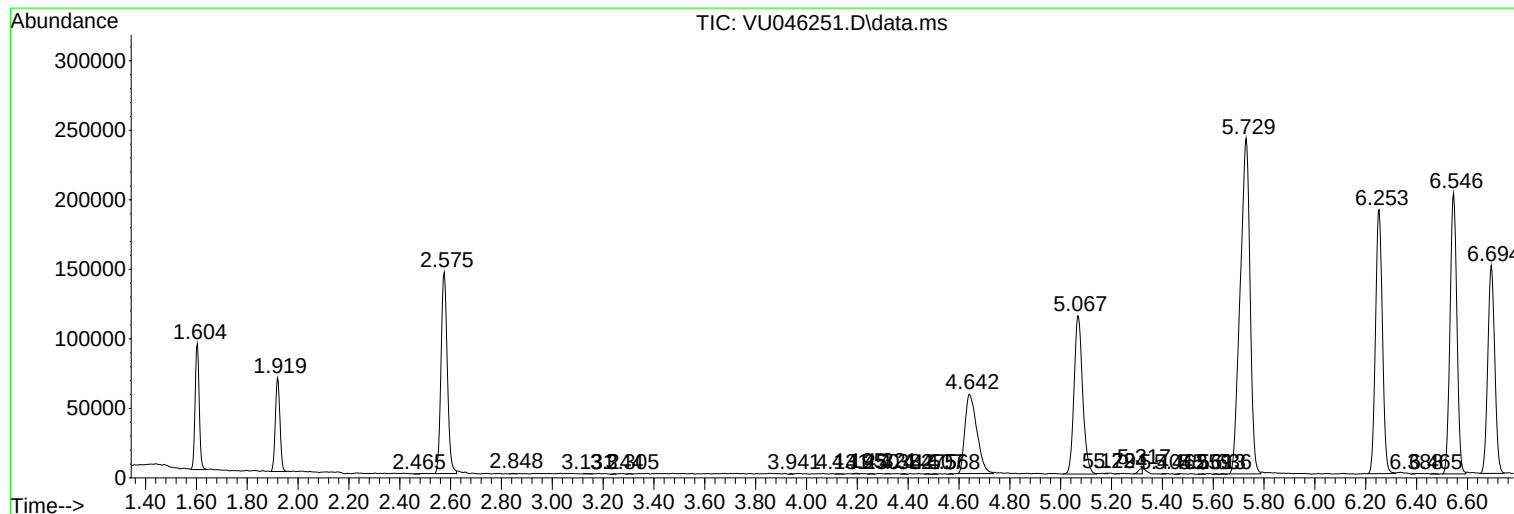

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046251.D
Acq On : 10 Dec 2021 03:16
Operator : SY/MD
Sample : M4982-16
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046251.D
Acq On : 10 Dec 2021 03:16
Operator : SY/MD
Sample : M4982-16
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc