

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046252.D
 Acq On : 10 Dec 2021 03:39
 Operator : SY/MD
 Sample : M4982-17
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	95	rVB	88758	98565	15.32%	1.931%
2	1.919	172	180	193	rVB	67095	85063	13.22%	1.667%
3	2.317	300	304	306	rBV	414	301	0.05%	0.006%
4	2.575	372	384	404	rBV	136298	226940	35.27%	4.447%
5	2.903	483	486	493	rVB2	493	551	0.09%	0.011%
6	3.192	571	576	581	rBV	596	691	0.11%	0.014%
7	3.288	603	606	610	rVB2	382	287	0.04%	0.006%
8	3.440	650	653	656	rBV2	406	357	0.06%	0.007%
9	3.504	667	673	675	rVV2	284	350	0.05%	0.007%
10	3.681	725	728	731	rBV	332	256	0.04%	0.005%
11	3.842	775	778	780	rBV	383	283	0.04%	0.006%
12	4.128	861	867	869	rBV	419	376	0.06%	0.007%
13	4.179	880	883	886	rVB	399	267	0.04%	0.005%
14	4.639	1010	1026	1058	rBV	58102	165169	25.67%	3.236%
15	5.070	1143	1160	1181	rBV	114286	261983	40.71%	5.133%
16	5.346	1243	1246	1255	rBV2	388	575	0.09%	0.011%
17	5.394	1256	1261	1263	rBV2	314	301	0.05%	0.006%
18	5.417	1265	1268	1272	rVB2	434	351	0.05%	0.007%
19	5.494	1289	1292	1297	rBV	413	314	0.05%	0.006%
20	5.597	1319	1324	1329	rVB	427	481	0.07%	0.009%
21	5.729	1344	1365	1382	rBV2	239473	643467	100.00%	12.608%
22	5.870	1407	1409	1418	rVB2	653	578	0.09%	0.011%
23	6.015	1451	1454	1458	rBV2	305	253	0.04%	0.005%
24	6.105	1478	1482	1487	rBV	417	449	0.07%	0.009%
25	6.253	1508	1528	1545	rBV	192652	360107	55.96%	7.056%
26	6.533	1606	1615	1629	rBV5	4118	8591	1.34%	0.168%
27	6.620	1638	1642	1646	rVB	397	315	0.05%	0.006%
28	6.645	1646	1650	1652	rBV2	419	318	0.05%	0.006%
29	6.693	1652	1665	1683	rBV	149939	287411	44.67%	5.632%
30	6.803	1697	1699	1708	rVB4	908	968	0.15%	0.019%
31	7.195	1818	1821	1825	rVB2	424	311	0.05%	0.006%
32	7.221	1825	1829	1832	rBV2	340	328	0.05%	0.006%
33	7.343	1864	1867	1873	rVB	230	267	0.04%	0.005%
34	7.388	1877	1881	1882	rBV	425	267	0.04%	0.005%
35	7.439	1894	1897	1900	rVV2	383	255	0.04%	0.005%
36	7.507	1915	1918	1920	rVV	366	283	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046252.D
 Acq On : 10 Dec 2021 03:39
 Operator : SY/MD
 Sample : M4982-17
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.568	1924	1937	1958	rVV	81689	142152	22.09%	2.785%
38	7.665	1964	1967	1970	rVV	332	281	0.04%	0.006%
39	7.684	1970	1973	1979	rVB3	484	527	0.08%	0.010%
40	7.838	2017	2021	2025	rBV2	295	289	0.04%	0.006%
41	7.899	2026	2040	2057	rBV	294128	513862	79.86%	10.069%
42	8.182	2117	2128	2145	rVV	57239	94118	14.63%	1.844%
43	8.282	2155	2159	2166	rBV2	198	304	0.05%	0.006%
44	8.385	2188	2191	2193	rBV	340	260	0.04%	0.005%
45	8.449	2208	2211	2213	rBV	416	297	0.05%	0.006%
46	8.472	2213	2218	2223	rVV3	880	1013	0.16%	0.020%
47	8.581	2247	2252	2257	rBV	510	690	0.11%	0.014%
48	8.636	2257	2269	2299	rVV	195056	341032	53.00%	6.682%
49	9.012	2382	2386	2389	rBV	368	262	0.04%	0.005%
50	9.034	2390	2393	2397	rVB	490	345	0.05%	0.007%
51	9.089	2406	2410	2412	rBV	322	258	0.04%	0.005%
52	9.144	2424	2427	2432	rVV2	468	413	0.06%	0.008%
53	9.369	2494	2497	2500	rVB	571	386	0.06%	0.008%
54	9.420	2500	2513	2541	rBV	286002	486138	75.55%	9.526%
55	9.690	2594	2597	2602	rVB3	497	460	0.07%	0.009%
56	9.719	2602	2606	2612	rBV2	290	295	0.05%	0.006%
57	9.754	2612	2617	2621	rBV2	350	369	0.06%	0.007%
58	9.870	2651	2653	2661	rVB2	345	330	0.05%	0.006%
59	10.047	2704	2708	2711	rBV	566	386	0.06%	0.008%
60	10.121	2727	2731	2735	rBV	413	397	0.06%	0.008%
61	10.481	2840	2843	2849	rVB	305	294	0.05%	0.006%
62	10.581	2871	2874	2877	rBV	450	328	0.05%	0.006%
63	10.674	2896	2903	2907	rBV2	895	992	0.15%	0.019%
64	10.758	2916	2929	2951	rBV	223178	355120	55.19%	6.958%
65	10.880	2964	2967	2971	rBV	470	504	0.08%	0.010%
66	11.018	3007	3010	3017	rVB	550	498	0.08%	0.010%
67	11.066	3022	3025	3033	rVB2	275	325	0.05%	0.006%
68	11.143	3045	3049	3052	rBV2	362	362	0.06%	0.007%
69	11.253	3076	3083	3087	rBV	458	591	0.09%	0.012%
70	11.378	3118	3122	3127	rBV2	294	318	0.05%	0.006%
71	11.465	3145	3149	3152	rVV3	438	317	0.05%	0.006%
72	11.645	3193	3205	3212	rVB2	513	1012	0.16%	0.020%
73	11.703	3219	3223	3227	rBV	465	402	0.06%	0.008%
74	11.812	3245	3257	3274	rBV	324409	501034	77.86%	9.818%
75	11.883	3274	3279	3284	rBV3	574	664	0.10%	0.013%
76	11.912	3284	3288	3292	rVB	415	321	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046252.D
 Acq On : 10 Dec 2021 03:39
 Operator : SY/MD
 Sample : M4982-17
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.047	3326	3330	3335	rBV2	343	344	0.05%	0.007%
78	12.195	3363	3376	3390	rBV	311221	497943	77.38%	9.757%
79	12.368	3425	3430	3435	rBB	464	508	0.08%	0.010%
80	12.433	3443	3450	3454	rBV2	294	359	0.06%	0.007%
81	12.510	3469	3474	3478	rBV2	477	518	0.08%	0.010%
82	12.687	3525	3529	3532	rBV	389	303	0.05%	0.006%
83	12.896	3591	3594	3597	rVB	415	269	0.04%	0.005%
84	13.577	3802	3806	3812	rVB	473	509	0.08%	0.010%
85	13.613	3812	3817	3823	rVB	341	363	0.06%	0.007%
86	13.709	3842	3847	3853	rBV	356	475	0.07%	0.009%
87	13.880	3897	3900	3902	rBV2	402	289	0.04%	0.006%
88	13.928	3911	3915	3918	rBV	439	371	0.06%	0.007%
89	13.944	3918	3920	3926	rVV	402	438	0.07%	0.009%
90	14.012	3939	3941	3947	rVB2	368	349	0.05%	0.007%
91	14.085	3957	3964	3968	rBV2	535	595	0.09%	0.012%
92	14.111	3968	3972	3979	rVV2	485	624	0.10%	0.012%
93	14.346	4041	4045	4051	rBV	568	564	0.09%	0.011%
94	14.401	4059	4062	4066	rVB	636	446	0.07%	0.009%
95	14.426	4066	4070	4074	rBV	691	609	0.09%	0.012%
96	15.304	4340	4343	4346	rBV	412	377	0.06%	0.007%
97	15.474	4393	4396	4399	rVB2	622	364	0.06%	0.007%
98	15.645	4445	4449	4452	rBV2	576	492	0.08%	0.010%
99	15.783	4489	4492	4494	rBV	384	268	0.04%	0.005%
100	15.831	4502	4507	4509	rBV2	545	522	0.08%	0.010%




Sum of corrected areas: 5103474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046252.D
Acq On : 10 Dec 2021 03:39
Operator : SY/MD
Sample : M4982-17
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COCT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

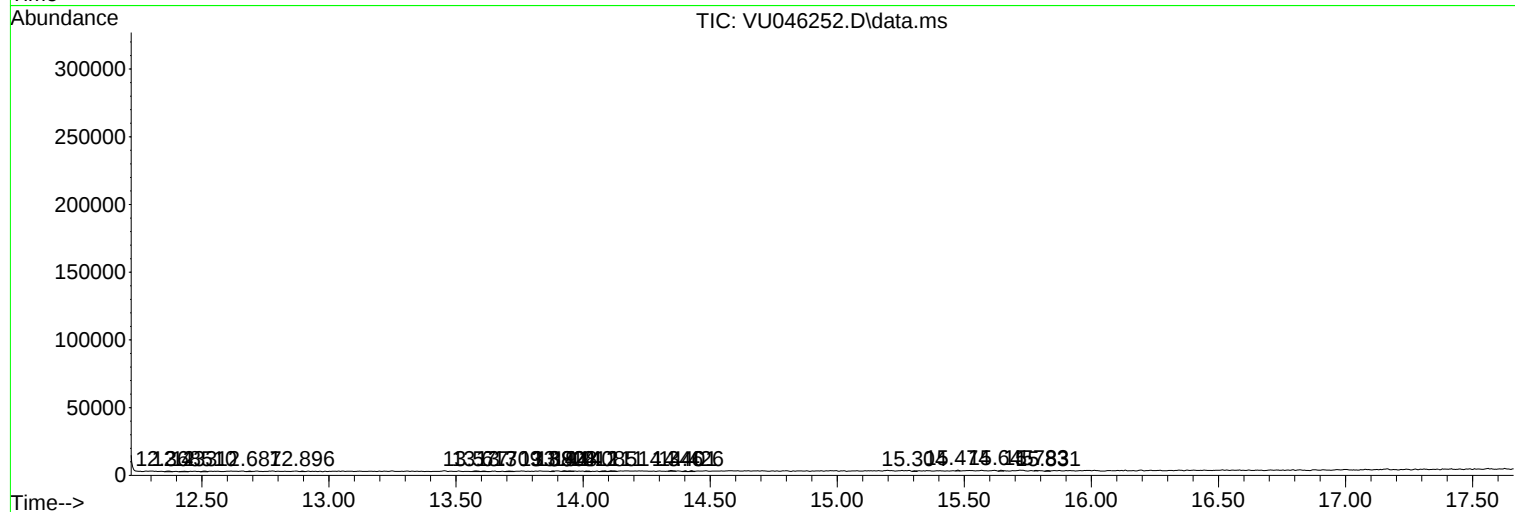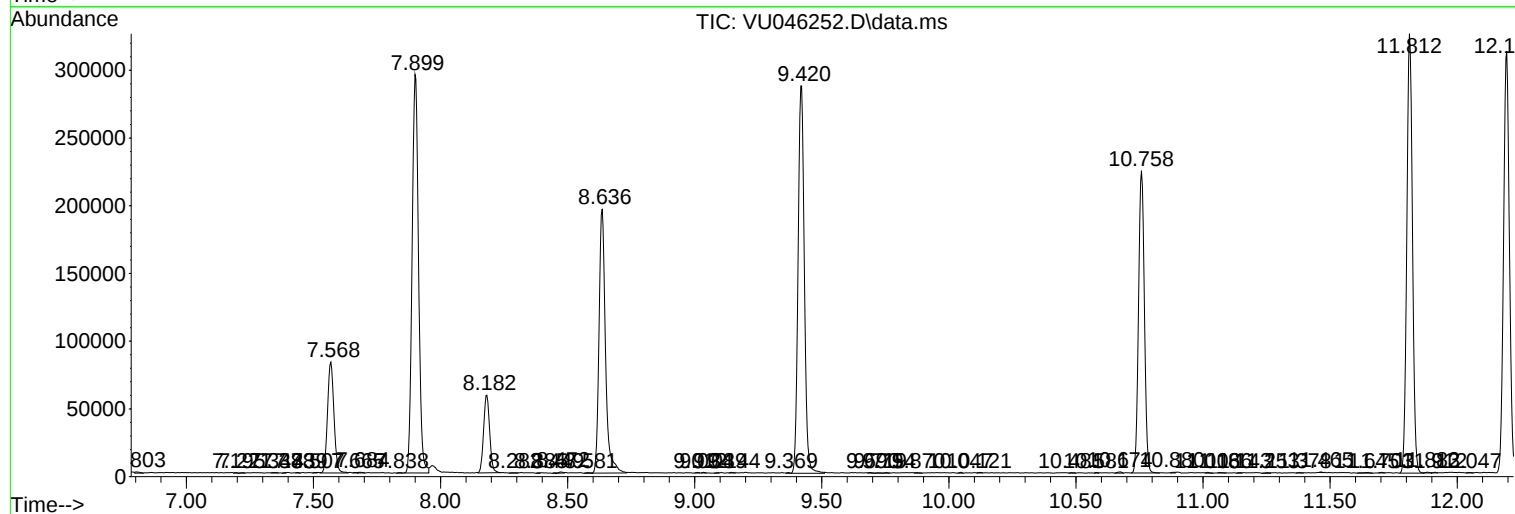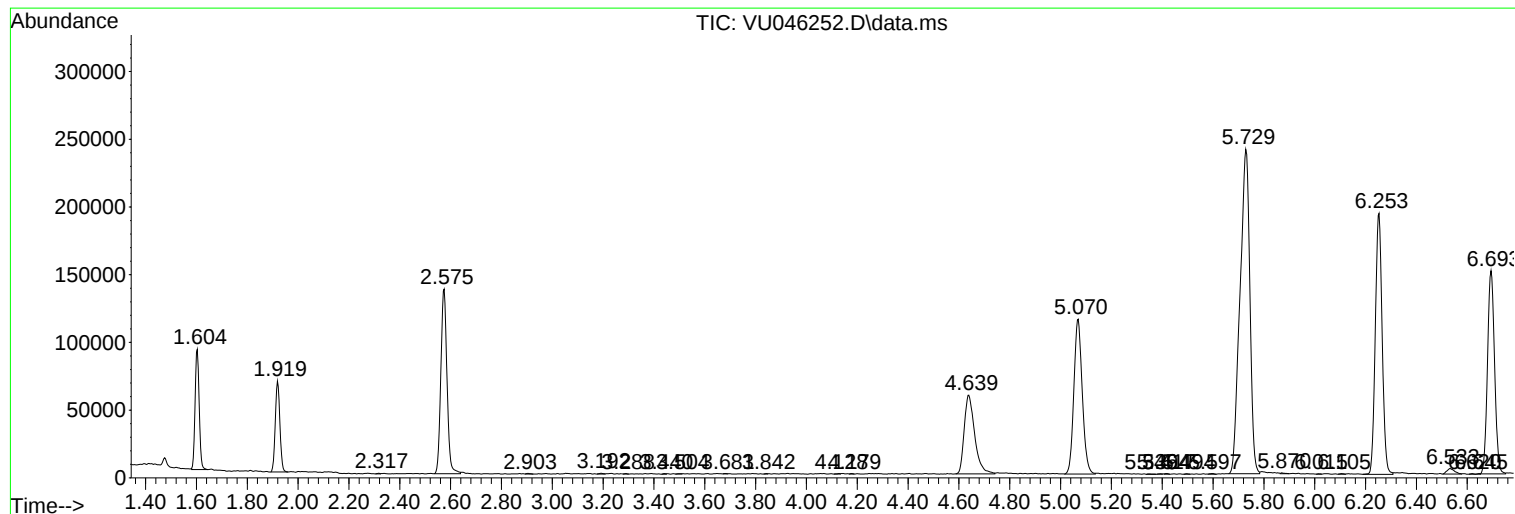

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046252.D
Acq On : 10 Dec 2021 03:39
Operator : SY/MD
Sample : M4982-17
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046252.D
Acq On : 10 Dec 2021 03:39
Operator : SY/MD
Sample : M4982-17
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc