

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046254.D
 Acq On : 10 Dec 2021 04:24
 Operator : SY/MD
 Sample : M4982-19
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	87044	97228	15.13%	1.902%
2	1.919	172	180	192	rVB	65060	83756	13.03%	1.639%
3	2.295	294	297	303	rBV4	545	626	0.10%	0.012%
4	2.388	320	326	329	rBV2	648	581	0.09%	0.011%
5	2.575	371	384	406	rVV	138004	229924	35.77%	4.499%
6	2.793	448	452	462	rVB	698	873	0.14%	0.017%
7	2.931	489	495	503	rVV2	540	833	0.13%	0.016%
8	3.054	531	533	540	rVB2	558	512	0.08%	0.010%
9	3.314	608	614	616	rBV	619	617	0.10%	0.012%
10	3.385	632	636	641	rVB	620	664	0.10%	0.013%
11	3.562	688	691	696	rVB	689	537	0.08%	0.011%
12	3.603	701	704	714	rVB	572	728	0.11%	0.014%
13	3.822	767	772	777	rBV	394	507	0.08%	0.010%
14	4.189	883	886	892	rVB2	527	593	0.09%	0.012%
15	4.224	892	897	900	rBV	538	598	0.09%	0.012%
16	4.282	910	915	919	rBV	522	518	0.08%	0.010%
17	4.562	997	1002	1006	rBV	627	669	0.10%	0.013%
18	4.639	1010	1026	1056	rVV2	55633	165260	25.71%	3.233%
19	4.870	1094	1098	1101	rBV2	522	520	0.08%	0.010%
20	4.922	1111	1114	1119	rBV2	402	449	0.07%	0.009%
21	4.951	1119	1123	1131	rVB2	608	703	0.11%	0.014%
22	5.070	1143	1160	1181	rBV	110815	261638	40.71%	5.119%
23	5.182	1192	1195	1199	rVB	733	625	0.10%	0.012%
24	5.211	1200	1204	1206	rBV	616	434	0.07%	0.008%
25	5.292	1223	1229	1232	rBV	598	468	0.07%	0.009%
26	5.420	1265	1269	1274	rBV2	375	418	0.07%	0.008%
27	5.729	1344	1365	1385	rBV2	237370	642751	100.00%	12.576%
28	5.812	1389	1391	1395	rVV3	600	467	0.07%	0.009%
29	5.912	1418	1422	1425	rBV	498	390	0.06%	0.008%
30	6.041	1457	1462	1467	rBV3	480	418	0.07%	0.008%
31	6.153	1492	1497	1500	rBV2	561	538	0.08%	0.011%
32	6.253	1514	1528	1548	rBV	193634	362028	56.32%	7.083%
33	6.533	1606	1615	1617	rBV4	4842	6226	0.97%	0.122%
34	6.693	1650	1665	1682	rBV	150909	287737	44.77%	5.630%
35	6.931	1733	1739	1741	rBV2	448	393	0.06%	0.008%
36	7.066	1776	1781	1783	rBV	438	418	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046254.D
 Acq On : 10 Dec 2021 04:24
 Operator : SY/MD
 Sample : M4982-19
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COCT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.182	1814	1817	1823	rVB	771	717	0.11%	0.014%
38	7.246	1831	1837	1840	rBV	458	477	0.07%	0.009%
39	7.488	1903	1912	1913	rBV2	682	823	0.13%	0.016%
40	7.568	1923	1937	1951	rBV2	83398	143055	22.26%	2.799%
41	7.822	2010	2016	2020	rBV	430	555	0.09%	0.011%
42	7.899	2026	2040	2058	rBV	291391	507695	78.99%	9.933%
43	8.057	2086	2089	2094	rBV3	539	554	0.09%	0.011%
44	8.182	2117	2128	2142	rVB	57993	92832	14.44%	1.816%
45	8.320	2167	2171	2174	rBV	480	431	0.07%	0.008%
46	8.471	2212	2218	2222	rVV3	808	981	0.15%	0.019%
47	8.584	2249	2253	2257	rBV2	506	502	0.08%	0.010%
48	8.635	2257	2269	2298	rVV	187877	335624	52.22%	6.567%
49	8.812	2321	2324	2328	rBV	657	462	0.07%	0.009%
50	8.934	2358	2362	2366	rVB	537	435	0.07%	0.009%
51	9.060	2398	2401	2409	rVV	677	751	0.12%	0.015%
52	9.127	2419	2422	2428	rVB	834	622	0.10%	0.012%
53	9.211	2445	2448	2452	rBV	550	430	0.07%	0.008%
54	9.259	2458	2463	2468	rVB	559	621	0.10%	0.012%
55	9.349	2488	2491	2497	rVB	585	525	0.08%	0.010%
56	9.420	2498	2513	2535	rBV	293406	493311	76.75%	9.652%
57	9.565	2552	2558	2559	rBV	580	581	0.09%	0.011%
58	9.668	2586	2590	2593	rBV2	391	390	0.06%	0.008%
59	9.761	2611	2619	2621	rBV2	344	479	0.07%	0.009%
60	9.893	2657	2660	2664	rVB	660	441	0.07%	0.009%
61	10.208	2754	2758	2764	rVB	595	488	0.08%	0.010%
62	10.266	2773	2776	2781	rBV2	429	433	0.07%	0.008%
63	10.314	2788	2791	2797	rVB	695	725	0.11%	0.014%
64	10.397	2811	2817	2824	rBV	568	827	0.13%	0.016%
65	10.465	2829	2838	2840	rBV2	916	1384	0.22%	0.027%
66	10.539	2858	2861	2863	rBV	651	460	0.07%	0.009%
67	10.661	2895	2899	2901	rBV	549	405	0.06%	0.008%
68	10.758	2916	2929	2949	rBV	226382	358610	55.79%	7.016%
69	10.880	2963	2967	2970	rBV	640	579	0.09%	0.011%
70	11.468	3146	3150	3152	rBV2	623	489	0.08%	0.010%
71	11.552	3171	3176	3181	rVB	712	720	0.11%	0.014%
72	11.632	3198	3201	3207	rVB	501	394	0.06%	0.008%
73	11.680	3212	3216	3219	rBV2	471	507	0.08%	0.010%
74	11.738	3231	3234	3244	rVB	490	711	0.11%	0.014%
75	11.812	3244	3257	3274	rBV	321437	504295	78.46%	9.867%
76	12.195	3364	3376	3392	rVV	309575	492062	76.56%	9.628%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046254.D
 Acq On : 10 Dec 2021 04:24
 Operator : SY/MD
 Sample : M4982-19
 Misc : 5.6mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CT6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.394	3435	3438	3443	rBV	464	462	0.07%	0.009%
78	12.446	3449	3454	3456	rBV	505	433	0.07%	0.008%
79	12.600	3495	3502	3505	rBV	610	651	0.10%	0.013%
80	12.770	3550	3555	3559	rBV3	622	745	0.12%	0.015%
81	13.237	3696	3700	3705	rBV	767	762	0.12%	0.015%
82	13.327	3724	3728	3729	rBV	530	387	0.06%	0.008%
83	13.362	3735	3739	3743	rBV2	609	453	0.07%	0.009%
84	13.439	3760	3763	3766	rVB	639	424	0.07%	0.008%
85	13.658	3827	3831	3835	rBV	556	606	0.09%	0.012%
86	13.864	3893	3895	3900	rVB	554	386	0.06%	0.008%
87	13.889	3900	3903	3905	rBV	790	603	0.09%	0.012%
88	13.941	3916	3919	3922	rBV	660	404	0.06%	0.008%
89	14.188	3989	3996	3999	rBV	467	625	0.10%	0.012%
90	14.233	4006	4010	4012	rBV	524	465	0.07%	0.009%
91	14.999	4243	4248	4253	rBV	579	739	0.11%	0.014%
92	15.072	4268	4271	4274	rBV	530	440	0.07%	0.009%
93	15.089	4274	4276	4279	rVB	795	408	0.06%	0.008%
94	15.211	4312	4314	4319	rVB2	720	542	0.08%	0.011%
95	15.535	4410	4415	4416	rBV	570	501	0.08%	0.010%
96	15.799	4493	4497	4500	rBV2	750	605	0.09%	0.012%
97	15.844	4506	4511	4514	rBV	741	660	0.10%	0.013%
98	16.314	4655	4657	4661	rVB	891	496	0.08%	0.010%
99	16.343	4663	4666	4670	rBV2	710	604	0.09%	0.012%
100	17.066	4888	4891	4894	rBV	813	534	0.08%	0.010%




Sum of corrected areas: 5110963

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046254.D
Acq On : 10 Dec 2021 04:24
Operator : SY/MD
Sample : M4982-19
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COCT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

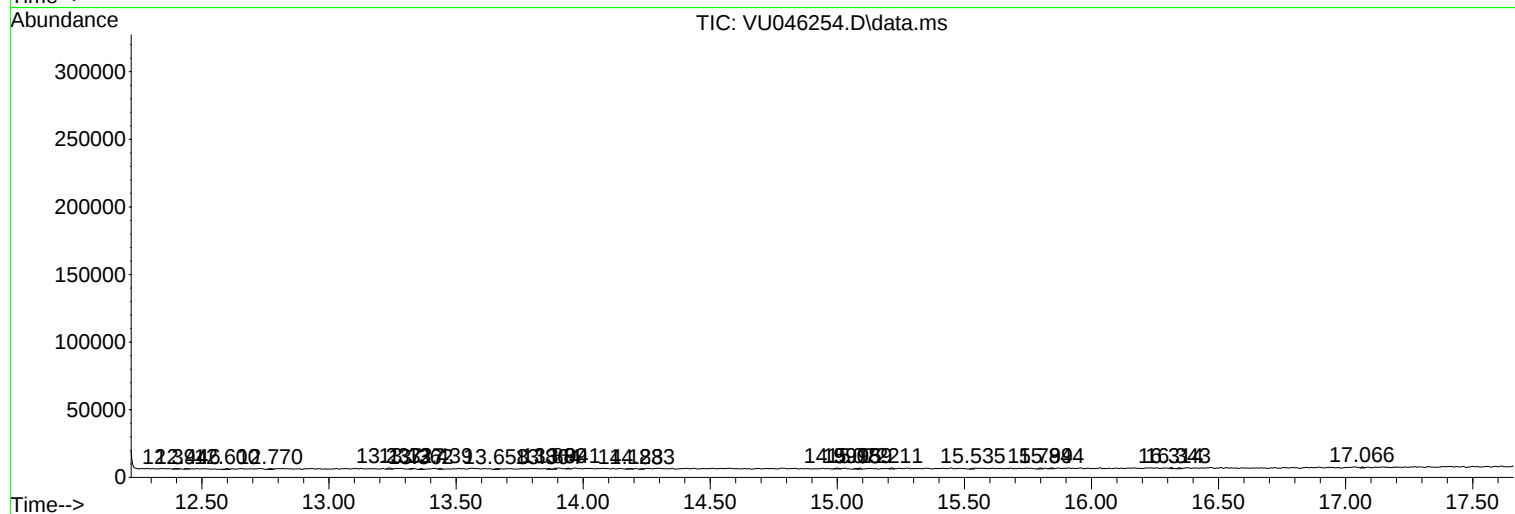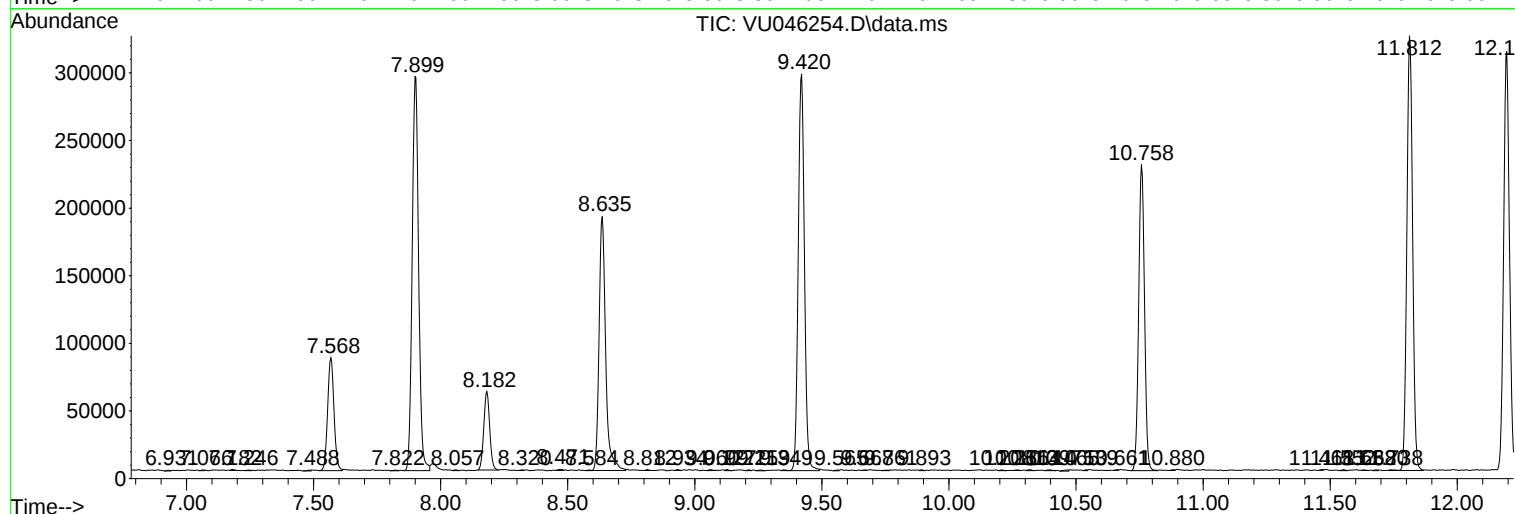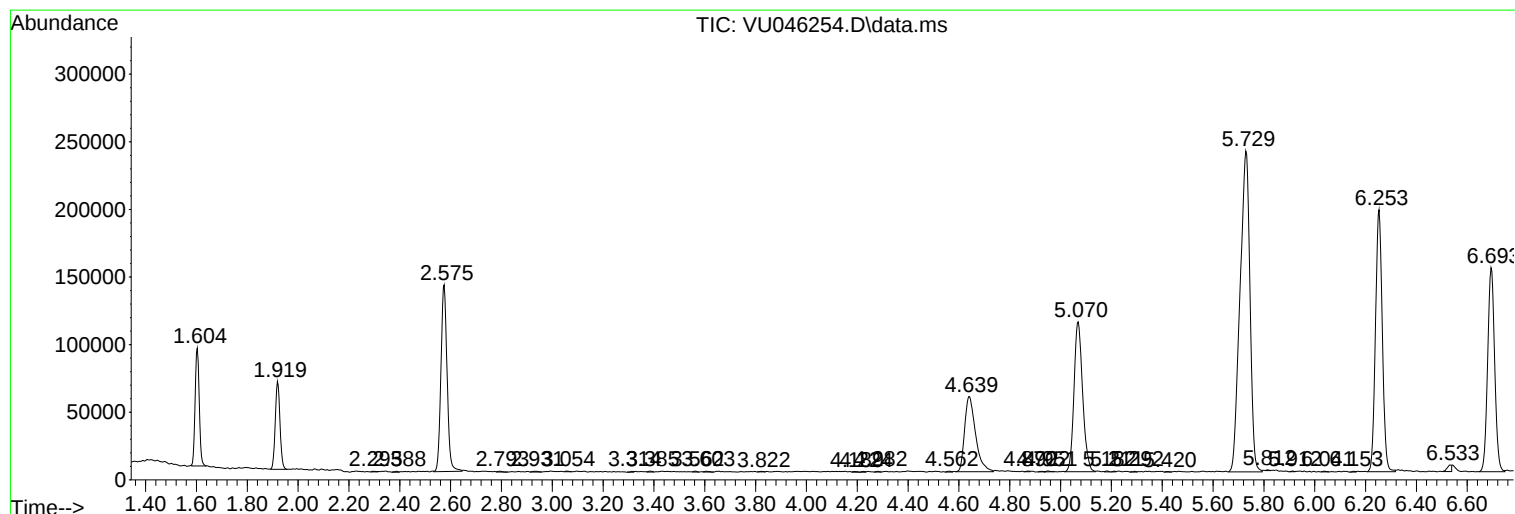

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046254.D
Acq On : 10 Dec 2021 04:24
Operator : SY/MD
Sample : M4982-19
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
Data File : VU046254.D
Acq On : 10 Dec 2021 04:24
Operator : SY/MD
Sample : M4982-19
Misc : 5.6mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CT6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
