


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120921\
 Data File : VU046207.D
 Acq On : 09 Dec 2021 09:11
 Operator : SY/MD
 Sample : BFB027
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB027

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 20 00:25:10 2021

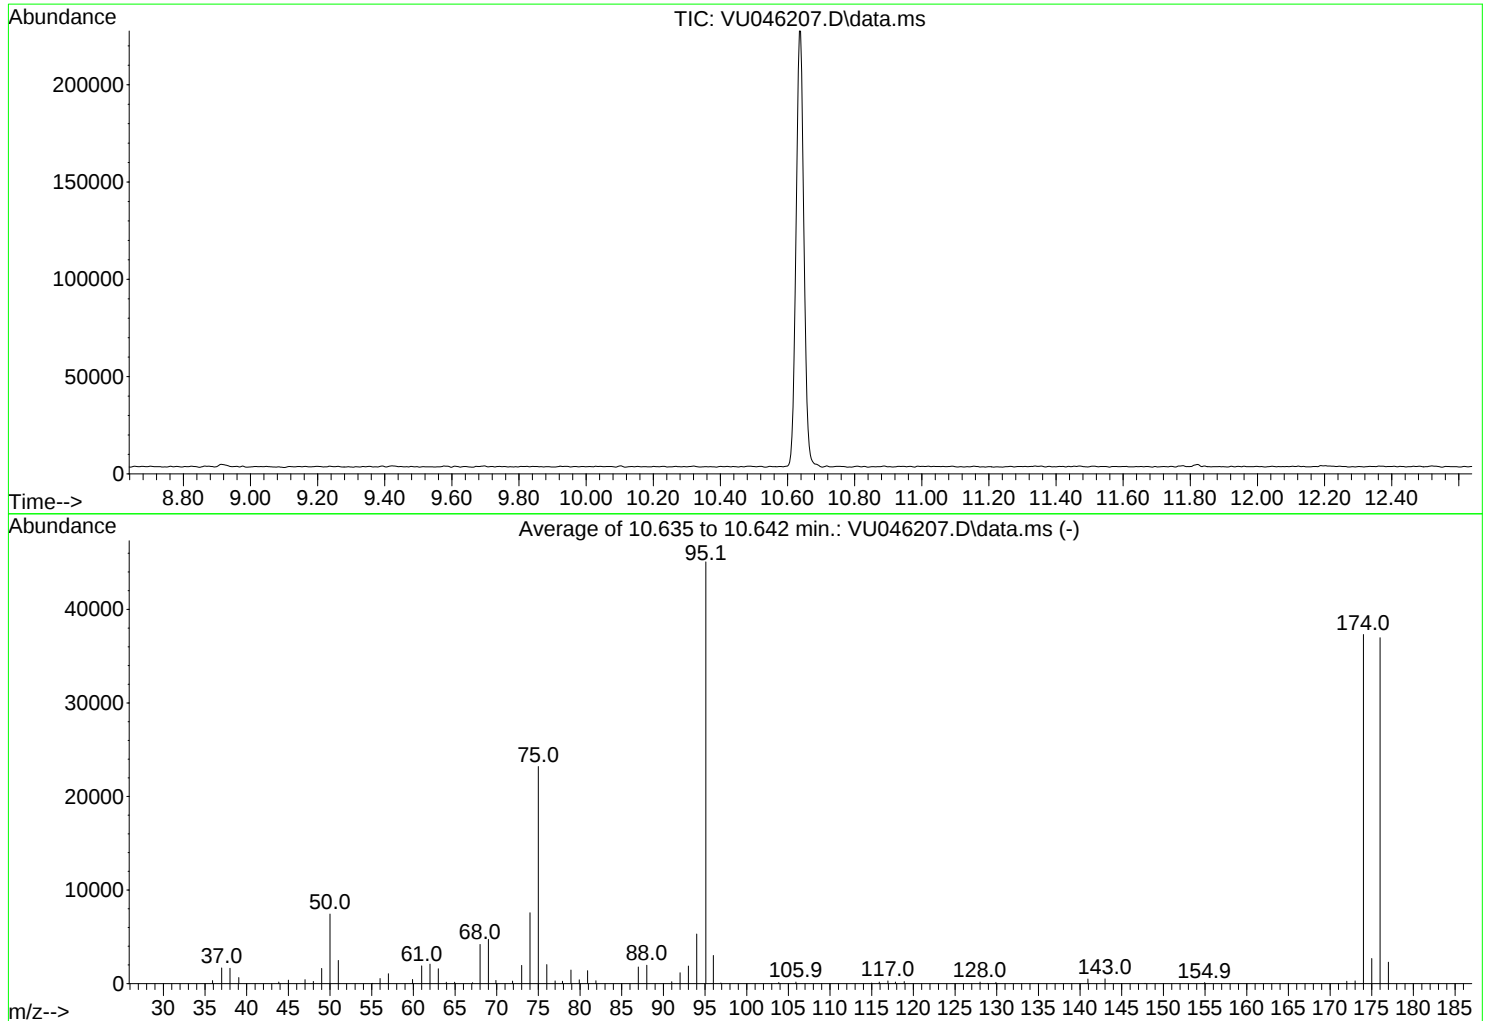

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	7447	PASS
75	95	30	80	51.5	23208	PASS
95	95	100	100	100.0	45080	PASS
96	95	5	9	6.7	3010	PASS
173	174	0.00	2	0.8	286	PASS
174	95	50	120	82.8	37323	PASS
175	174	5	9	7.2	2692	PASS
176	174	95	101	99.0	36965	PASS
177	176	5	9	6.2	2295	PASS

m/z	Abundance
39.90	3705.0
43.80	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	317.0
37.00	1815.0
38.00	1708.0
39.00	697.0
39.90	3680.0
43.90	373.0
45.00	416.0
47.00	470.0
48.00	208.0
49.00	1661.0
50.00	7805.0
51.00	2615.0
56.00	594.0
57.00	1096.0
59.90	423.0
61.00	2113.0
62.00	2274.0
63.00	1629.0
63.90	184.0
65.00	184.0
67.00	106.0
68.00	4431.0
69.00	5058.0
69.90	361.0
71.90	314.0
73.00	2003.0
74.00	8142.0
75.00	24040.0
76.00	2205.0
77.00	349.0
77.90	257.0
78.90	1414.0
79.90	428.0
80.90	1437.0
81.90	316.0
87.00	1898.0
88.00	1993.0
91.00	225.0
92.00	1184.0
93.00	1975.0
94.00	5443.0
95.10	46584.0
96.00	3056.0
96.90	111.0
103.90	116.0
105.90	166.0
115.90	198.0
116.90	298.0
117.80	180.0
118.90	244.0
128.00	186.0
128.90	105.0
129.90	163.0
141.00	535.0
143.00	552.0
147.80	101.0
154.90	110.0
172.00	278.0
173.00	279.0
174.00	38120.0
175.00	2900.0
176.00	37112.0
177.00	2350.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	339.0
37.00	1719.0
38.00	1732.0
39.00	663.0
39.90	3632.0
43.90	393.0
45.00	375.0
47.00	445.0
48.00	241.0
49.00	1681.0
50.00	7677.0
51.00	2574.0
56.00	569.0
57.00	1092.0
59.90	471.0
61.00	1935.0
62.00	2133.0
63.00	1648.0
64.00	149.0
64.90	146.0
67.10	112.0
68.00	4323.0
69.00	4933.0
69.90	355.0
71.90	293.0
73.00	2004.0
74.00	7787.0
75.00	23976.0
76.00	2110.0
77.00	288.0
77.90	280.0
78.90	1524.0
79.90	425.0
80.90	1427.0
81.90	314.0
87.00	1821.0
88.00	2047.0
91.00	212.0
92.00	1188.0
93.00	1929.0
94.00	5541.0
95.10	46624.0
96.00	3139.0
96.90	104.0
103.80	112.0
105.90	184.0
115.00	108.0
115.90	188.0
116.90	283.0
117.90	184.0
118.90	229.0
128.00	177.0
129.90	137.0
141.00	521.0
143.00	533.0
155.00	125.0
172.00	267.0
173.00	294.0
174.00	38424.0
175.00	2754.0
176.00	38216.0
177.00	2357.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	342.0
37.00	1474.0
38.00	1513.0
39.10	585.0
40.00	3548.0
43.90	387.0
45.00	334.0
47.00	371.0
48.00	258.0
49.00	1521.0
50.00	6858.0
51.00	2254.0
55.10	117.0
56.00	503.0
57.00	1001.0
59.90	438.0
61.00	1668.0
62.00	1862.0
63.00	1481.0
64.00	126.0
64.90	118.0
67.20	112.0
68.00	3838.0
69.00	4242.0
69.90	302.0
71.90	233.0
73.00	1862.0
74.00	6790.0
75.00	21608.0
76.00	1821.0
77.00	222.0
77.90	224.0
78.90	1411.0
79.90	401.0
80.90	1296.0
81.90	288.0
87.00	1602.0
88.00	1849.0
91.00	175.0
92.00	1095.0
93.00	1753.0
94.00	4920.0
95.10	42032.0
96.00	2836.0
103.90	131.0
105.90	185.0
115.00	118.0
115.90	158.0
117.00	274.0
117.90	172.0
118.90	215.0
128.00	143.0
129.90	121.0
140.90	426.0
143.00	472.0
155.00	114.0
172.00	224.0
173.00	284.0
174.00	35424.0
175.00	2422.0
176.00	35568.0
177.00	2178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027