


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052329.D
Acq On : 10 Dec 2022 02:26
Operator : JC/MD
Sample : N5979-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0ER9

Manual IntegrationsAPPROVED

Quant Time: Dec 10 03:24:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
Supervised By :Mahesh Dadoda 12/12/2022

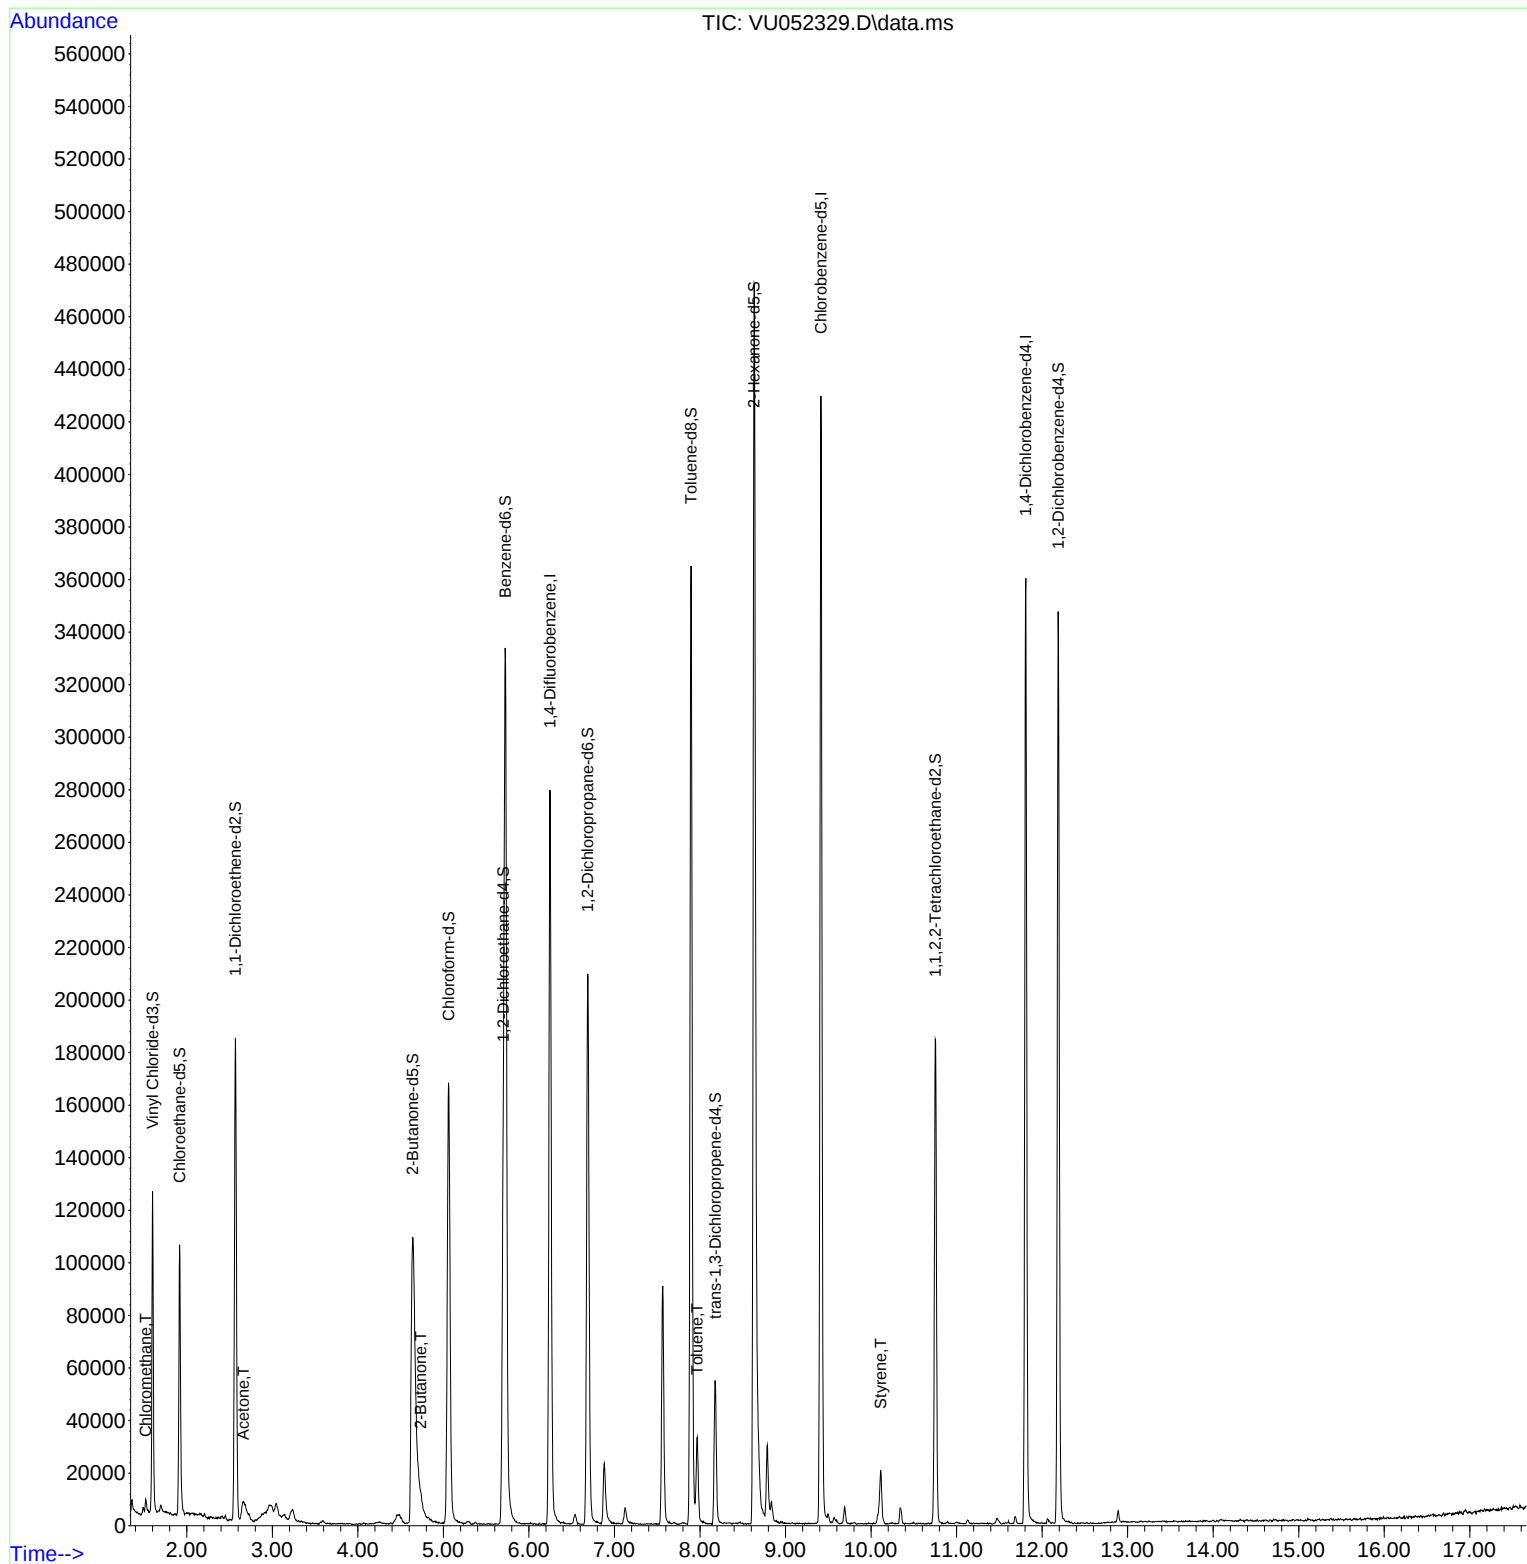




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052329.D
 Acq On : 10 Dec 2022 02:26
 Operator : JC/MD
 Sample : N5979-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ER9

Manual IntegrationsAPPROVED

Quant Time: Dec 10 03:24:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
 Supervised By :Mahesh Dadoda 12/12/2022

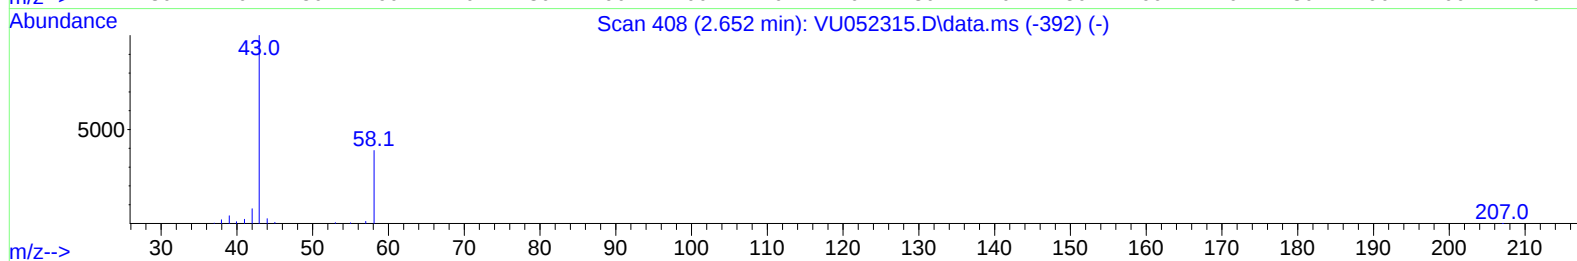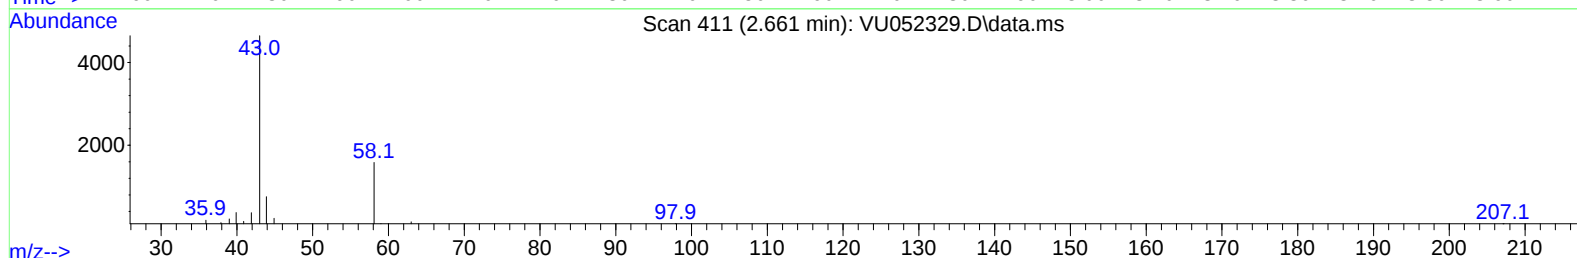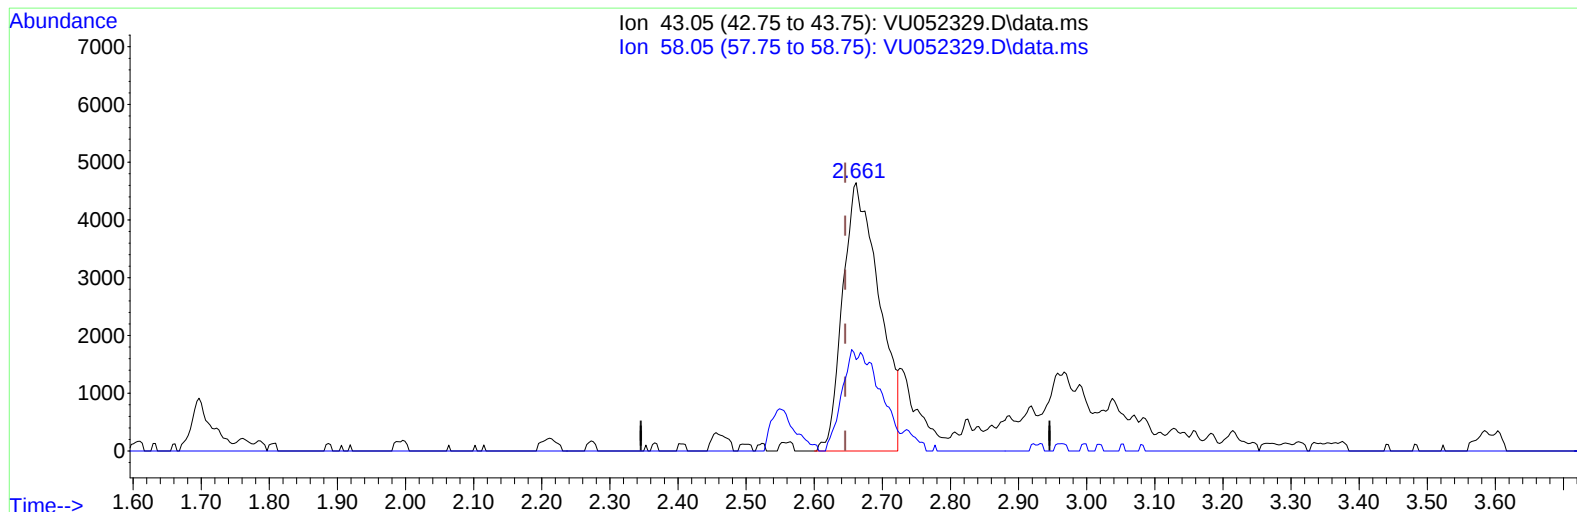

TIC: VU052329.D\data.ms

(13) Acetone (T)

2.661min (+ 0.016) 6.17 ug/L

response 17236

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	15.32
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052329.D
 Acq On : 10 Dec 2022 02:26
 Operator : JC/MD
 Sample : N5979-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ER9

Manual IntegrationsAPPROVED

Quant Time: Dec 10 03:24:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
 Supervised By :Mahesh Dadoda 12/12/2022

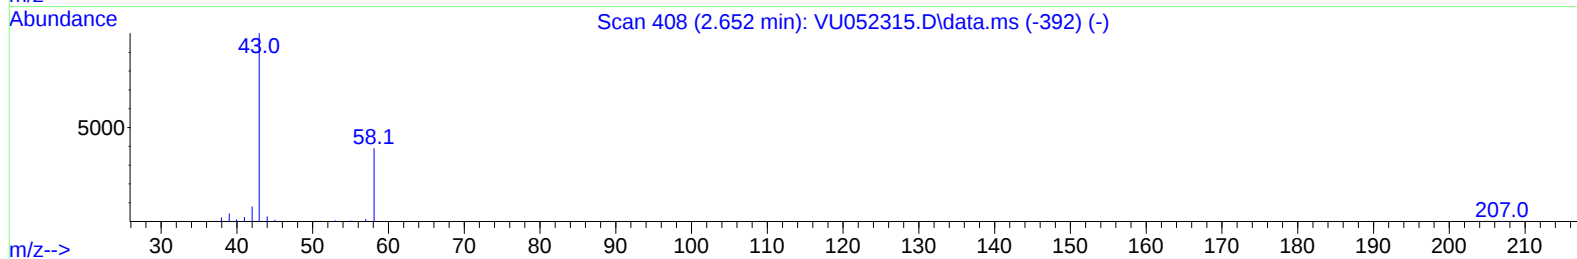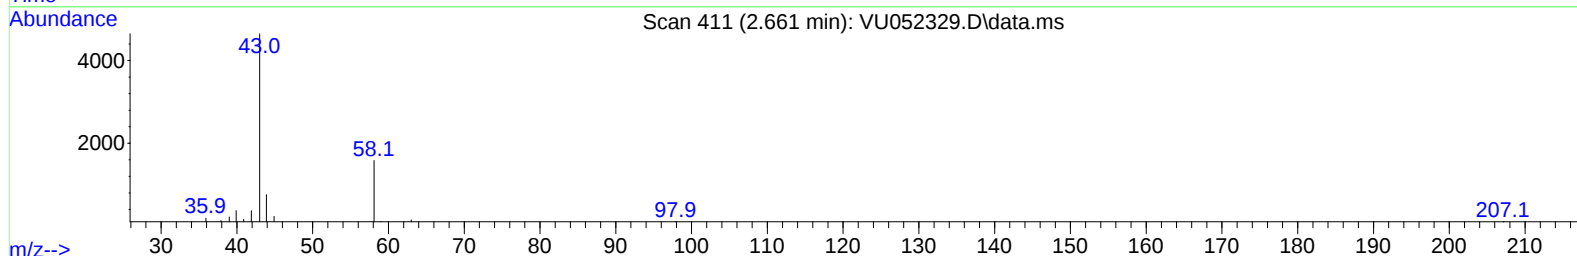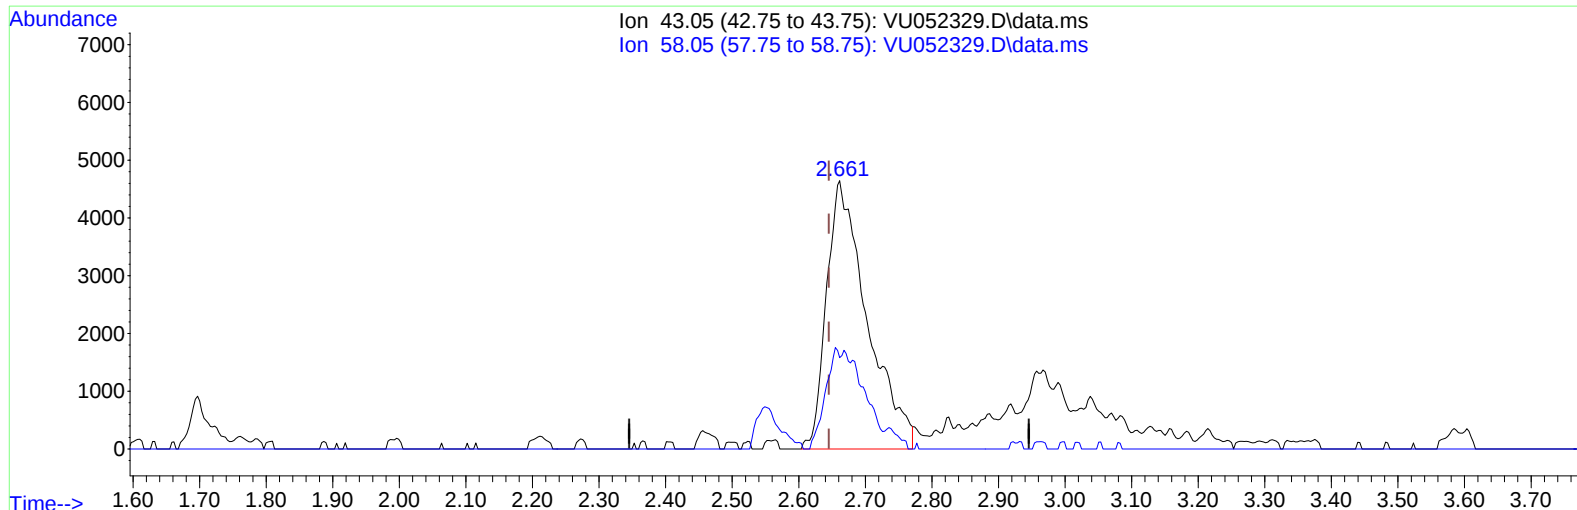

TIC: VU052329.D\data.ms

(13) Acetone (T)

2.661min (+ 0.016) 7.04 ug/L m

response 19651

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	38.00	13.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052329.D
 Acq On : 10 Dec 2022 02:26
 Operator : JC/MD
 Sample : N5979-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0ER9

Manual IntegrationsAPPROVED

Quant Time: Dec 10 03:24:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
 Supervised By :Mahesh Dadoda 12/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	233232	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	244412	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	100098	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	88835	3.916	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.400%	
7) Chloroethane-d5	1.916	69	79474	4.510	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.200%	
11) 1,1-Dichloroethene-d2	2.568	65	34247	4.211	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	84.200%	
20) 2-Butanone-d5	4.642	46	237615	57.783	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.560%	
24) Chloroform-d	5.060	84	162749	4.882	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.700	65	85973	5.106	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.200%	
32) Benzene-d6	5.726	84	328122	4.522	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	6.687	67	110068	4.902	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.000%	
41) Toluene-d8	7.896	98	257144	3.917	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.400%	
43) trans-1,3-Dichloroprop...	8.179	79	33070	4.041	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	80.800%	
46) 2-Hexanone-d5	8.632	63	161187	46.479	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	92.960%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	96369	4.950	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.000%	
66) 1,2-Dichlorobenzene-d4	12.188	152	94749	4.944	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	98.800%	
Target Compounds						
3) Chloromethane	1.520	50	3199	0.121	ug/L	89
13) Acetone	2.661	43	19651m	7.037	ug/L	
21) 2-Butanone	4.732	43	9327m	2.084	ug/L	
42) Toluene	7.967	91	23431	0.286	ug/L	96
55) Styrene	10.111	104	9957	0.200	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed