

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052296.D
 Acq On : 09 Dec 2022 13:02
 Operator : JC/MD
 Sample : N5916-13DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5N31DL

Quant Time: Dec 09 23:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	246442	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	247926	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	97434	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	69532	2.901	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	58.000%	
7) Chloroethane-d5	1.916	69	64426	3.460	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	69.200%	
11) 1,1-Dichloroethene-d2	2.569	65	29597	3.444	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	4.636	46	231670	53.317	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	106.640%	
24) Chloroform-d	5.061	84	146428	4.157	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.200%	
26) 1,2-Dichloroethane-d4	5.700	65	76265	4.287	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
32) Benzene-d6	5.726	84	283399	3.850	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.000%	
36) 1,2-Dichloropropane-d6	6.688	67	99650	4.375	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.400%	
41) Toluene-d8	7.897	98	213642	3.208	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	64.200%#	
43) trans-1,3-Dichloroprop...	8.176	79	29830	3.594	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	71.800%	
46) 2-Hexanone-d5	8.633	63	155649	44.246	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.500%	
56) 1,1,2,2-Tetrachloroeth...	10.752	84	89008	4.507	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.200%	
66) 1,2-Dichlorobenzene-d4	12.189	152	80824	4.333	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	86.600%	
Target Compounds						
16) Methylene chloride	3.048	84	13715	0.567	ug/L	92
27) 1,2-Dichloroethane	5.790	62	114626	5.347	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052296.D
Acq On : 09 Dec 2022 13:02
Operator : JC/MD
Sample : N5916-13DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5N31DL

Quant Time: Dec 09 23:11:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration




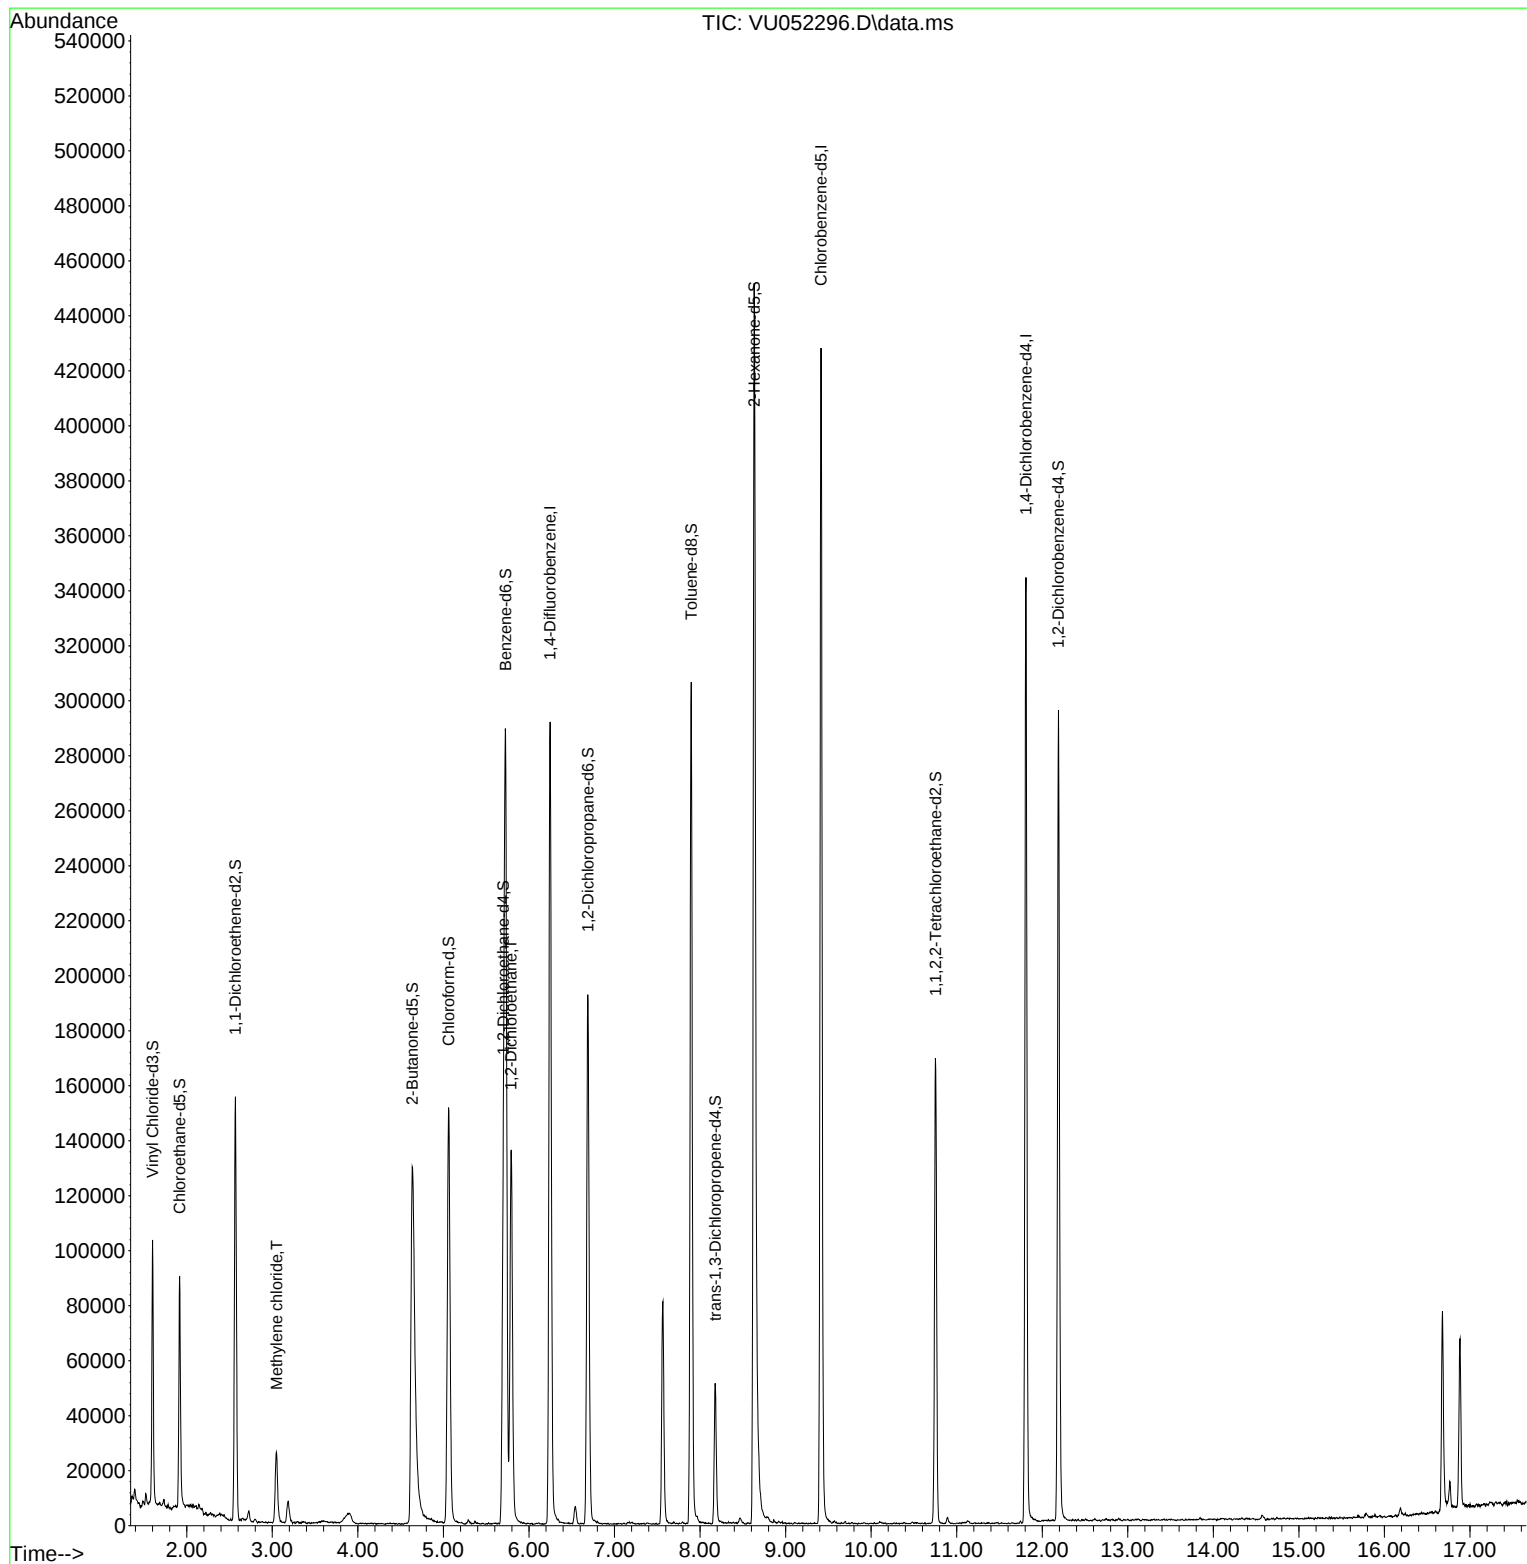


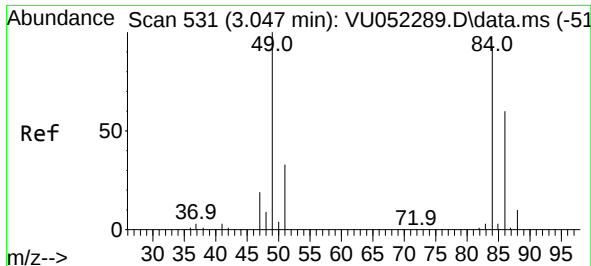

#16
Methylene chloride
Concen: 0.567 ug/L
RT: 3.048 min Scan# 51
Delta R.T. 0.000 min
Lab File: VU052296.D
Acq: 09 Dec 2022 13:02

Instrument :
MSVOA_U
ClientSampleId :
F5N31DL

Tgt Ion: 84 Resp: 13715
Ion Ratio Lower Upper
84 100
86 67.0 43.8 81.4
49 118.0 75.9 141.1

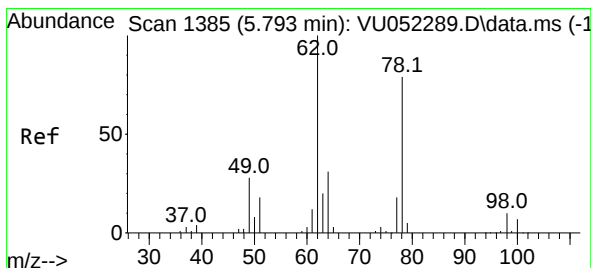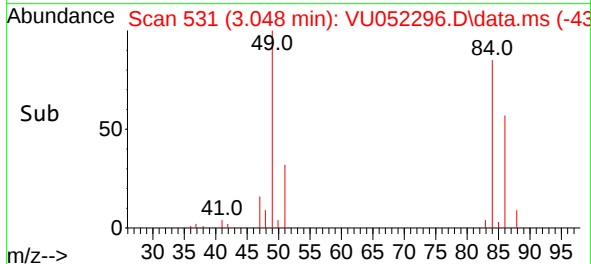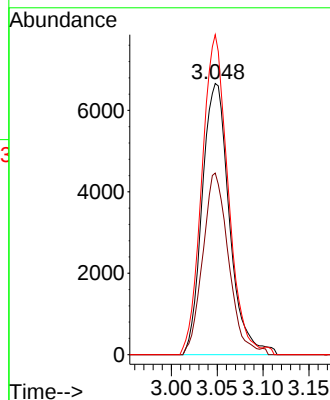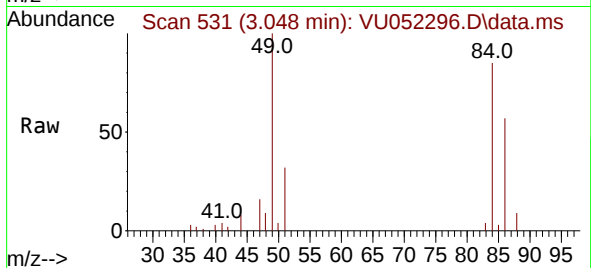

#27
1,2-Dichloroethane
Concen: 5.347 ug/L
RT: 5.790 min Scan# 1384
Delta R.T. -0.003 min
Lab File: VU052296.D
Acq: 09 Dec 2022 13:02

Tgt Ion: 62 Resp: 114626
Ion Ratio Lower Upper
62 100
98 10.6 8.4 12.6

