

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052301.D
 Acq On : 09 Dec 2022 15:02
 Operator : JC/MD
 Sample : N5958-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EN2

Quant Time: Dec 09 23:12:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 08 04:19:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	207560	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	208862	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	80855	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	69540	3.444	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.800%
7) Chloroethane-d5	1.916	69	66976	4.271	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.400%
11) 1,1-Dichloroethene-d2	2.568	65	29733	4.109	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%
20) 2-Butanone-d5	4.633	46	242765	66.337	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.680%#
24) Chloroform-d	5.060	84	150994	5.090	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
26) 1,2-Dichloroethane-d4	5.700	65	80269	5.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.200%
32) Benzene-d6	5.726	84	295709	4.769	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.687	67	103582	5.398	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.000%
41) Toluene-d8	7.896	98	219747	3.917	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.400%
43) trans-1,3-Dichloroprop...	8.176	79	31518	4.507	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.200%
46) 2-Hexanone-d5	8.632	63	165451	55.829	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.660%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	93815	5.639	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	112.800%
66) 1,2-Dichlorobenzene-d4	12.189	152	83106	5.369	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.400%
Target Compounds					Qvalue	
13) Acetone	2.655	43	6817	2.743	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052301.D
Acq On : 09 Dec 2022 15:02
Operator : JC/MD
Sample : N5958-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0EN2

Quant Time: Dec 09 23:12:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 08 04:19:43 2022
Response via : Initial Calibration

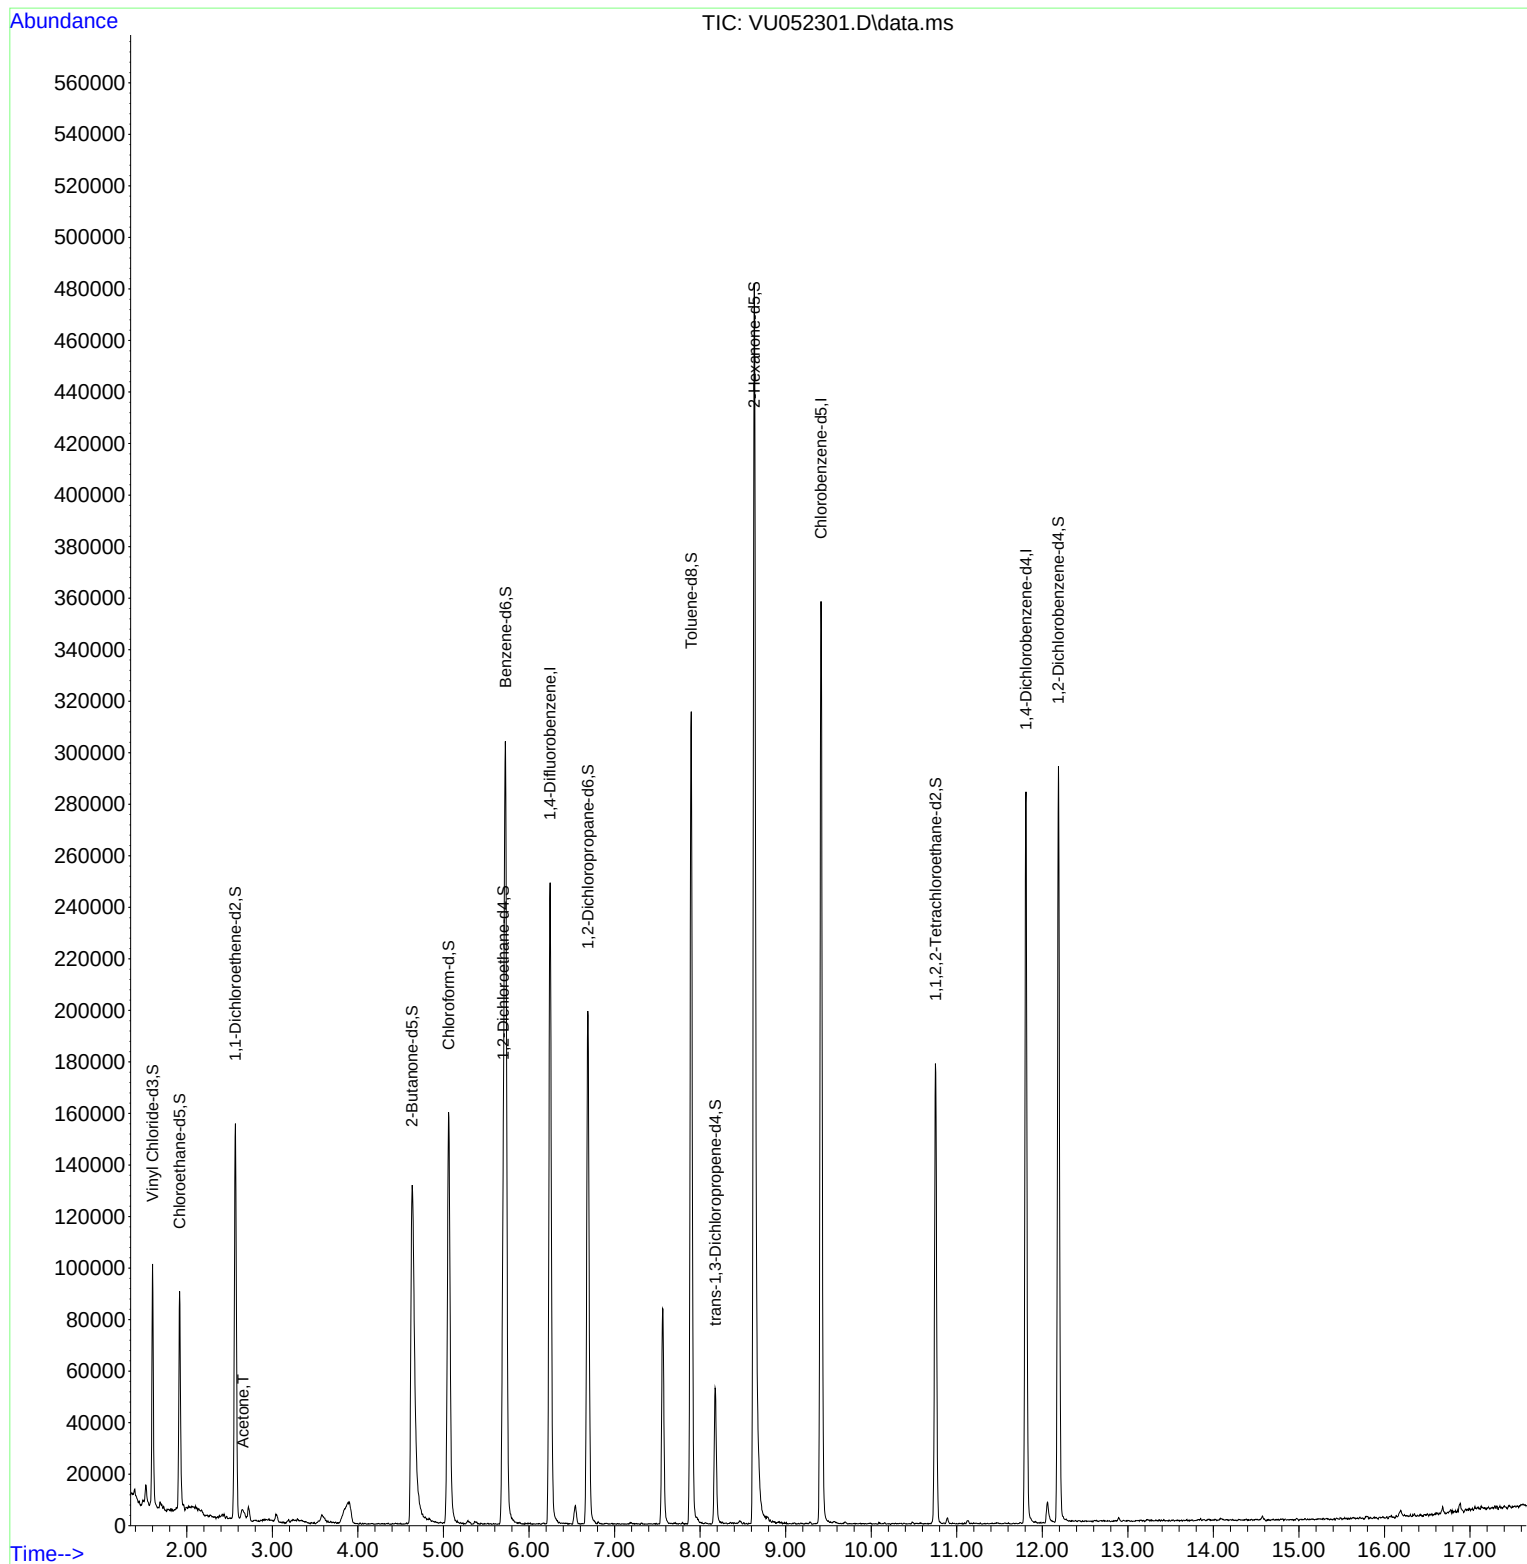

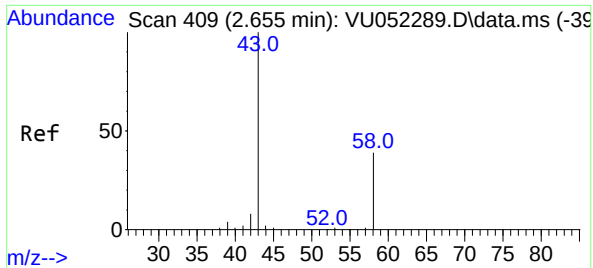

#13
 Acetone
 Concen: 2.743 ug/L
 RT: 2.655 min Scan# 409
 Delta R.T. 0.010 min
 Lab File: VU052301.D
 Acq: 09 Dec 2022 15:02

Instrument :
 MSVOA_U
 ClientSampleId :
 C0EN2

Tgt Ion: 43 Resp: 6817
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 76.0

