

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052290.D
 Acq On : 09 Dec 2022 10:31
 Operator : JC/MD
 Sample : VU1209WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK155

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052290.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	104475	119761	13.08%	1.806%
2	1.916	171	179	197	rVB	90882	123244	13.46%	1.859%
3	2.568	369	382	398	rBV	163443	268618	29.35%	4.052%
4	3.047	521	531	545	rBV2	8778	16524	1.81%	0.249%
5	3.186	559	574	588	rBV	12088	26037	2.84%	0.393%
6	4.639	1011	1026	1081	rBV2	126442	456855	49.91%	6.891%
7	5.060	1140	1157	1182	rBV2	158621	356391	38.94%	5.375%
8	5.723	1342	1363	1388	rBV3	309252	810347	88.53%	12.223%
9	6.247	1512	1526	1553	rBV	250760	484383	52.92%	7.306%
10	6.539	1603	1617	1632	rBV5	21706	42830	4.68%	0.646%
11	6.687	1649	1663	1687	rBV	200933	399135	43.61%	6.020%
12	7.565	1921	1936	1956	rBV2	78241	141791	15.49%	2.139%
13	7.896	2025	2039	2069	rBV	319923	564195	61.64%	8.510%
14	8.176	2114	2126	2144	rBV2	48204	85823	9.38%	1.294%
15	8.636	2256	2269	2301	rBV2	443615	915332	100.00%	13.806%
16	9.414	2498	2511	2539	rBV	360729	613390	67.01%	9.252%
17	10.751	2912	2927	2945	rBV	173885	283544	30.98%	4.277%
18	11.809	3243	3256	3271	rBV	285510	454801	49.69%	6.860%
19	12.188	3362	3374	3399	rBV	279372	466925	51.01%	7.043%




Sum of corrected areas: 6629926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052290.D
Acq On : 09 Dec 2022 10:31
Operator : JC/MD
Sample : VU1209WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

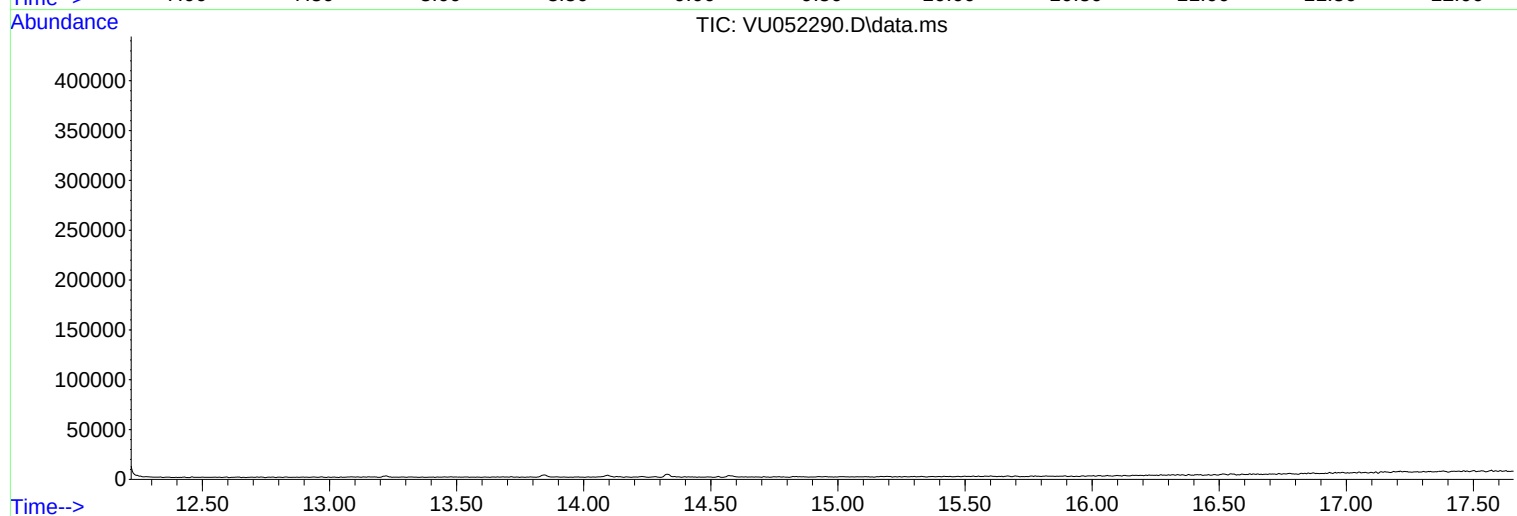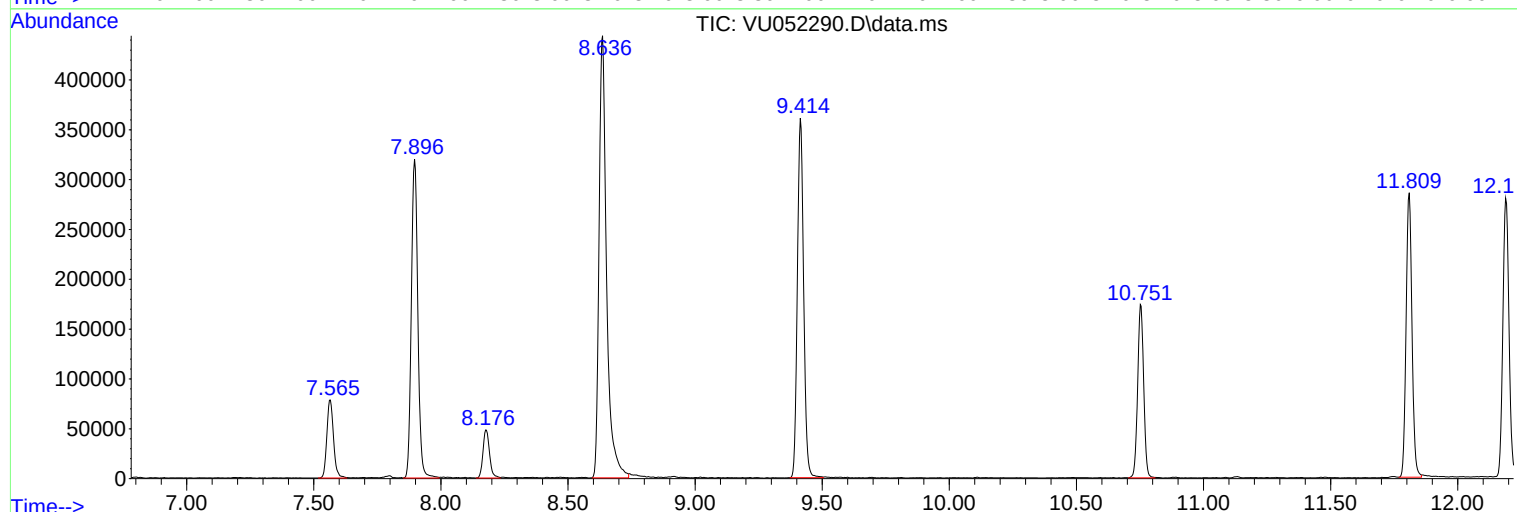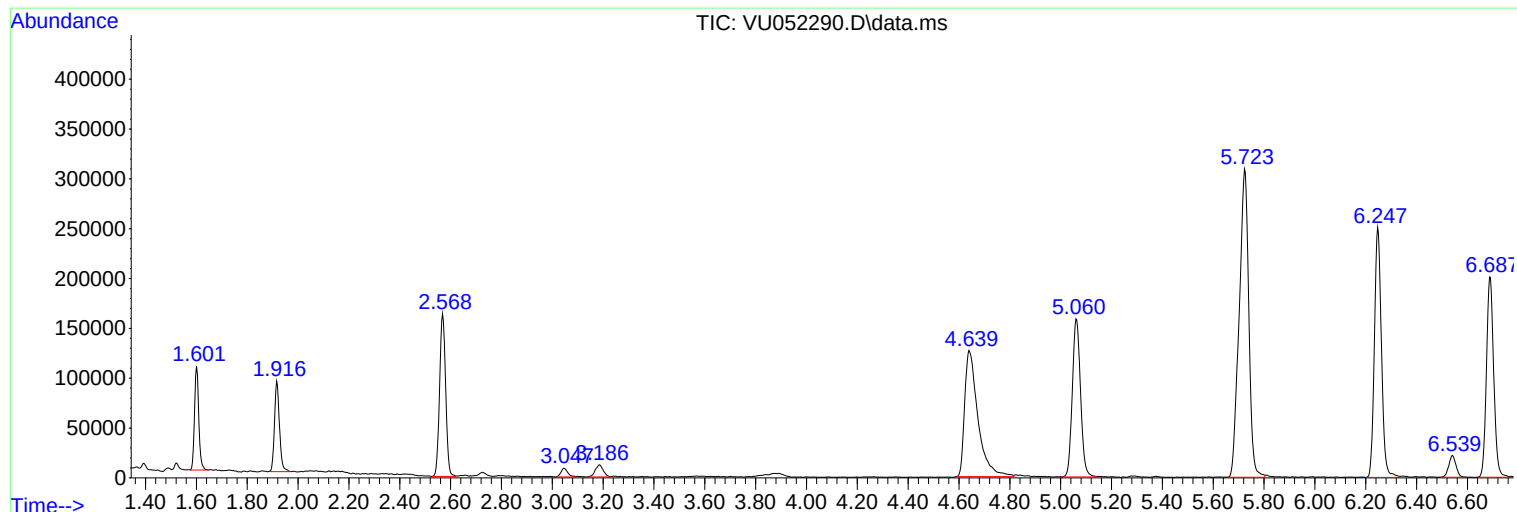

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052290.D
Acq On : 09 Dec 2022 10:31
Operator : JC/MD
Sample : VU1209WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052290.D
Acq On : 09 Dec 2022 10:31
Operator : JC/MD
Sample : VU1209WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK155

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc