

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052305.D
 Acq On : 09 Dec 2022 16:39
 Operator : JC/MD
 Sample : N5960-03DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L26DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	93	rVB	97737	113570	11.70%	1.532%
2	1.916	170	179	197	rBV	89284	120370	12.41%	1.623%
3	2.568	370	382	397	rBV	162833	262955	27.10%	3.546%
4	3.047	519	531	548	rVB3	16923	33418	3.44%	0.451%
5	3.186	559	574	587	rBV2	16329	39197	4.04%	0.529%
6	4.645	1004	1028	1072	rBV3	142941	584377	60.23%	7.881%
7	5.060	1137	1157	1178	rBV2	159613	351357	36.21%	4.738%
8	5.722	1342	1363	1387	rBV2	304381	809706	83.45%	10.920%
9	6.247	1511	1526	1549	rBV	262974	510211	52.58%	6.881%
10	6.539	1604	1617	1638	rBV	279489	533210	54.95%	7.191%
11	6.687	1649	1663	1683	rBV	196395	390588	40.25%	5.267%
12	7.565	1924	1936	1955	rBV	81277	147673	15.22%	1.991%
13	7.896	2025	2039	2055	rBV	319341	553219	57.02%	7.461%
14	8.179	2114	2127	2144	rBV2	51712	91414	9.42%	1.233%
15	8.636	2256	2269	2301	rBV2	465639	970287	100.00%	13.085%
16	9.414	2498	2511	2531	rBV	373664	638809	65.84%	8.615%
17	10.751	2913	2927	2951	rBV	179485	290925	29.98%	3.923%
18	11.809	3242	3256	3274	rBV	302033	490015	50.50%	6.608%
19	12.188	3361	3374	3398	rBV	292810	483921	49.87%	6.526%




Sum of corrected areas: 7415222

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052305.D
Acq On : 09 Dec 2022 16:39
Operator : JC/MD
Sample : N5960-03DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

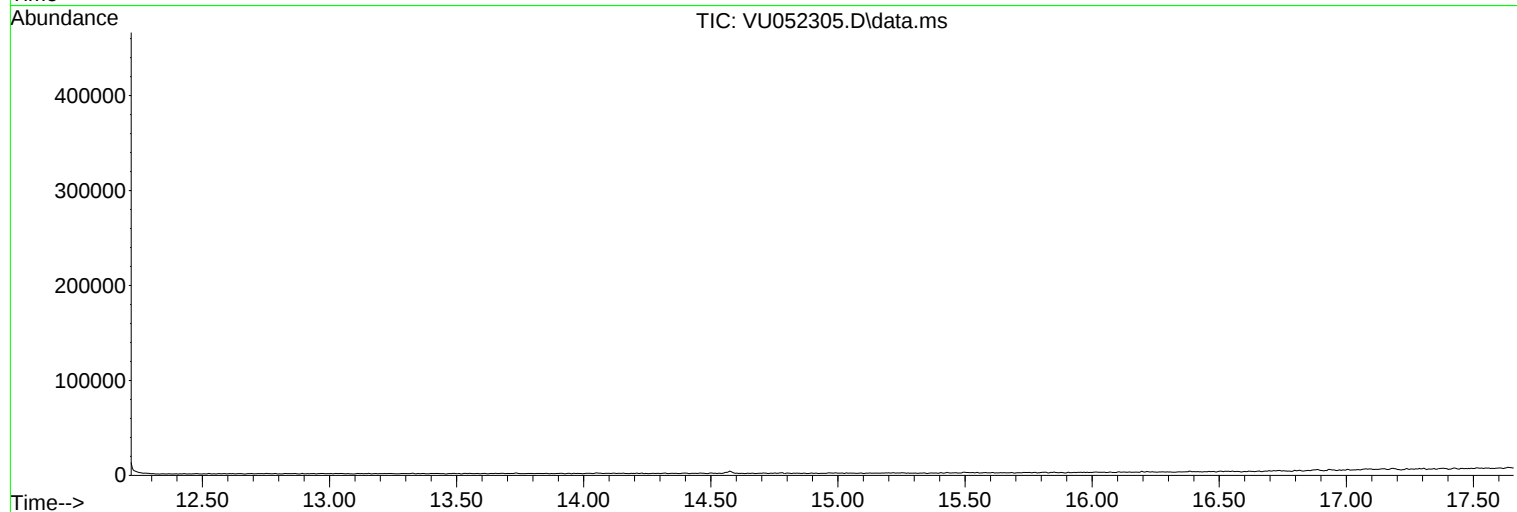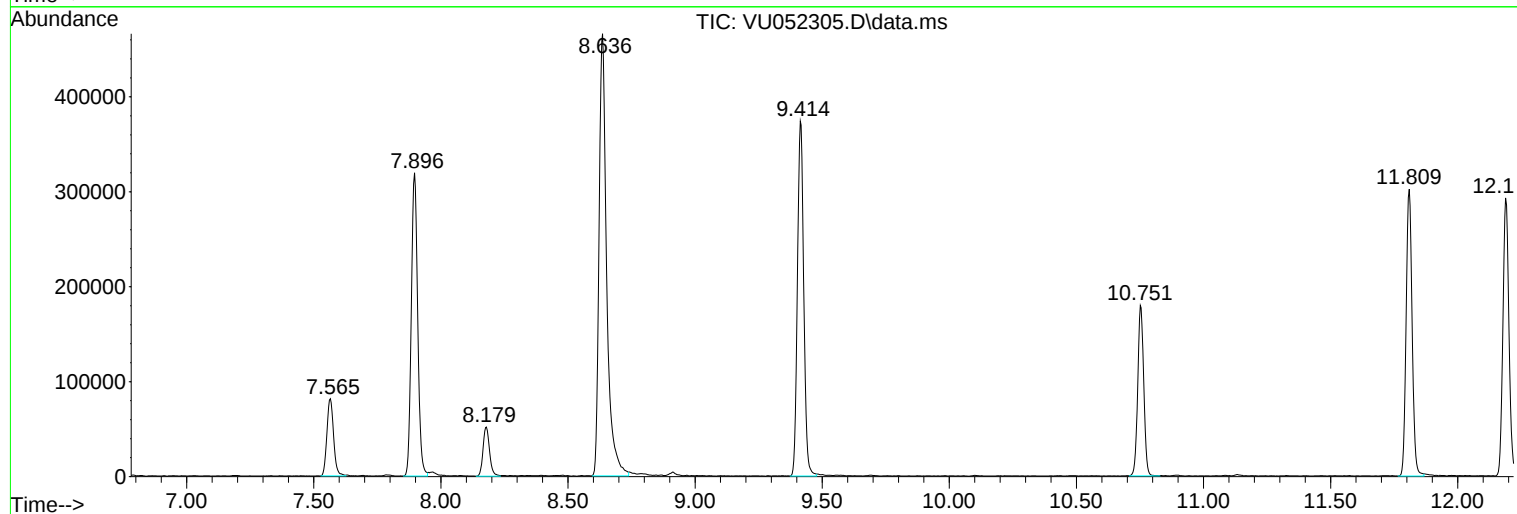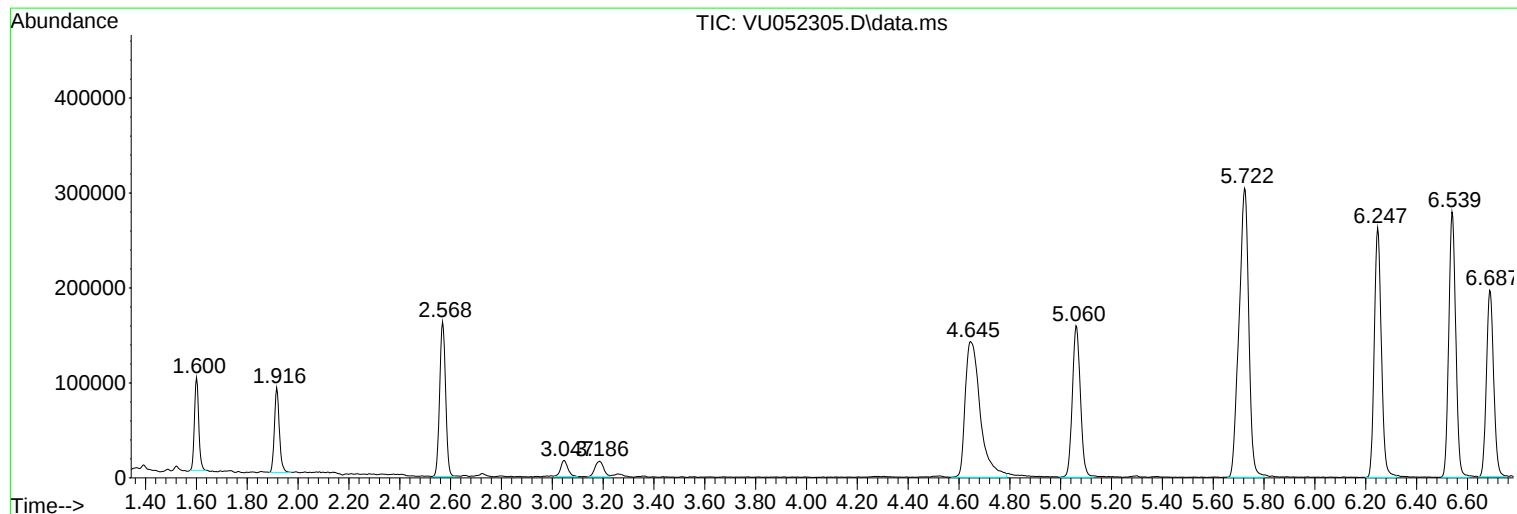

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052305.D
Acq On : 09 Dec 2022 16:39
Operator : JC/MD
Sample : N5960-03DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052305.D
Acq On : 09 Dec 2022 16:39
Operator : JC/MD
Sample : N5960-03DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc