

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052306.D
 Acq On : 09 Dec 2022 17:02
 Operator : JC/MD
 Sample : N5960-04DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L27DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	12	16	33	rVB	7685	10733	1.11%	0.145%
2	1.601	73	81	94	rVB	88470	103949	10.71%	1.409%
3	1.916	170	179	195	rBV	85229	119197	12.28%	1.615%
4	2.568	370	382	402	rVB	149446	244376	25.17%	3.312%
5	3.044	520	530	552	rVB2	17433	35631	3.67%	0.483%
6	3.183	558	573	585	rBV	15442	35168	3.62%	0.477%
7	4.646	1006	1028	1066	rBV	140335	552897	56.94%	7.492%
8	5.060	1140	1157	1177	rBV	153582	339809	35.00%	4.605%
9	5.723	1342	1363	1389	rBV3	294933	786092	80.96%	10.653%
10	6.247	1510	1526	1549	rBV	255952	497974	51.28%	6.748%
11	6.539	1603	1617	1646	rBV	304731	575027	59.22%	7.792%
12	6.687	1650	1663	1684	rBV	196346	389879	40.15%	5.283%
13	7.562	1924	1935	1961	rBV	82437	150688	15.52%	2.042%
14	7.896	2025	2039	2061	rBV	309763	543358	55.96%	7.363%
15	8.176	2113	2126	2143	rBV2	52117	90994	9.37%	1.233%
16	8.636	2253	2269	2296	rBV2	466160	971010	100.00%	13.158%
17	9.414	2499	2511	2535	rBV	382957	638136	65.72%	8.648%
18	10.751	2910	2927	2945	rBV	180582	294833	30.36%	3.995%
19	11.809	3243	3256	3272	rBV	317147	508481	52.37%	6.891%
20	12.189	3359	3374	3395	rBV	294135	491181	50.58%	6.656%




Sum of corrected areas: 7379413

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052306.D
Acq On : 09 Dec 2022 17:02
Operator : JC/MD
Sample : N5960-04DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

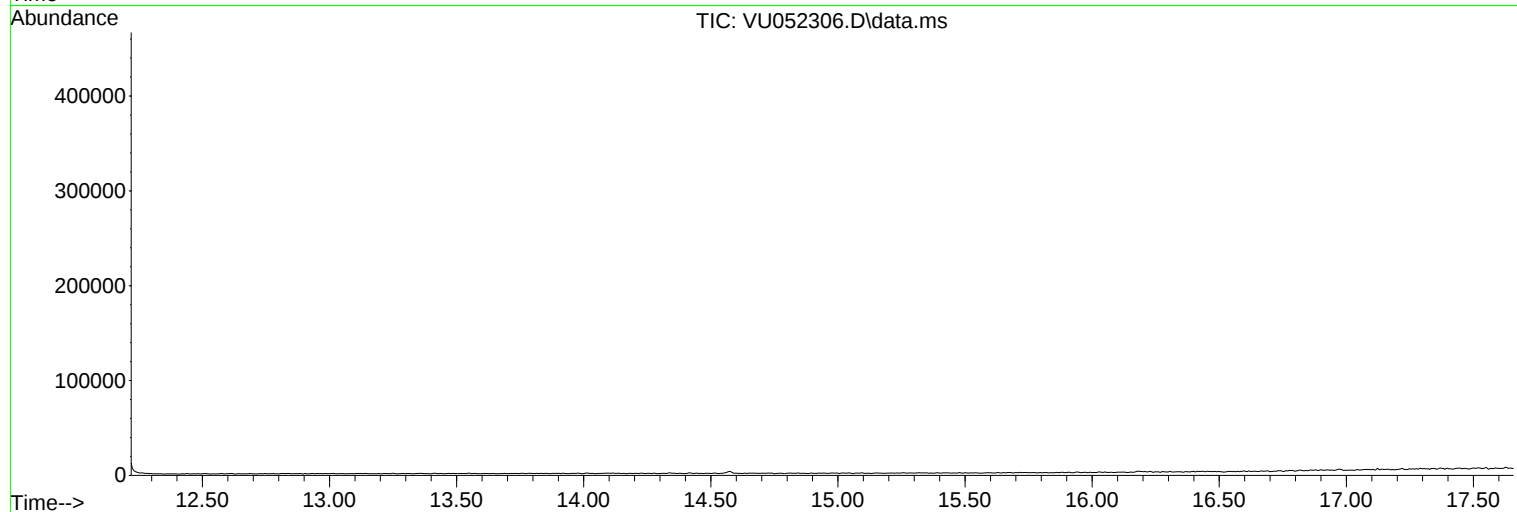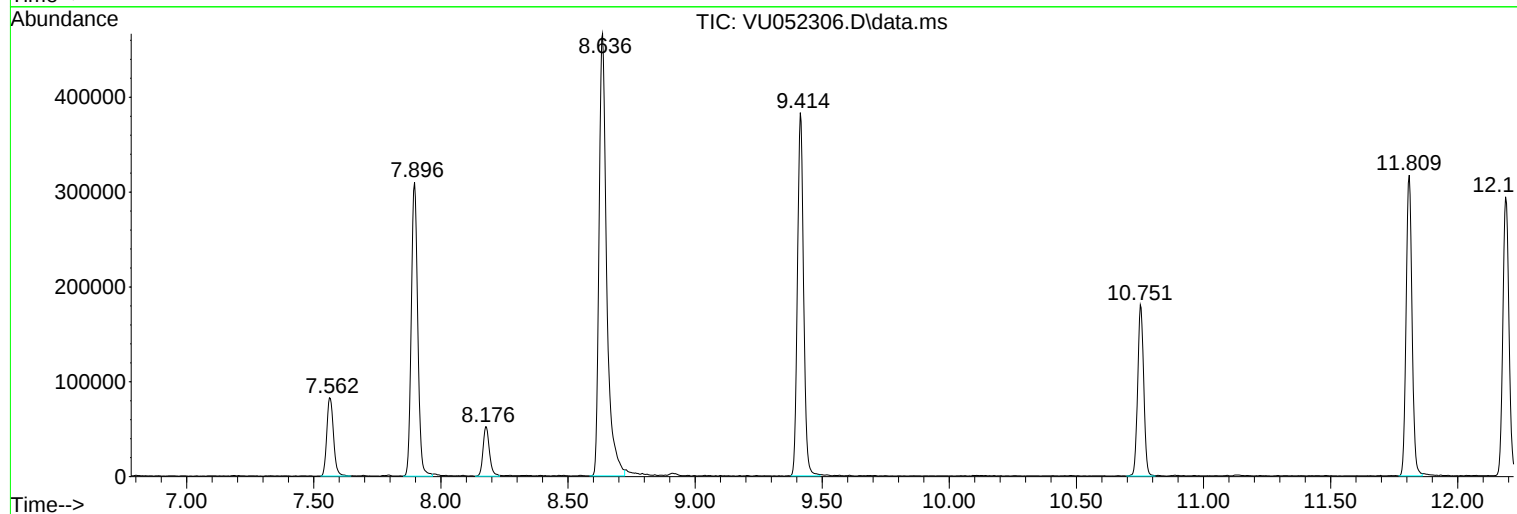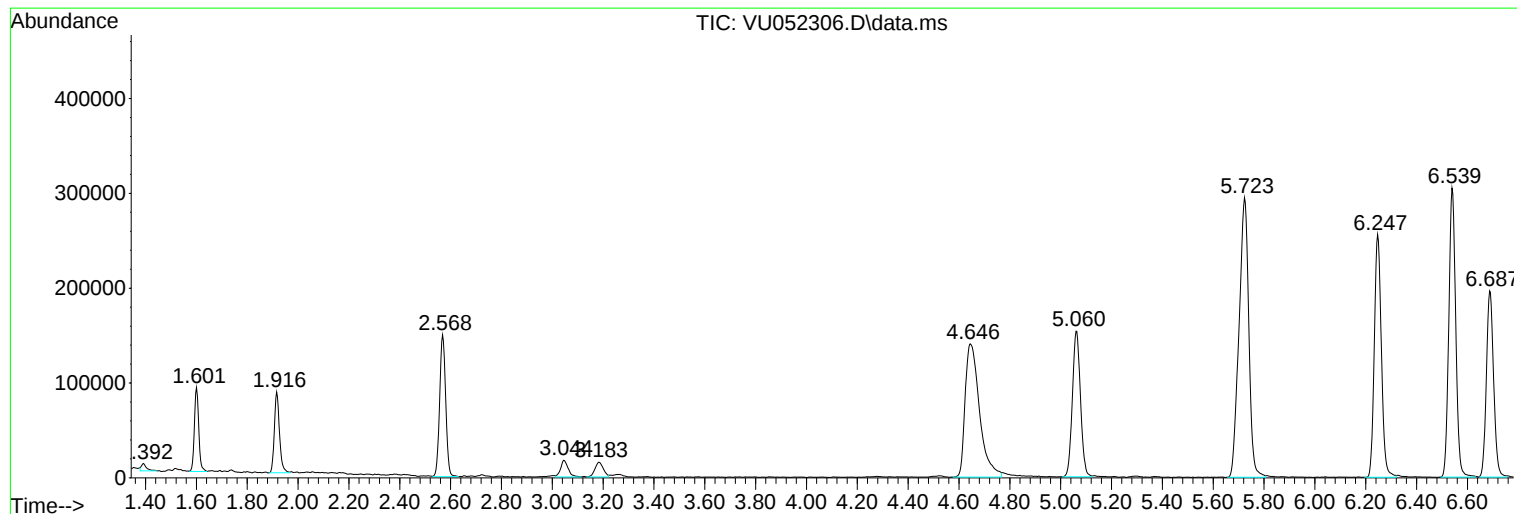

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052306.D
Acq On : 09 Dec 2022 17:02
Operator : JC/MD
Sample : N5960-04DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052306.D
Acq On : 09 Dec 2022 17:02
Operator : JC/MD
Sample : N5960-04DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc