

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052309.D
 Acq On : 09 Dec 2022 18:13
 Operator : JC/MD
 Sample : N5960-02DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L25DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB	170939	203662	7.92%	1.742%
2	1.916	169	179	194	rBV	124058	169254	6.58%	1.448%
3	2.568	369	382	400	rBV	246823	406915	15.83%	3.481%
4	3.044	519	530	550	rVB2	19604	39289	1.53%	0.336%
5	3.186	560	574	584	rBV2	10828	25795	1.00%	0.221%
6	4.658	1006	1032	1074	rBV3	233195	864493	33.62%	7.395%
7	5.060	1141	1157	1179	rBV2	198959	440270	17.12%	3.766%
8	5.723	1342	1363	1394	rBV2	406405	1064824	41.42%	9.108%
9	6.247	1511	1526	1550	rBV	330074	636542	24.76%	5.445%
10	6.539	1601	1617	1650	rBV	1363641	2571069	100.00%	21.992%
11	6.687	1650	1663	1692	rVB	261238	518788	20.18%	4.438%
12	7.565	1923	1936	1956	rBV	110831	199428	7.76%	1.706%
13	7.896	2024	2039	2072	rBV	466376	822666	32.00%	7.037%
14	8.176	2113	2126	2146	rBV	67964	118426	4.61%	1.013%
15	8.636	2253	2269	2304	rBV2	553574	1139657	44.33%	9.748%
16	9.414	2498	2511	2530	rBV	490638	807859	31.42%	6.910%
17	10.751	2912	2927	2949	rBV	213677	352133	13.70%	3.012%
18	11.809	3243	3256	3279	rBV	403054	644677	25.07%	5.514%
19	12.189	3361	3374	3392	rBV	402161	665012	25.87%	5.688%




Sum of corrected areas: 11690759

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052309.D
Acq On : 09 Dec 2022 18:13
Operator : JC/MD
Sample : N5960-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

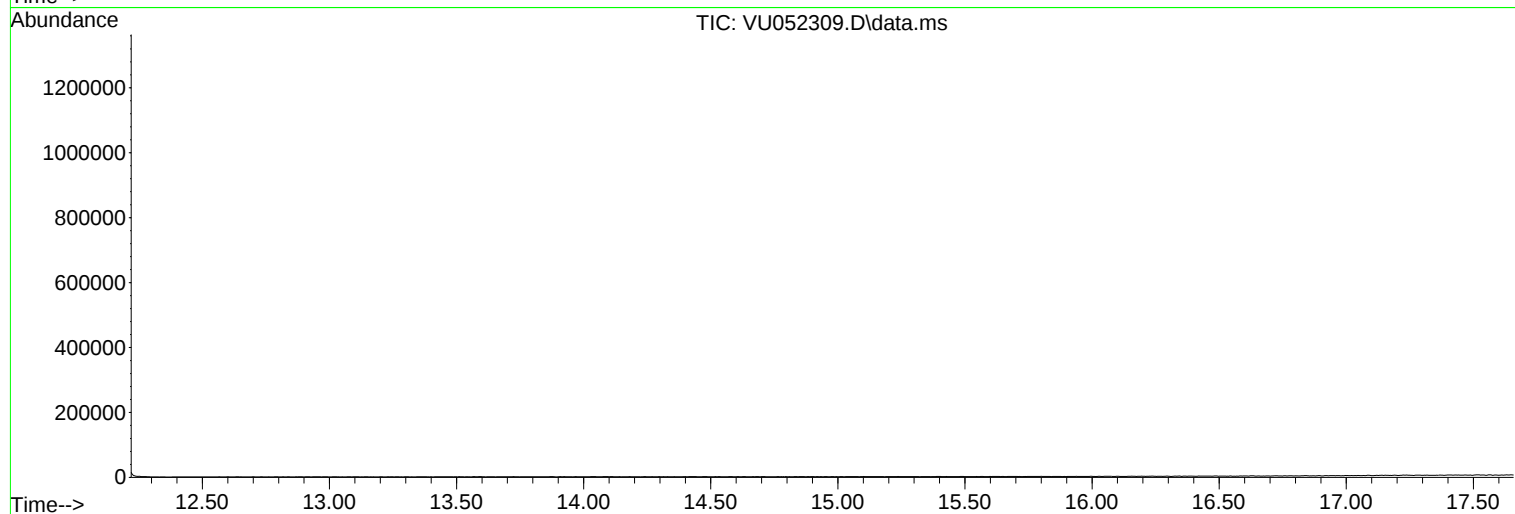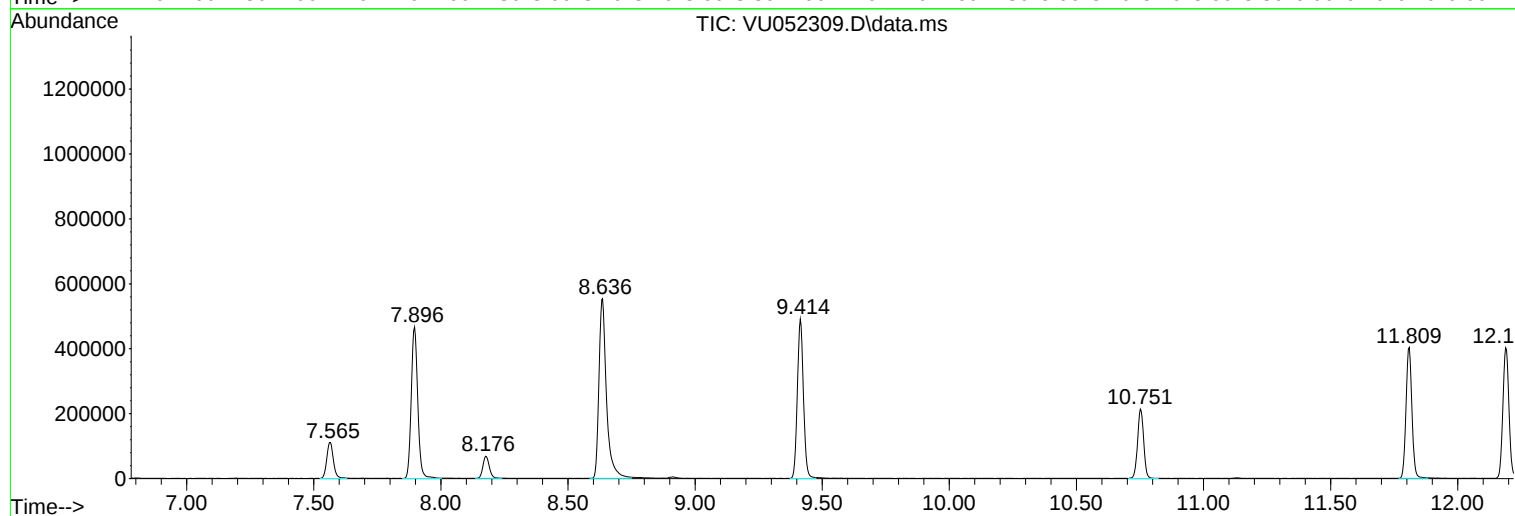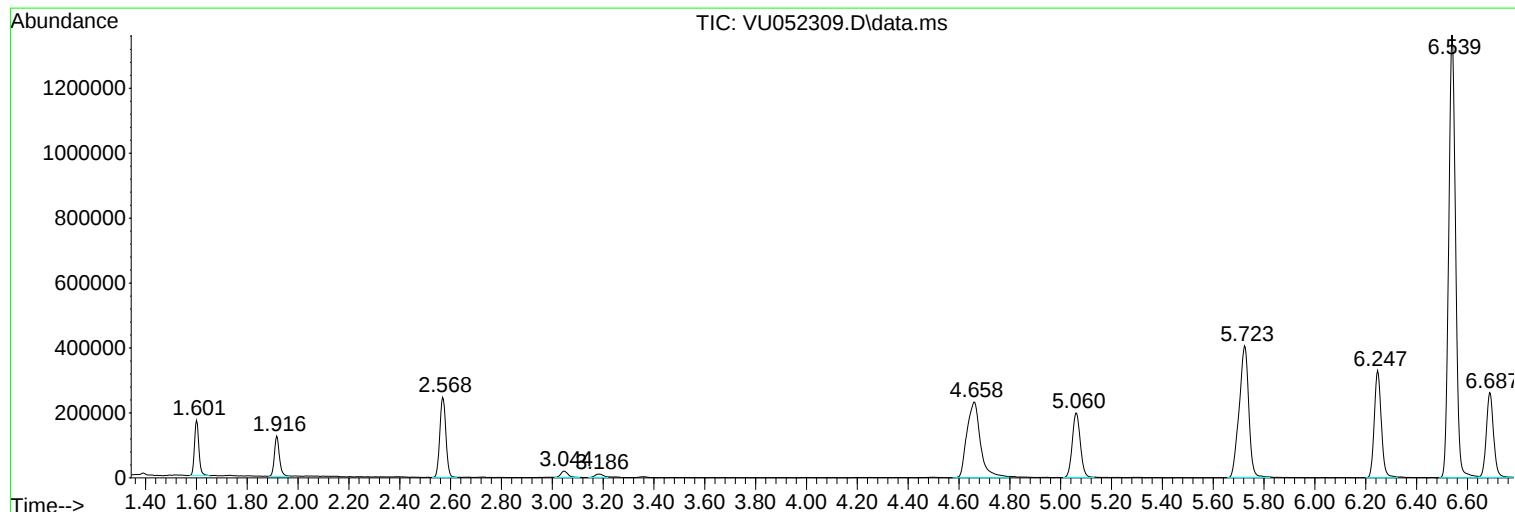

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052309.D
Acq On : 09 Dec 2022 18:13
Operator : JC/MD
Sample : N5960-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052309.D
Acq On : 09 Dec 2022 18:13
Operator : JC/MD
Sample : N5960-02DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc