

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052310.D
 Acq On : 09 Dec 2022 18:36
 Operator : JC/MD
 Sample : N5949-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZA2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rVB	87277	102845	10.75%	1.610%
2	1.916	171	179	192	rBV	79802	107592	11.25%	1.685%
3	2.568	370	382	399	rBV	140941	228063	23.84%	3.571%
4	3.237	575	590	605	rVB	5269	14796	1.55%	0.232%
5	3.871	773	787	801	rBV2	6293	13981	1.46%	0.219%
6	4.642	1010	1027	1070	rBV	119384	425082	44.44%	6.656%
7	5.060	1140	1157	1180	rBV	145140	324031	33.87%	5.074%
8	5.723	1341	1363	1393	rBV2	280635	752466	78.66%	11.782%
9	6.247	1513	1526	1558	rBV	239717	466937	48.81%	7.311%
10	6.539	1607	1617	1634	rVB6	9477	18365	1.92%	0.288%
11	6.687	1649	1663	1680	rBV	187511	366916	38.35%	5.745%
12	7.562	1920	1935	1957	rBV2	76874	138549	14.48%	2.169%
13	7.896	2026	2039	2062	rBV	291370	509923	53.30%	7.984%
14	8.176	2114	2126	2142	rBV2	49035	85445	8.93%	1.338%
15	8.636	2255	2269	2302	rBV2	461985	956636	100.00%	14.979%
16	9.414	2499	2511	2530	rBV	360056	599890	62.71%	9.393%
17	10.751	2911	2927	2946	rBV	176054	288640	30.17%	4.520%
18	11.809	3243	3256	3277	rBV	303894	489472	51.17%	7.664%
19	12.060	3327	3334	3349	rBV4	6050	10787	1.13%	0.169%
20	12.189	3361	3374	3390	rBV	295135	486120	50.82%	7.612%




Sum of corrected areas: 6386536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052310.D
Acq On : 09 Dec 2022 18:36
Operator : JC/MD
Sample : N5949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

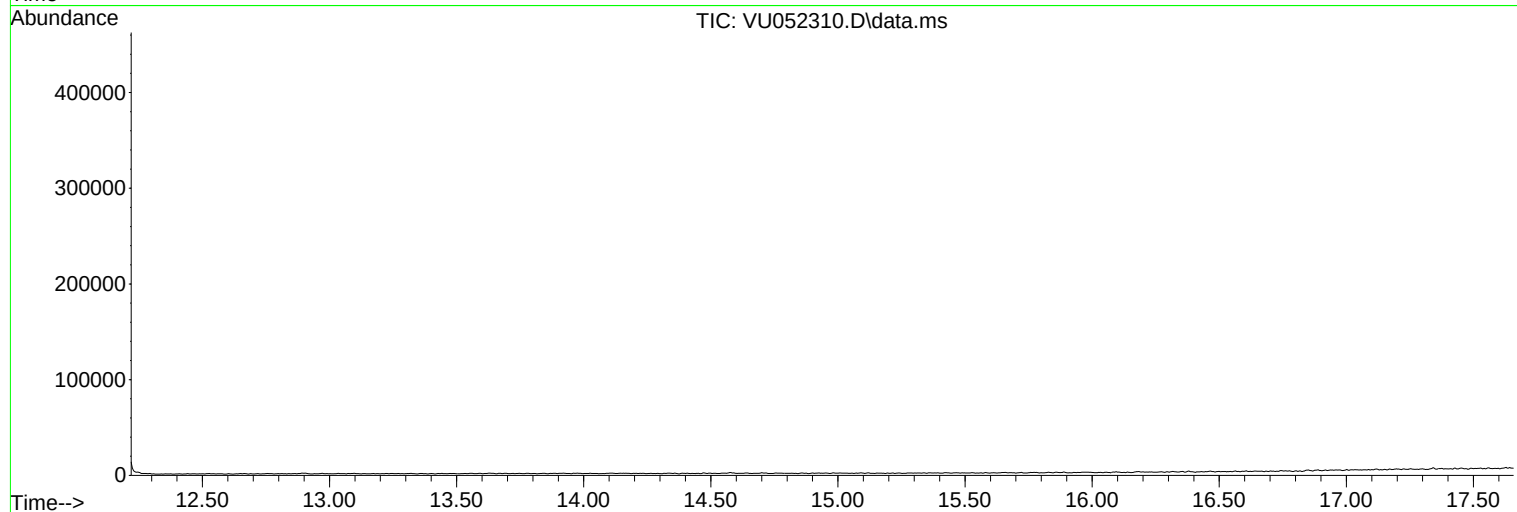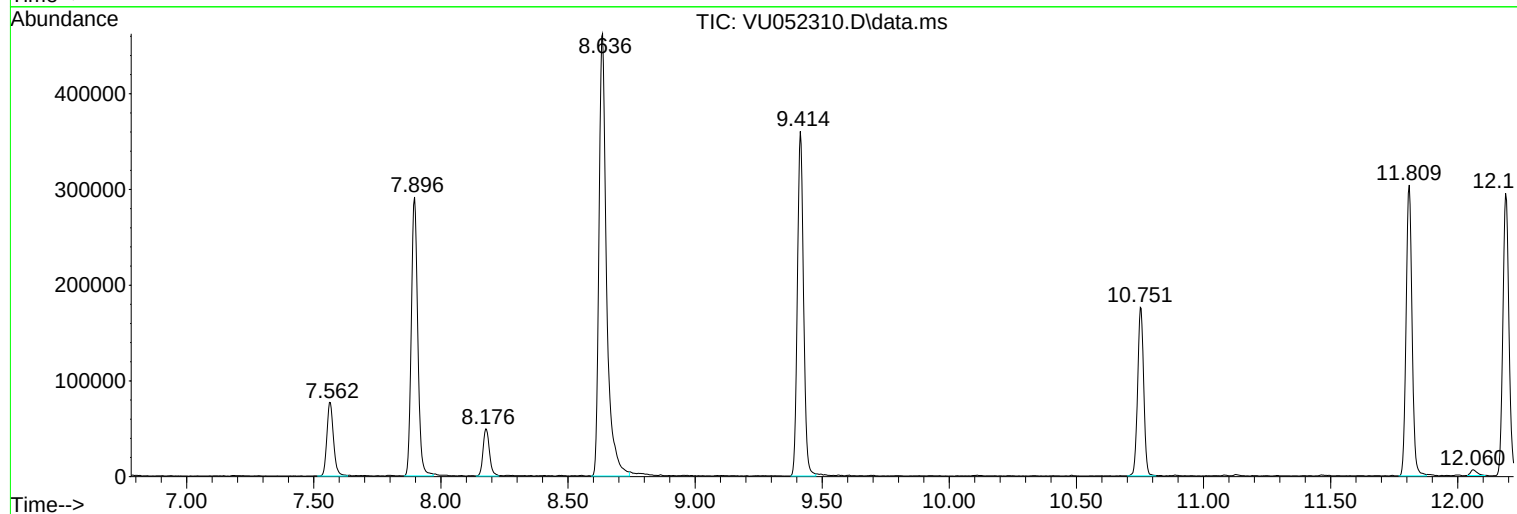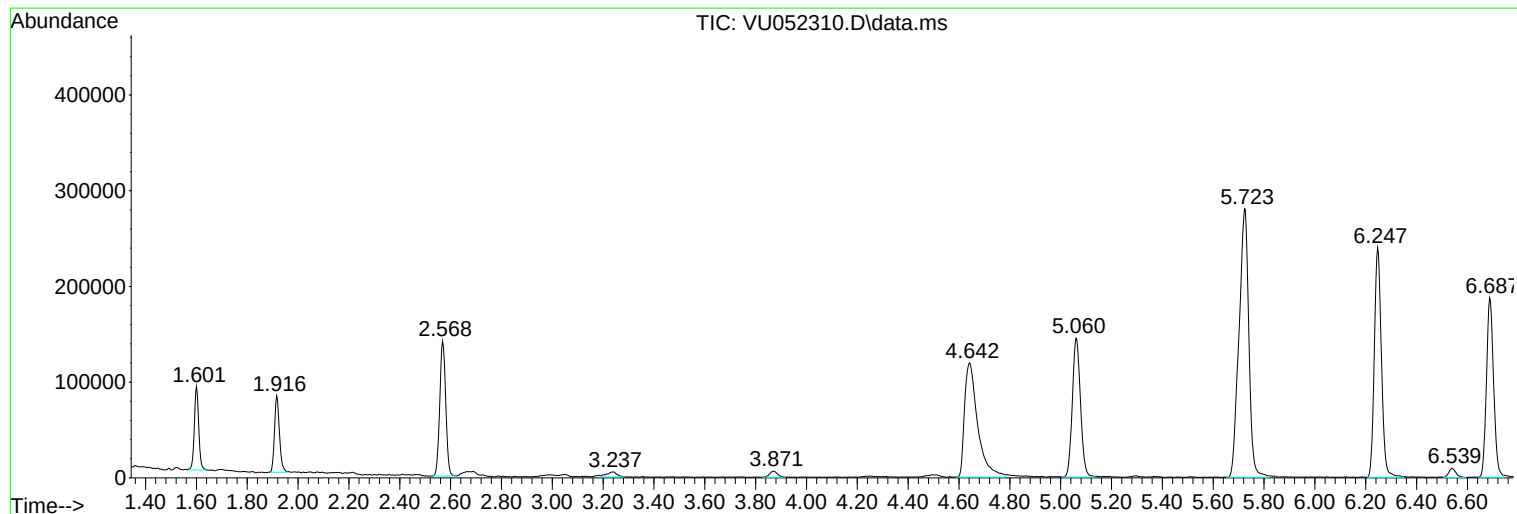

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052310.D
Acq On : 09 Dec 2022 18:36
Operator : JC/MD
Sample : N5949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052310.D
Acq On : 09 Dec 2022 18:36
Operator : JC/MD
Sample : N5949-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc