

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052311.D
 Acq On : 09 Dec 2022 19:00
 Operator : JC/MD
 Sample : N5949-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	96	rVB	131029	157317	15.93%	2.090%
2	1.916	171	179	192	rBV	101846	134957	13.67%	1.793%
3	2.568	369	382	399	rBV	194876	324709	32.89%	4.313%
4	3.269	582	600	616	rVB	5376	16135	1.63%	0.214%
5	3.359	616	628	645	rVB5	10525	23959	2.43%	0.318%
6	3.870	771	787	806	rBV2	28992	70207	7.11%	0.933%
7	4.655	1012	1031	1059	rBV3	151838	597111	60.48%	7.931%
8	5.060	1140	1157	1181	rBV	166046	365490	37.02%	4.855%
9	5.722	1339	1363	1380	rBV3	330382	873015	88.43%	11.596%
10	6.247	1510	1526	1570	rBV	275197	534734	54.16%	7.102%
11	6.542	1606	1618	1633	rVB3	23325	44461	4.50%	0.591%
12	6.687	1642	1663	1686	rBV	209599	417136	42.25%	5.540%
13	7.562	1923	1935	1955	rBV	87537	158644	16.07%	2.107%
14	7.896	2026	2039	2059	rBV	364426	635789	64.40%	8.445%
15	8.176	2116	2126	2140	rBV2	56477	96464	9.77%	1.281%
16	8.552	2234	2243	2254	rBV3	9156	16043	1.63%	0.213%
17	8.632	2254	2268	2305	rBV2	483274	987245	100.00%	13.113%
18	9.414	2495	2511	2530	rBV	405140	670622	67.93%	8.907%
19	10.751	2912	2927	2946	rBV	185912	303416	30.73%	4.030%
20	11.809	3243	3256	3284	rBV	336787	544069	55.11%	7.226%
21	12.188	3362	3374	3396	rBV	340524	557346	56.45%	7.403%




Sum of corrected areas: 7528869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052311.D
Acq On : 09 Dec 2022 19:00
Operator : JC/MD
Sample : N5949-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

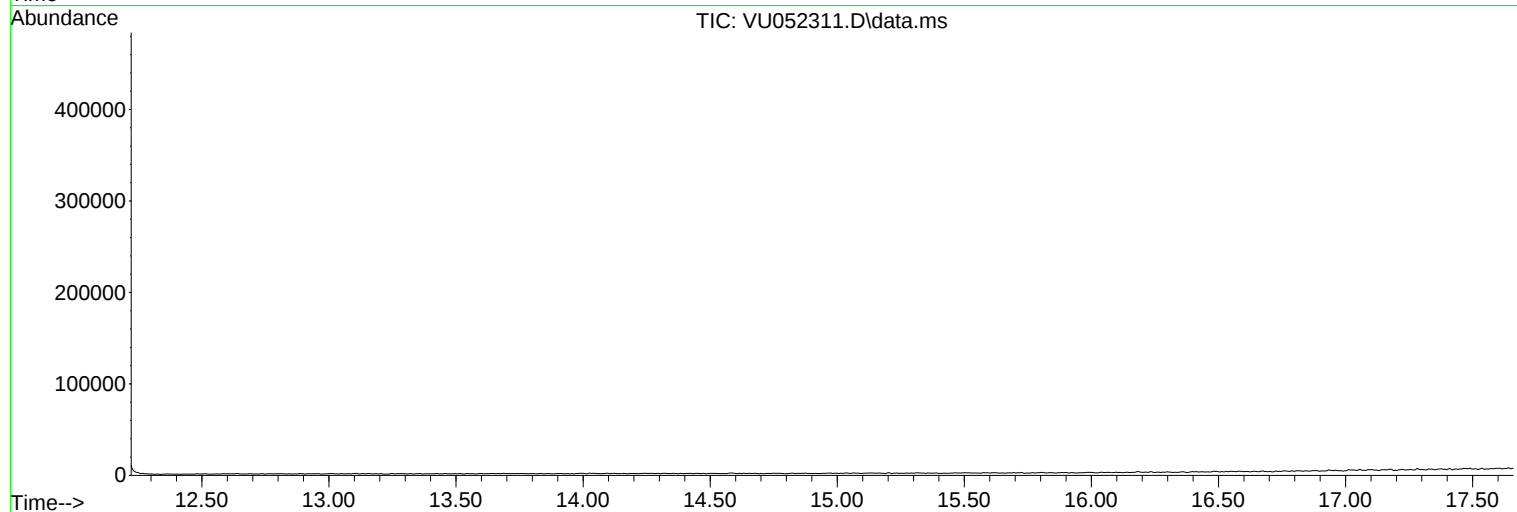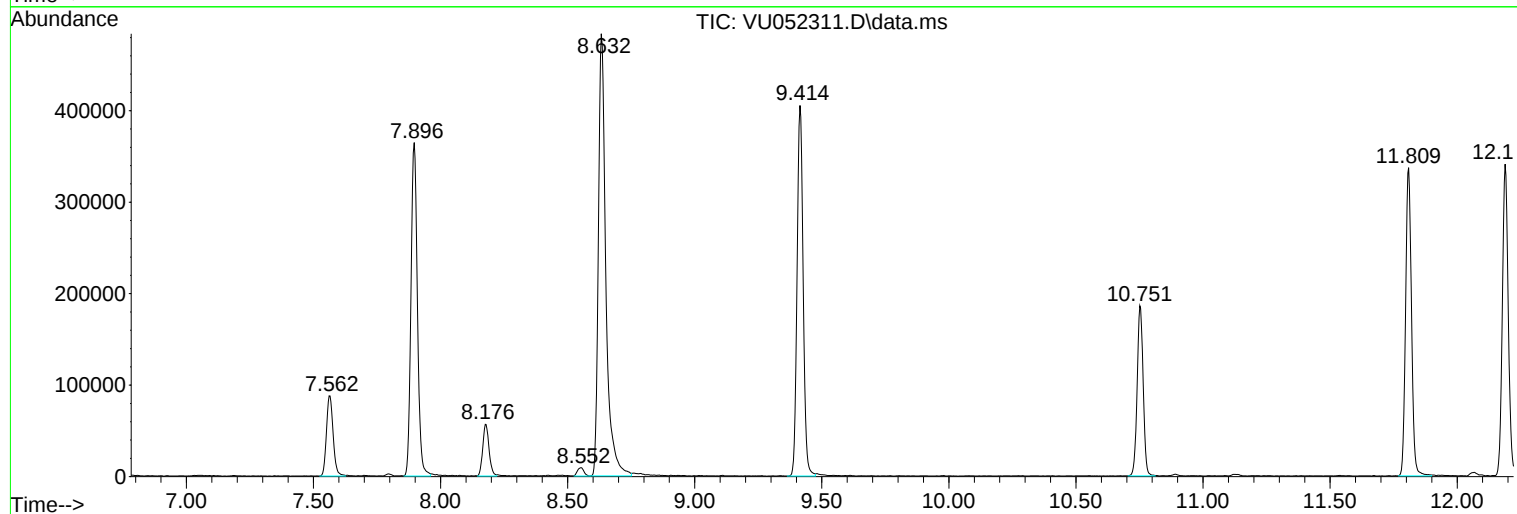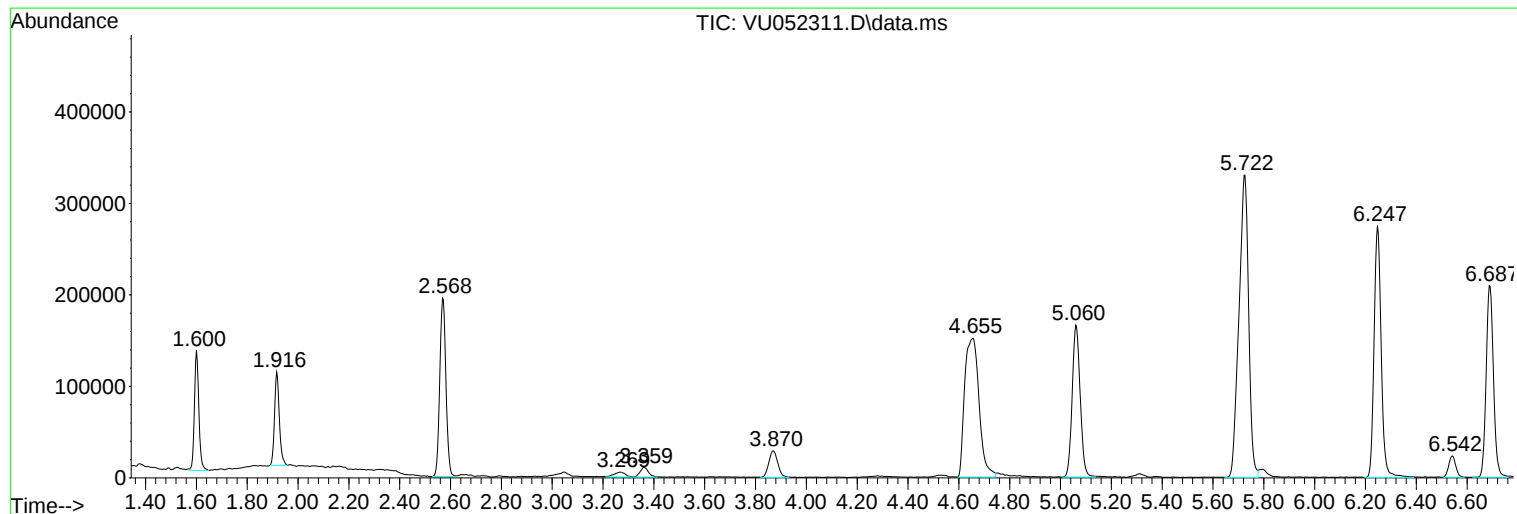

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052311.D
Acq On : 09 Dec 2022 19:00
Operator : JC/MD
Sample : N5949-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052311.D
Acq On : 09 Dec 2022 19:00
Operator : JC/MD
Sample : N5949-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc