

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
 Data File : VU052316.D
 Acq On : 09 Dec 2022 21:22
 Operator : JC/MD
 Sample : VU1209WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK157

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	97	rVB	134028	154431	14.91%	1.992%
2	1.916	170	179	194	rBV	110380	148647	14.35%	1.917%
3	2.569	369	382	399	rBV	207400	337917	32.62%	4.359%
4	3.048	521	531	548	rVB3	10791	21377	2.06%	0.276%
5	3.183	562	573	585	rBV	5084	10903	1.05%	0.141%
6	4.639	1007	1026	1082	rBV2	131833	480810	46.41%	6.202%
7	5.060	1141	1157	1175	rBV	175578	391458	37.79%	5.049%
8	5.723	1342	1363	1395	rBV2	359537	956660	92.35%	12.339%
9	6.247	1512	1526	1546	rBV	276952	531385	51.29%	6.854%
10	6.687	1646	1663	1689	rBV	226838	454847	43.91%	5.867%
11	7.565	1923	1936	1957	rBV	96166	175350	16.93%	2.262%
12	7.896	2025	2039	2059	rBV	409800	720240	69.52%	9.290%
13	8.176	2116	2126	2145	rBV	59431	104336	10.07%	1.346%
14	8.633	2256	2268	2310	rBV2	498423	1035952	100.00%	13.362%
15	9.414	2498	2511	2535	rBV	408713	692282	66.83%	8.929%
16	10.751	2911	2927	2943	rBV	194217	318214	30.72%	4.104%
17	11.809	3244	3256	3288	rBV	352269	571389	55.16%	7.370%
18	12.189	3361	3374	3398	rBV	376607	609009	58.79%	7.855%
19	13.838	3878	3887	3900	rBV3	7981	12411	1.20%	0.160%
20	14.086	3956	3964	3974	rBV2	7605	12025	1.16%	0.155%
21	14.327	4031	4039	4048	rBV3	9066	13315	1.29%	0.172%




Sum of corrected areas: 7752958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052316.D
Acq On : 09 Dec 2022 21:22
Operator : JC/MD
Sample : VU1209WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

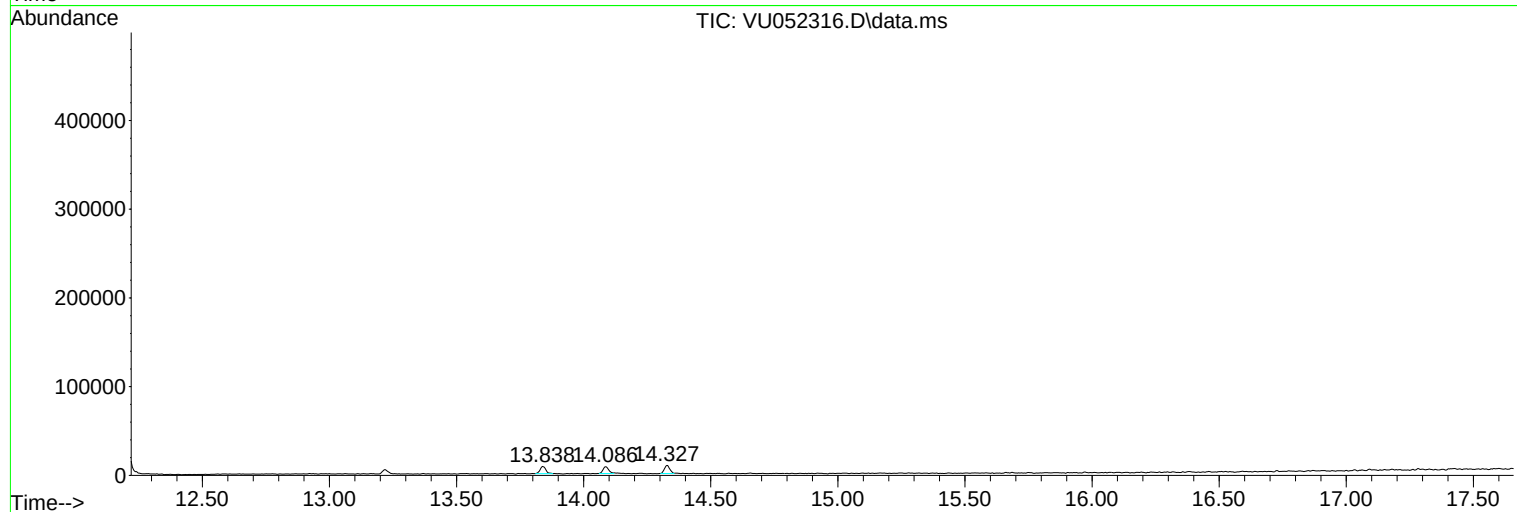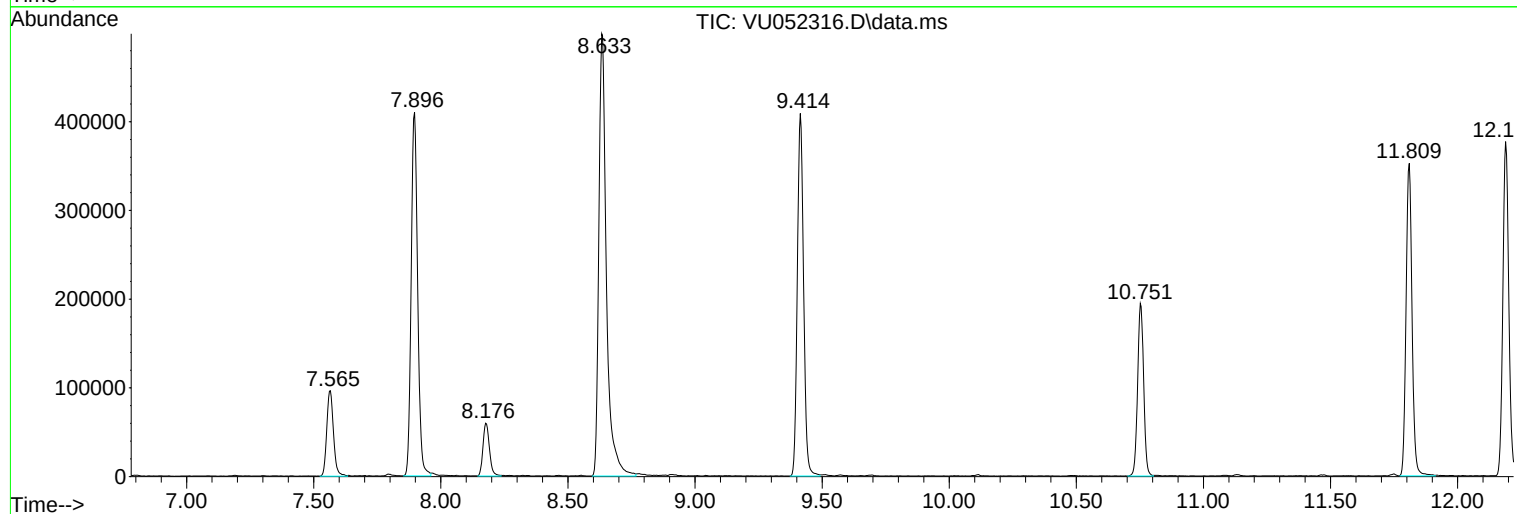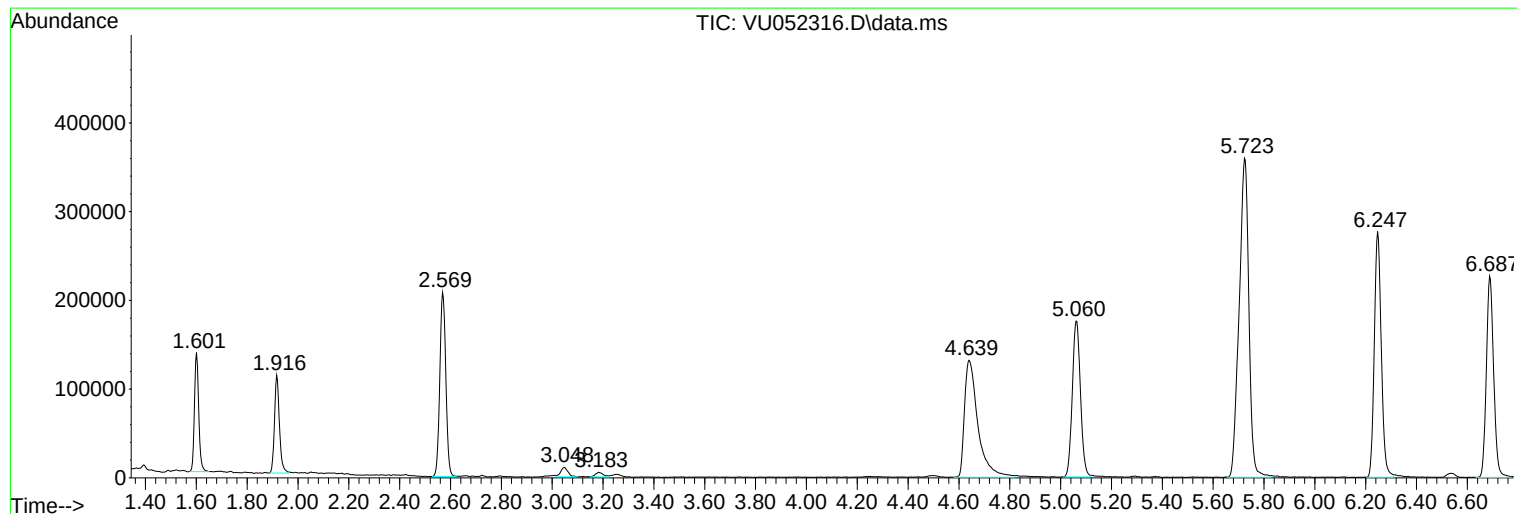

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052316.D
Acq On : 09 Dec 2022 21:22
Operator : JC/MD
Sample : VU1209WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052316.D
Acq On : 09 Dec 2022 21:22
Operator : JC/MD
Sample : VU1209WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc