


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120922\
Data File : VU052288.D
Acq On : 09 Dec 2022 08:56
Operator : JC/MD
Sample : BFB176
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB176

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 08 04:19:43 2022

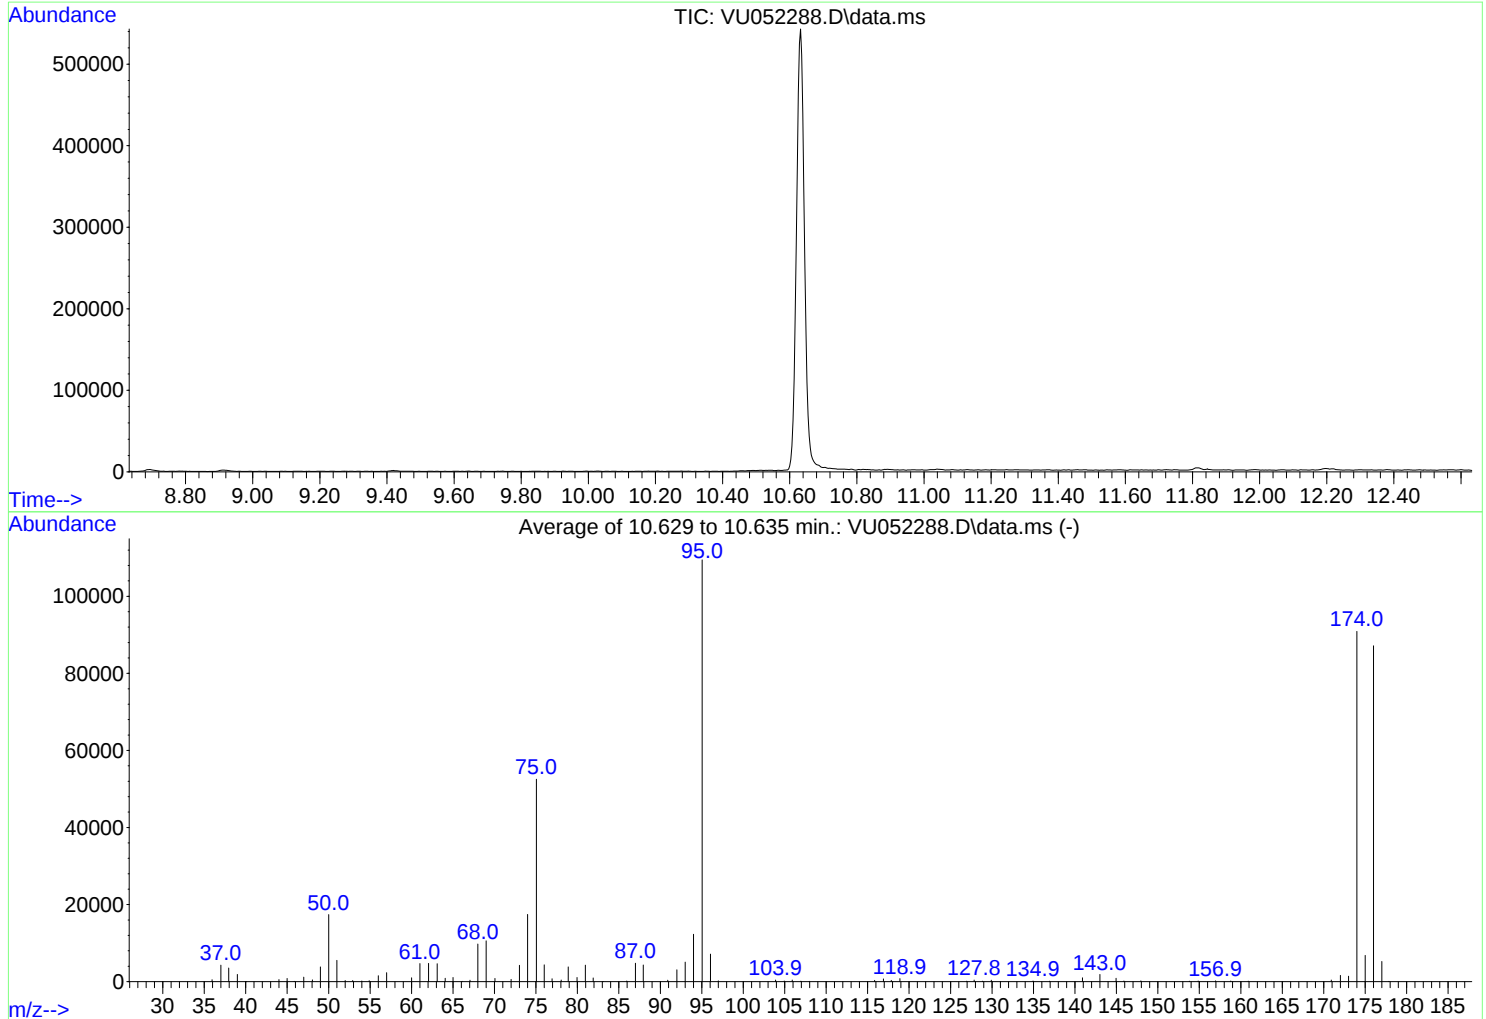

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	17381	PASS
75	95	30	80	48.0	52523	PASS
95	95	100	100	100.0	109467	PASS
96	95	5	9	6.5	7131	PASS
173	174	0.00	2	1.5	1400	PASS
174	95	50	120	83.0	90909	PASS
175	174	5	9	7.5	6826	PASS
176	174	95	101	95.9	87155	PASS
177	176	5	9	6.0	5230	PASS

m/z	Abundance
35.10	191.0
36.00	886.0
37.90	409.0
39.90	221.0
44.00	520.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
36.00	1559.0
37.00	4480.0
38.00	4007.0
39.00	1895.0
40.10	234.0
44.00	956.0
45.00	891.0
45.80	160.0
47.00	1123.0
48.00	469.0
49.00	3846.0
50.00	17384.0
51.00	5495.0
52.00	316.0
52.90	301.0
54.00	111.0
54.90	244.0
56.00	1614.0
57.00	2342.0
60.00	1096.0
61.00	4942.0
62.10	4860.0
63.10	4515.0
64.00	907.0
65.00	1010.0
66.10	126.0
67.00	356.0
68.00	9961.0
69.00	10761.0
70.00	890.0
72.00	569.0
73.00	4259.0
74.00	17704.0
75.10	53416.0
76.00	4700.0
77.00	898.0
78.00	542.0
78.90	3837.0
79.90	1132.0
80.90	4139.0
81.90	875.0
86.00	193.0
87.00	4974.0
87.90	4214.0
90.90	412.0
92.00	3152.0
93.00	4922.0
94.00	12474.0
95.00	110000.0
96.10	7102.0
97.10	211.0
103.90	434.0
105.00	191.0
105.90	405.0
106.90	165.0
115.80	304.0
116.90	691.0
117.80	342.0
118.90	765.0
127.00	132.0
127.90	450.0
128.80	126.0
129.90	385.0
135.00	180.0
136.90	136.0
140.90	1005.0
143.00	1845.0
145.00	936.0
145.90	190.0
147.90	198.0
153.80	111.0
154.80	178.0
156.90	187.0
158.80	122.0
160.90	137.0
170.90	396.0
172.00	1462.0
173.00	1491.0
174.00	88664.0
175.00	6890.0
176.00	84912.0
177.00	5075.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
35.90	1392.0
37.00	4448.0
38.00	4073.0
39.00	1921.0
40.00	231.0
44.00	1136.0
45.00	852.0
45.90	141.0
47.00	1258.0
48.10	464.0
49.00	3997.0
50.00	17888.0
51.00	5714.0
52.00	325.0
52.90	311.0
54.00	156.0
54.90	270.0
56.00	1616.0
57.00	2338.0
60.00	1014.0
61.00	4851.0
62.00	4833.0
63.10	4811.0
64.10	839.0
65.00	1118.0
66.10	108.0
67.10	396.0
68.00	10042.0
69.00	11052.0
70.10	880.0
72.00	621.0
73.00	4332.0
74.00	18024.0
75.10	54056.0
76.00	4505.0
77.00	811.0
78.00	440.0
78.90	3920.0
79.90	1071.0
81.00	4490.0
81.90	950.0
86.00	187.0
87.00	4977.0
88.00	4379.0
90.90	372.0
92.00	3178.0
93.00	5267.0
94.00	12691.0
95.10	112992.0
96.10	7306.0
97.00	215.0
103.90	448.0
105.00	145.0
105.90	446.0
106.90	158.0
107.90	105.0
115.80	334.0
116.90	712.0
117.90	324.0
118.90	820.0
127.00	113.0
127.80	433.0
128.80	133.0
129.90	394.0
134.90	174.0
137.00	119.0
140.90	1028.0
143.00	1939.0
145.00	911.0
145.80	157.0
147.90	223.0
153.80	123.0
154.80	170.0
157.00	238.0
158.80	157.0
160.90	139.0
170.90	443.0
172.00	1675.0
173.00	1478.0
174.00	93840.0
175.00	7087.0
176.00	89928.0
177.00	5337.0
177.80	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176

m/z	Abundance
35.90	1203.0
37.00	3928.0
38.00	3794.0
39.00	1840.0
39.90	266.0
44.00	1153.0
45.00	782.0
47.00	1175.0
48.10	440.0
49.00	3630.0
50.00	16872.0
51.00	5375.0
52.00	298.0
52.90	220.0
54.00	196.0
54.90	293.0
56.00	1425.0
57.00	2339.0
60.00	844.0
61.00	4325.0
62.00	4547.0
63.10	4649.0
64.00	821.0
65.00	1158.0
67.10	354.0
68.00	9246.0
69.00	10012.0
70.00	757.0
72.00	616.0
73.00	4180.0
74.00	16600.0
75.00	50096.0
76.00	3940.0
76.90	592.0
78.10	334.0
78.90	3756.0
80.00	992.0
81.00	4247.0
81.90	1001.0
83.10	123.0
85.90	166.0
87.00	4413.0
88.00	4397.0
90.90	341.0
92.00	2856.0
93.00	4979.0
94.00	11753.0
95.10	105408.0
96.00	6984.0
96.90	232.0
103.90	420.0
104.90	120.0
105.90	429.0
107.00	119.0
108.00	120.0
115.90	311.0
116.90	721.0
117.90	315.0
118.90	734.0
126.90	116.0
127.90	381.0
128.90	129.0
129.90	383.0
131.00	105.0
134.90	174.0
137.00	132.0
140.90	1015.0
143.00	1821.0
144.90	790.0
146.00	131.0
148.00	246.0
153.80	122.0
154.90	164.0
157.00	227.0
158.80	169.0
160.90	100.0
170.90	438.0
172.00	1688.0
173.00	1231.0
174.00	90224.0
175.00	6502.0
176.00	86624.0
177.00	5277.0
177.90	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB176