

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
 Data File : VU062195.D
 Acq On : 10 Dec 2024 07:17
 Operator : MD/SY
 Sample : P5111-11DL 5X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG460DL

Quant Time: Dec 10 07:37:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 10 00:32:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	93747	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.409	117	87275	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.804	152	41838	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	31867	5.039	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.800%
7) Chloroethane-d5	1.904	69	21956	4.882	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.600%
11) 1,1-Dichloroethene-d2	2.557	65	15036	4.998	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	100.000%
20) 2-Butanone-d5	4.628	46	65562	54.101	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.200%
24) Chloroform-d	5.052	84	70532	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.692	65	37497	5.572	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.400%
32) Benzene-d6	5.718	84	132197	5.259	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.200%
36) 1,2-Dichloropropane-d6	6.682	67	38906	5.409	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.200%
41) Toluene-d8	7.891	98	120281	5.065	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
43) trans-1,3-Dichloroprop...	8.174	79	15090	4.767	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.400%
46) 2-Hexanone-d5	8.631	63	51133	53.538	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.080%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	30615	5.470	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	42482	5.510	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds						
2) Dichlorodifluoromethane	1.380	85	5948	0.677	ug/L	97
17) Methyl tert-butyl Ether	3.354	73	138646	8.793	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062195.D
Acq On : 10 Dec 2024 07:17
Operator : MD/SY
Sample : P5111-11DL 5X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG460DL

Quant Time: Dec 10 07:37:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 10 00:32:19 2024
Response via : Initial Calibration




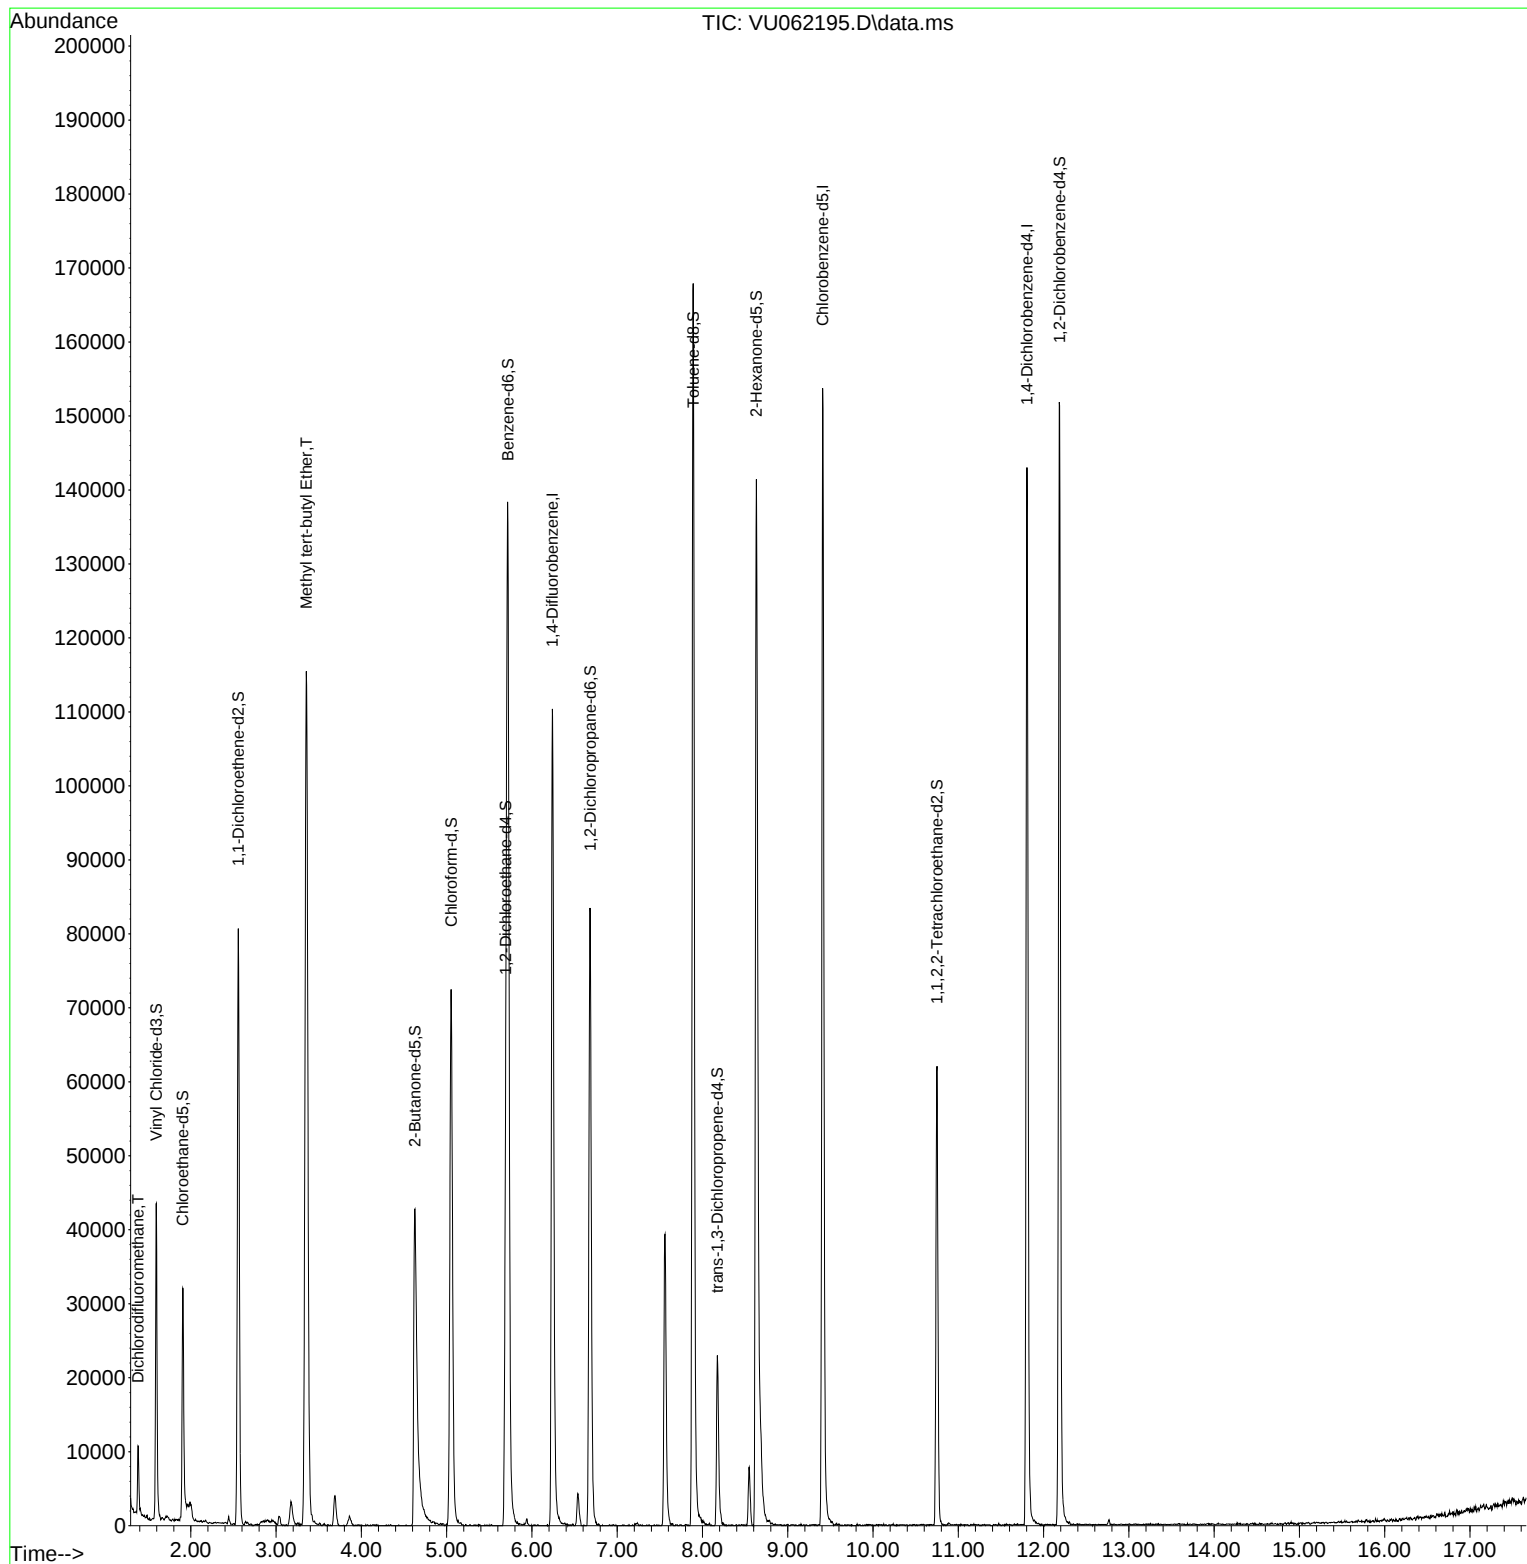


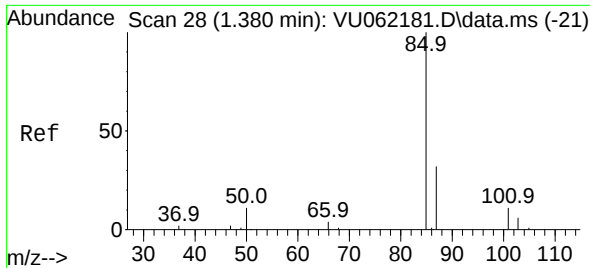

#2
 Dichlorodifluoromethane
 Concen: 0.677 ug/L
 RT: 1.380 min Scan# 21
 Delta R.T. -0.003 min
 Lab File: VU062195.D
 Acq: 10 Dec 2024 07:17

Instrument :
 MSVOA_U
 ClientSampleId :
 BG460DL

Tgt Ion: 85 Resp: 5948
 Ion Ratio Lower Upper
 85 100
 87 35.0 26.6 40.0

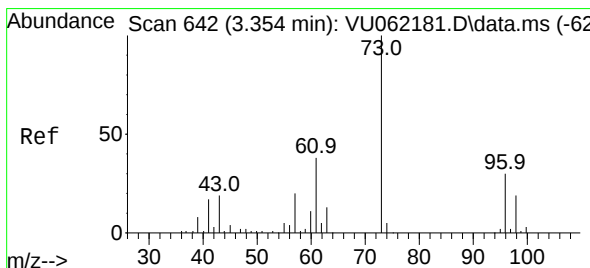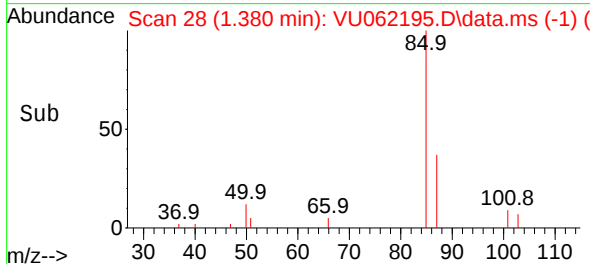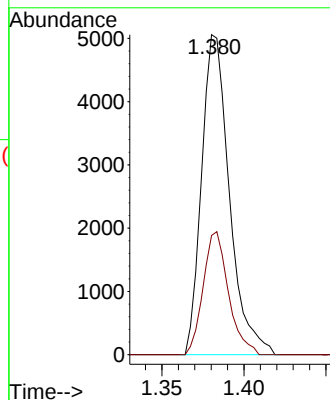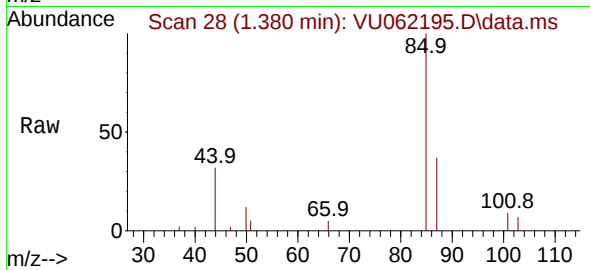

#17
 Methyl tert-butyl Ether
 Concen: 8.793 ug/L
 RT: 3.354 min Scan# 642
 Delta R.T. 0.000 min
 Lab File: VU062195.D
 Acq: 10 Dec 2024 07:17

Tgt Ion: 73 Resp: 138646
 Ion Ratio Lower Upper
 73 100
 43 19.1 16.3 24.5
 57 20.0 17.1 25.7

