

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062194.D
Acq On : 10 Dec 2024 06:53
Operator : MD/SY
Sample : P5111-01DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG450DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU062194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.383	23	29	41	rVB	4911	5348	1.60%	0.169%
2	1.596	87	95	114	rVB	42372	48054	14.41%	1.517%
3	1.907	183	192	208	rVB	31090	40897	12.27%	1.291%
4	2.560	384	395	414	rBV2	75009	131444	39.42%	4.149%
5	3.184	576	589	599	rVB3	1859	4362	1.31%	0.138%
6	3.695	739	748	759	rBV5	2915	5398	1.62%	0.170%
7	4.624	1024	1037	1075	rBV4	42771	149638	44.88%	4.724%
8	5.055	1155	1171	1191	rBV	66181	150143	45.03%	4.740%
9	5.718	1358	1377	1406	rBV2	129105	333442	100.00%	10.526%
10	6.242	1528	1540	1559	rBV	111785	219449	65.81%	6.927%
11	6.534	1619	1631	1665	rBV	102960	202716	60.79%	6.399%
12	6.682	1665	1677	1703	rBV	75772	150406	45.11%	4.748%
13	7.560	1939	1950	1973	rBV	36342	67916	20.37%	2.144%
14	7.891	2041	2053	2074	rBV	150947	272658	81.77%	8.607%
15	8.174	2131	2141	2160	rBV2	21151	37921	11.37%	1.197%
16	8.544	2245	2256	2272	rBV	146471	254928	76.45%	8.047%
17	8.627	2272	2282	2313	rVV3	126833	271588	81.45%	8.573%
18	9.409	2514	2525	2547	rBV	153769	266322	79.87%	8.407%
19	10.746	2931	2941	2962	rBV	56447	93760	28.12%	2.960%
20	11.804	3260	3270	3289	rBV	140068	235183	70.53%	7.424%
21	12.187	3375	3389	3413	rBV	131159	226279	67.86%	7.143%




Sum of corrected areas: 3167852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062194.D
Acq On : 10 Dec 2024 06:53
Operator : MD/SY
Sample : P5111-01DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG450DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

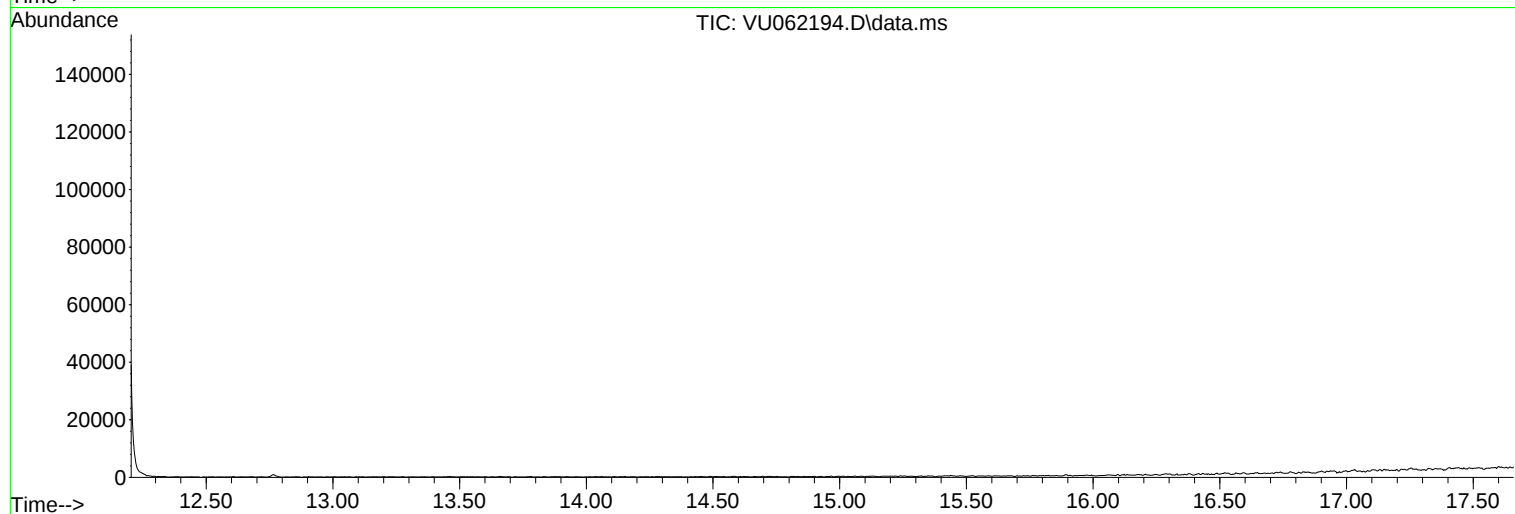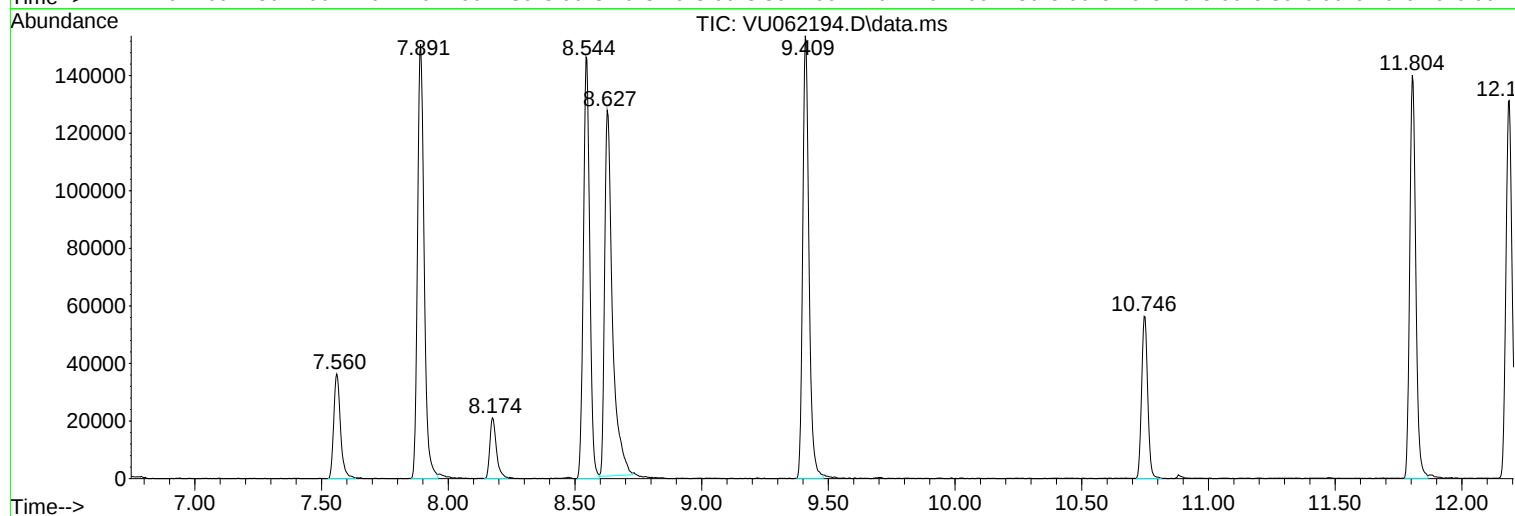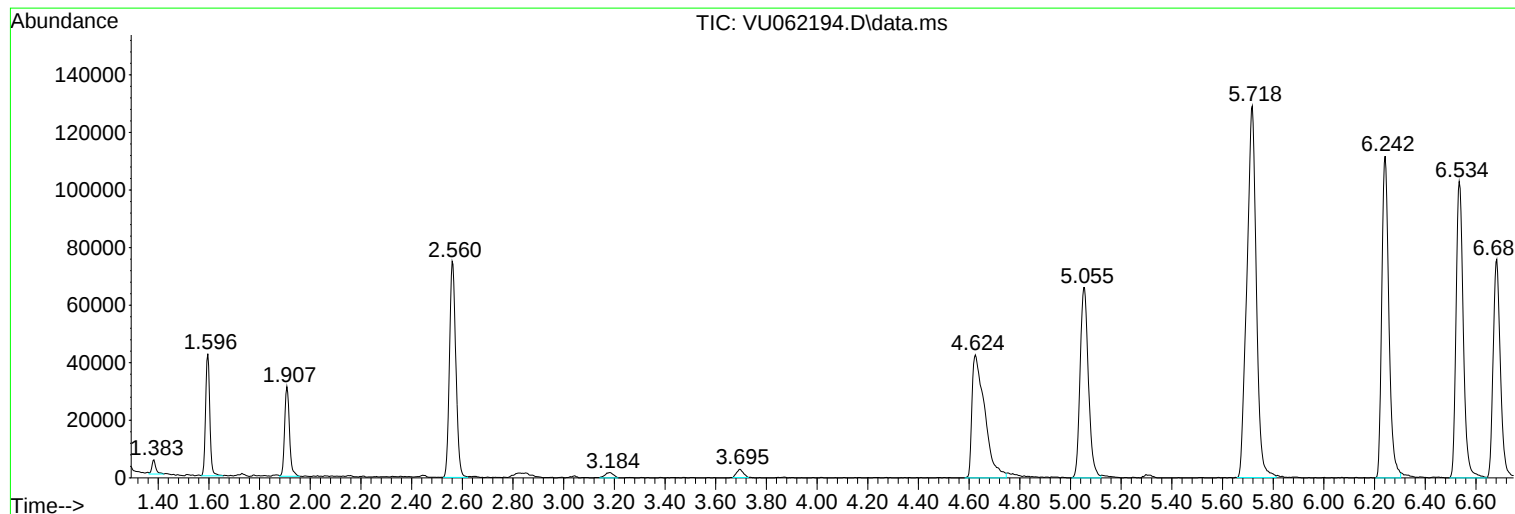

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062194.D
Acq On : 10 Dec 2024 06:53
Operator : MD/SY
Sample : P5111-01DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG450DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062194.D
Acq On : 10 Dec 2024 06:53
Operator : MD/SY
Sample : P5111-01DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG450DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------