
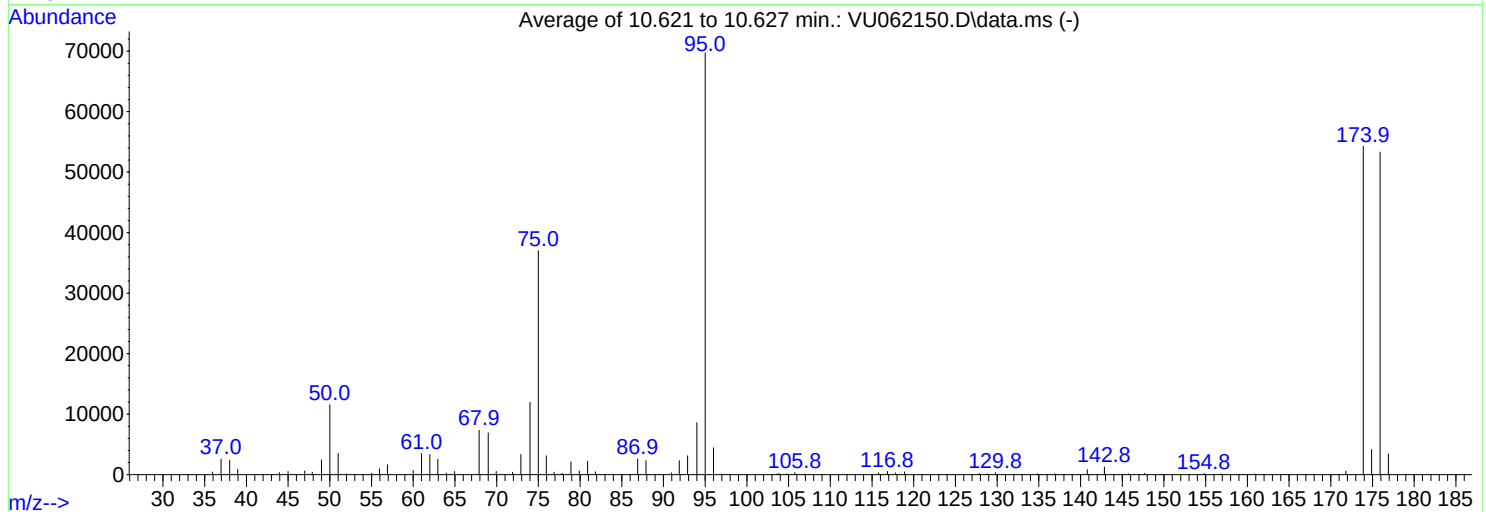


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU120924\
Data File : VU062150.D
Acq On : 09 Dec 2024 07:53
Operator : MD/SY
Sample : BFB042
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB042

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 10 00:32:19 2024

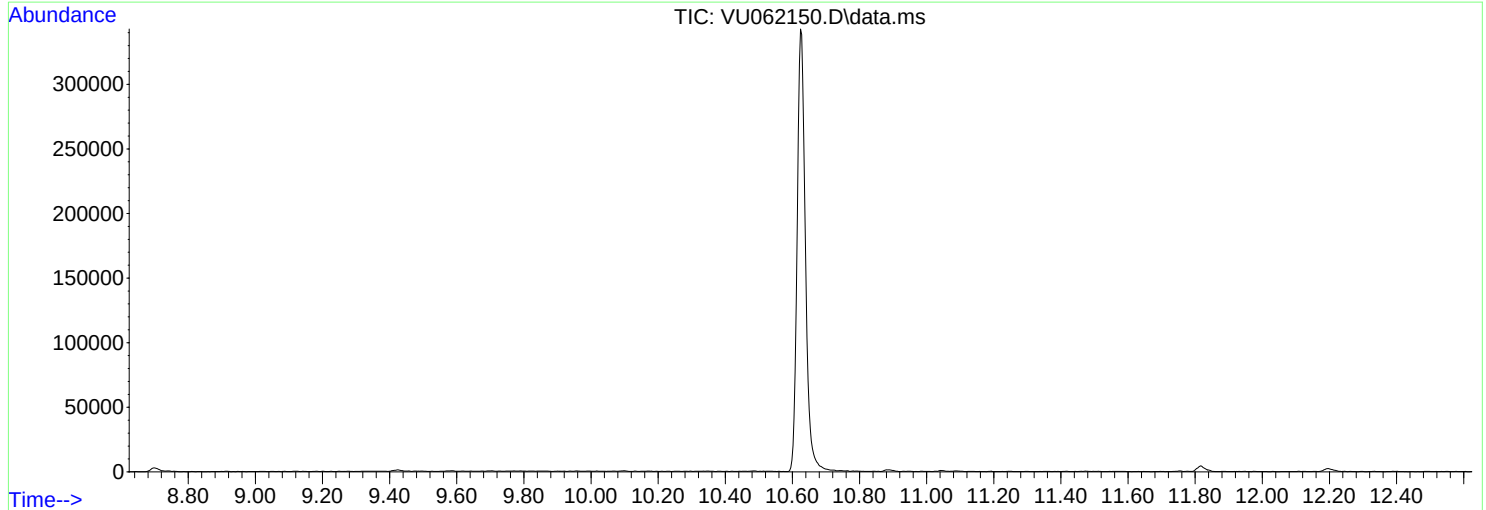

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	11543	PASS
75	95	30	80	53.1	37027	PASS
95	95	100	100	100.0	69720	PASS
96	95	5	9	6.4	4444	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.8	54256	PASS
175	174	5	9	7.7	4161	PASS
176	174	95	101	98.3	53328	PASS
177	176	5	9	6.4	3402	PASS

m/z	Abundance
35.90	273.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
36.00	700.0
37.00	2446.0
38.00	2394.0
39.00	852.0
44.00	317.0
45.00	504.0
47.00	521.0
47.90	372.0
49.00	2347.0
50.00	10774.0
51.00	3286.0
51.90	125.0
55.00	222.0
55.90	966.0
56.90	1689.0
60.00	616.0
61.00	3474.0
62.00	3171.0
63.00	2381.0
63.90	246.0
64.90	479.0
67.90	7133.0
69.00	6718.0
70.00	479.0
71.90	415.0
72.90	3225.0
74.00	11545.0
75.00	35576.0
75.90	3174.0
76.90	358.0
77.80	248.0
78.90	2006.0
79.90	570.0
80.90	2175.0
81.80	471.0
86.90	2470.0
87.90	2220.0
91.00	286.0
91.90	2209.0
92.90	3140.0
94.00	7961.0
95.00	66160.0
96.00	4394.0
96.90	136.0
103.90	338.0
104.80	129.0
105.70	348.0
115.80	333.0
116.90	515.0
117.90	300.0
118.90	376.0
127.80	187.0
128.80	121.0
129.80	304.0
134.80	123.0
137.00	169.0
140.80	773.0
142.00	107.0
142.90	1308.0
145.80	101.0
147.70	238.0
149.70	111.0
154.80	213.0
156.90	128.0
158.80	102.0
160.90	116.0
171.80	550.0
173.90	50832.0
174.90	3838.0
175.90	49936.0
176.90	3325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
36.00	679.0
36.90	2645.0
38.00	2472.0
39.00	892.0
44.00	364.0
45.00	538.0
47.00	634.0
47.90	405.0
49.00	2480.0
50.00	11923.0
51.00	3611.0
52.00	118.0
55.00	227.0
56.00	993.0
56.90	1699.0
60.00	700.0
61.00	3613.0
62.00	3411.0
62.90	2640.0
64.00	279.0
65.00	520.0
67.90	7553.0
69.00	7259.0
69.90	550.0
71.90	409.0
72.90	3451.0
74.00	12343.0
75.00	38200.0
76.00	3204.0
76.90	405.0
77.80	255.0
78.90	2160.0
79.90	565.0
80.90	2259.0
81.90	500.0
86.90	2681.0
87.90	2439.0
91.00	319.0
91.90	2459.0
92.90	3231.0
94.00	8977.0
95.00	71792.0
96.00	4552.0
96.90	118.0
103.80	332.0
104.80	132.0
105.70	375.0
106.90	111.0
115.80	337.0
116.80	546.0
117.80	281.0
118.90	459.0
127.90	230.0
128.80	124.0
129.80	340.0
134.90	168.0
136.90	165.0
140.80	883.0
142.80	1314.0
145.00	116.0
145.70	149.0
147.70	231.0
149.80	110.0
154.80	212.0
156.90	133.0
160.90	140.0
171.80	610.0
173.90	55784.0
174.90	4330.0
175.90	55192.0
176.90	3466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042

m/z	Abundance
36.00	693.0
36.90	2631.0
38.00	2272.0
38.90	908.0
43.90	365.0
45.00	539.0
47.00	664.0
47.90	397.0
49.00	2472.0
50.00	11932.0
51.00	3690.0
52.10	119.0
55.00	204.0
56.00	935.0
56.90	1553.0
60.00	733.0
61.00	3388.0
62.00	3413.0
62.90	2621.0
64.00	308.0
65.00	562.0
67.90	7315.0
69.00	6768.0
69.90	578.0
71.90	381.0
72.90	3298.0
74.00	11960.0
75.00	37304.0
76.00	2982.0
76.90	445.0
77.90	227.0
78.90	2202.0
79.90	568.0
80.90	2183.0
81.80	494.0
86.90	2684.0
87.90	2366.0
90.90	304.0
91.90	2334.0
92.90	3023.0
94.00	8831.0
95.00	71208.0
96.00	4386.0
96.90	103.0
103.60	316.0
104.80	124.0
105.80	348.0
106.90	141.0
115.80	291.0
116.80	532.0
117.70	302.0
118.90	503.0
127.90	247.0
128.80	133.0
129.80	336.0
134.90	213.0
136.80	142.0
140.80	912.0
142.80	1151.0
144.70	117.0
145.00	121.0
145.70	173.0
147.70	173.0
154.80	204.0
156.80	120.0
160.90	132.0
171.80	618.0
173.90	56152.0
174.90	4314.0
175.90	54856.0
176.90	3414.0

Instrument :
MSVOA_U
ClientSampleId :
BFB042