


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU121018\
Data File : VU028539.D
Acq On : 10 Dec 2018 08:43
Operator : MD/SY
Sample : BFB62
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM120718WMA.M
Title : VOC Analysis
Last Update : Wed Dec 12 05:44:10 2018

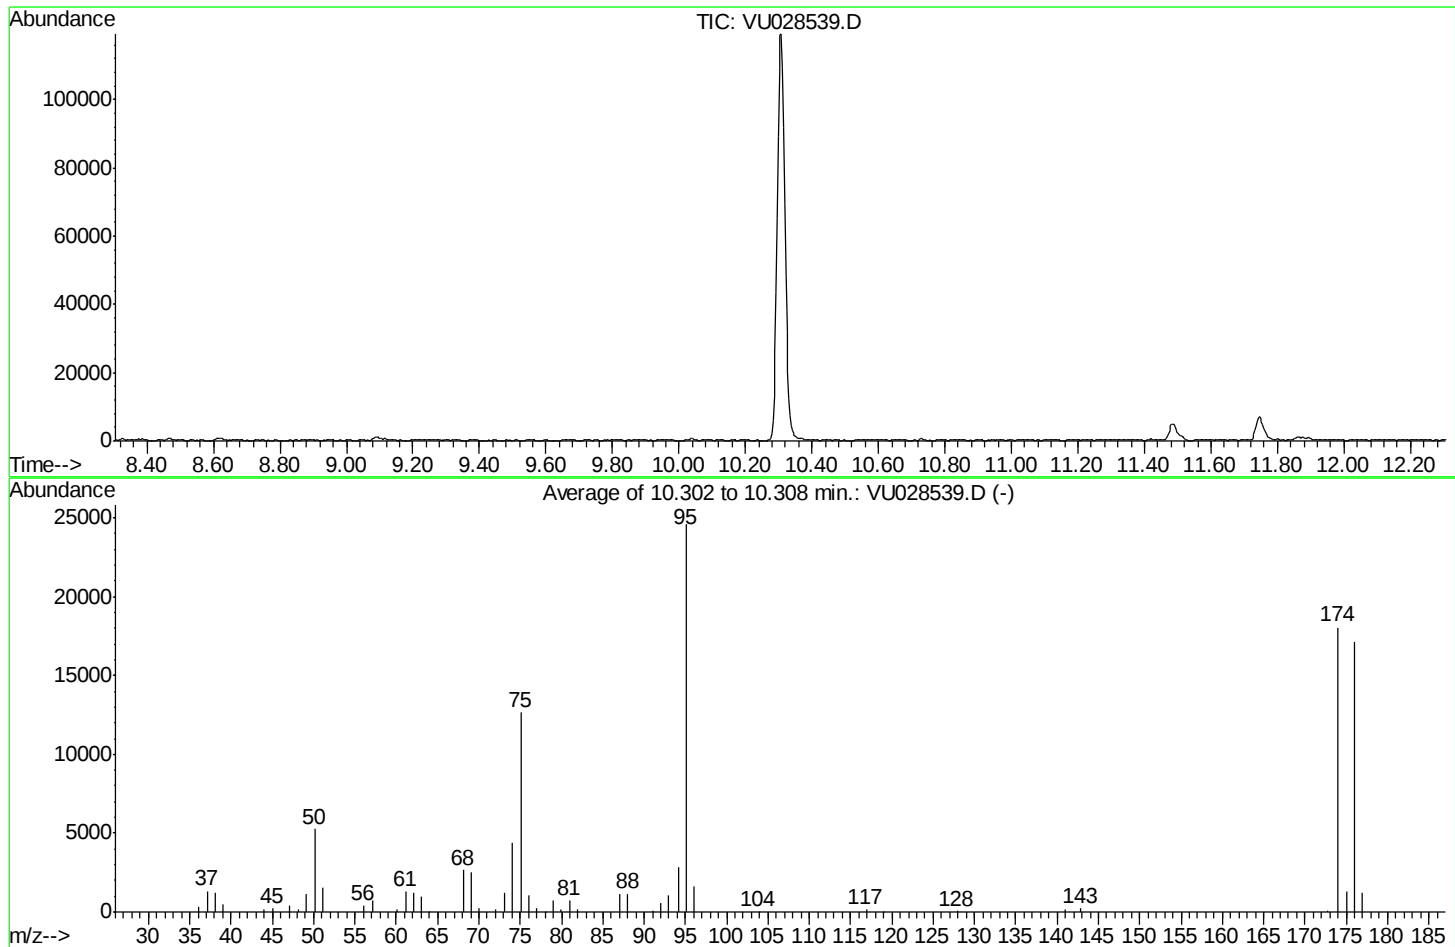

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	5252	PASS
75	95	30	80	51.4	12639	PASS
95	95	100	100	100.0	24589	PASS
96	95	5	9	6.5	1587	PASS
173	174	0.00	2	0.4	64	PASS
174	95	50	120	73.3	18032	PASS
175	174	5	9	7.1	1284	PASS
176	174	95	101	95.1	17152	PASS
177	176	5	9	6.9	1182	PASS

m/z	Abundance
44.00	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
36.00	334.0
37.10	1239.0
38.10	1131.0
39.10	489.0
44.00	308.0
45.10	194.0
47.00	363.0
48.10	148.0
49.10	1089.0
50.10	4878.0
51.10	1523.0
56.00	355.0
57.10	680.0
60.10	179.0
61.10	1218.0
62.10	1129.0
63.10	919.0
68.10	2656.0
69.10	2393.0
70.00	191.0
72.00	197.0
73.00	1097.0
74.10	4277.0
75.10	11845.0
76.10	1046.0
77.00	264.0
78.00	101.0
79.00	713.0
80.00	160.0
81.00	644.0
81.90	123.0
87.00	1112.0
88.00	1207.0
92.00	460.0
93.00	913.0
94.10	2632.0
95.10	23176.0
96.10	1436.0
116.90	122.0
127.90	102.0
140.90	158.0
142.90	233.0
174.00	16472.0
175.00	1255.0
176.00	15922.0
177.00	1121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
36.00	322.0
37.10	1379.0
38.10	1269.0
39.00	537.0
44.00	351.0
45.00	230.0
47.00	382.0
48.10	189.0
49.10	1185.0
50.10	5371.0
51.10	1578.0
56.00	382.0
57.10	733.0
60.10	207.0
61.10	1322.0
62.10	1270.0
63.10	997.0
68.10	2783.0
69.00	2527.0
70.00	246.0
72.00	190.0
73.00	1242.0
74.10	4559.0
75.10	13044.0
76.10	1045.0
77.00	251.0
79.00	766.0
79.90	199.0
81.00	708.0
81.90	147.0
87.00	1192.0
88.10	1188.0
91.00	120.0
92.00	524.0
93.00	1060.0
94.10	2899.0
95.10	25400.0
96.10	1616.0
117.00	130.0
127.90	112.0
140.90	170.0
142.90	211.0
172.80	194.0
174.00	18568.0
175.00	1314.0
176.00	17688.0
177.00	1208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62

m/z	Abundance
36.00	268.0
37.10	1395.0
38.10	1289.0
39.00	521.0
44.00	364.0
45.00	239.0
47.00	384.0
48.10	210.0
49.10	1198.0
50.10	5508.0
51.10	1552.0
56.00	415.0
57.10	726.0
60.10	214.0
61.10	1308.0
62.10	1251.0
63.10	954.0
63.90	114.0
68.10	2596.0
69.00	2521.0
70.00	264.0
72.00	167.0
73.10	1255.0
74.10	4442.0
75.10	13028.0
76.10	973.0
77.00	190.0
79.00	737.0
79.90	211.0
81.00	728.0
81.90	159.0
87.10	1165.0
88.00	1120.0
91.00	120.0
91.90	616.0
93.00	1093.0
94.10	2886.0
95.10	25192.0
96.00	1709.0
103.90	105.0
117.00	130.0
119.00	122.0
141.00	205.0
142.90	177.0
174.00	19056.0
175.10	1283.0
176.00	17848.0
177.00	1217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB62