

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121019\
 Data File : VU036080.D
 Acq On : 10 Dec 2019 13:25
 Operator : JC/MD
 Sample : K6105-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFE28

Quant Time: Dec 11 07:07:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 11 06:27:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	322594	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	351780	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	93901	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	139920	4.87	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.40%
7) Chloroethane-d5	1.93	69	128456	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.59	63	155738	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	4.69	46	236948	48.36	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.72%
24) Chloroform-d	5.11	84	208755	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.75	65	117446	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
32) Benzene-d6	5.77	84	436352	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.73	67	134639	5.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.20%
41) Toluene-d8	7.93	98	354279	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.20%
43) trans-1,3-Dichloropropene-	8.21	79	51189	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.70	63	198437	49.00	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.00%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	118366	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.80%
64) 1,2-Dichlorobenzene-d4	12.22	152	93489	5.18	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.60%


Target Compounds					Ovalue
13) Acetone	2.66	43	11788	1.895 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121019\
Data File : VU036080.D
Acq On : 10 Dec 2019 13:25
Operator : JC/MD
Sample : K6105-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFE28

Quant Time: Dec 11 07:07:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 11 06:27:41 2019
Response via : Initial Calibration

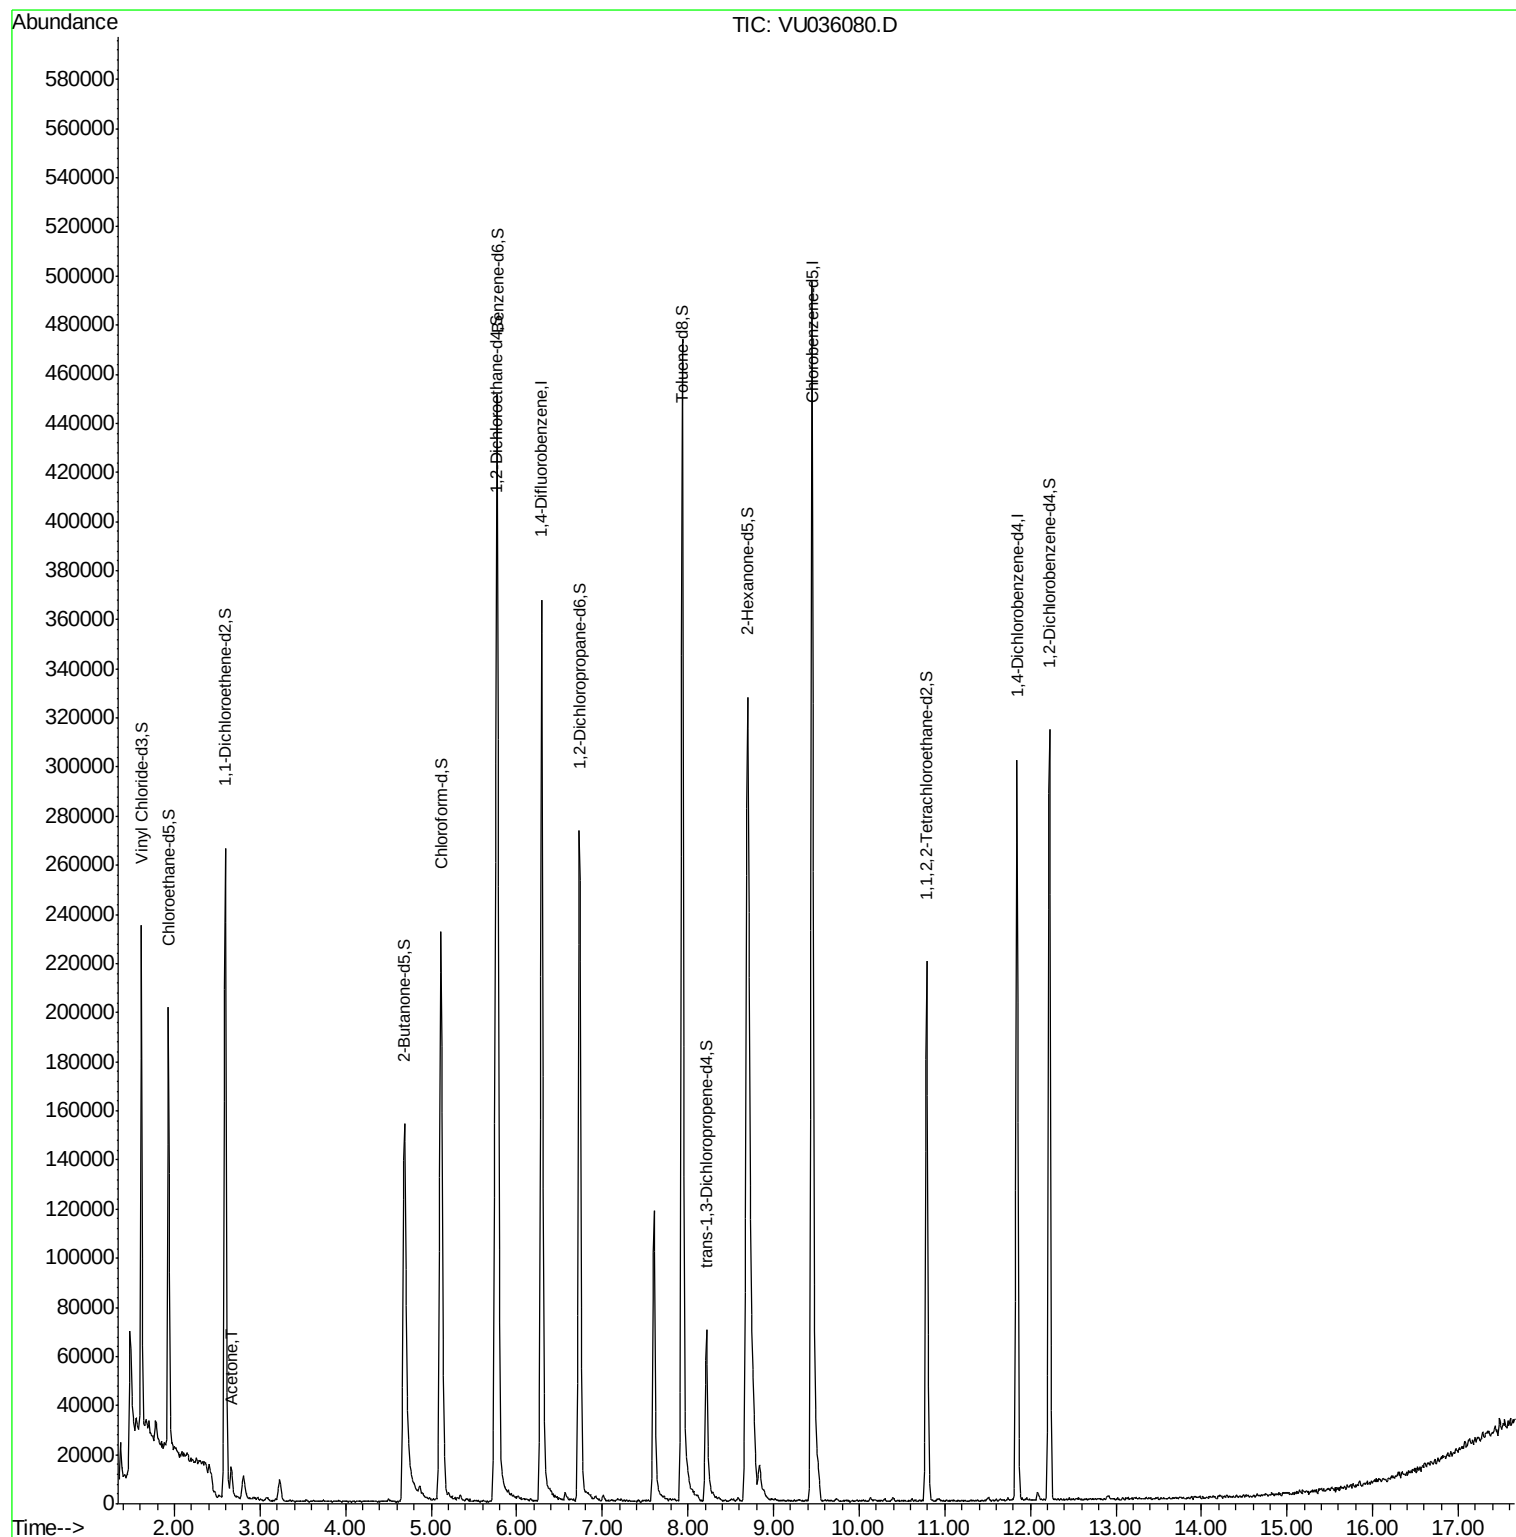

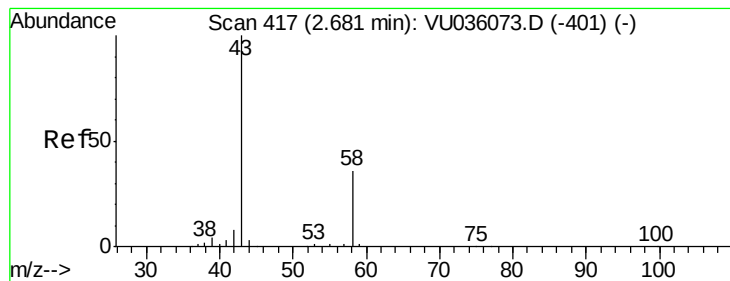

#13

Acetone

Concen: 1.895 ug/L

RT: 2.66 min Scan# 412

Delta R.T. -0.02 min

Lab File: VU036080.D

Acq: 10 Dec 2019 13:25


Instrument :
MSVOA_U
ClientSampleId :
BFE28

Tot Ion: 43 Resp: 11788

Ion Ratio Lower Upper

43 100

58 41.3 0.0 74.2

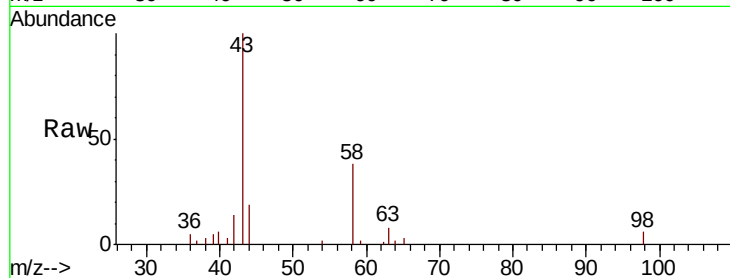

Abundance Ion 43.05 (42.75 to 43.75): VU036080.D (-324) (-)

