


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121019\
Data File : VU036072.D
Acq On : 10 Dec 2019 09:25
Operator : JC/MD
Sample : BFB15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Dec 12 16:48:53 2019

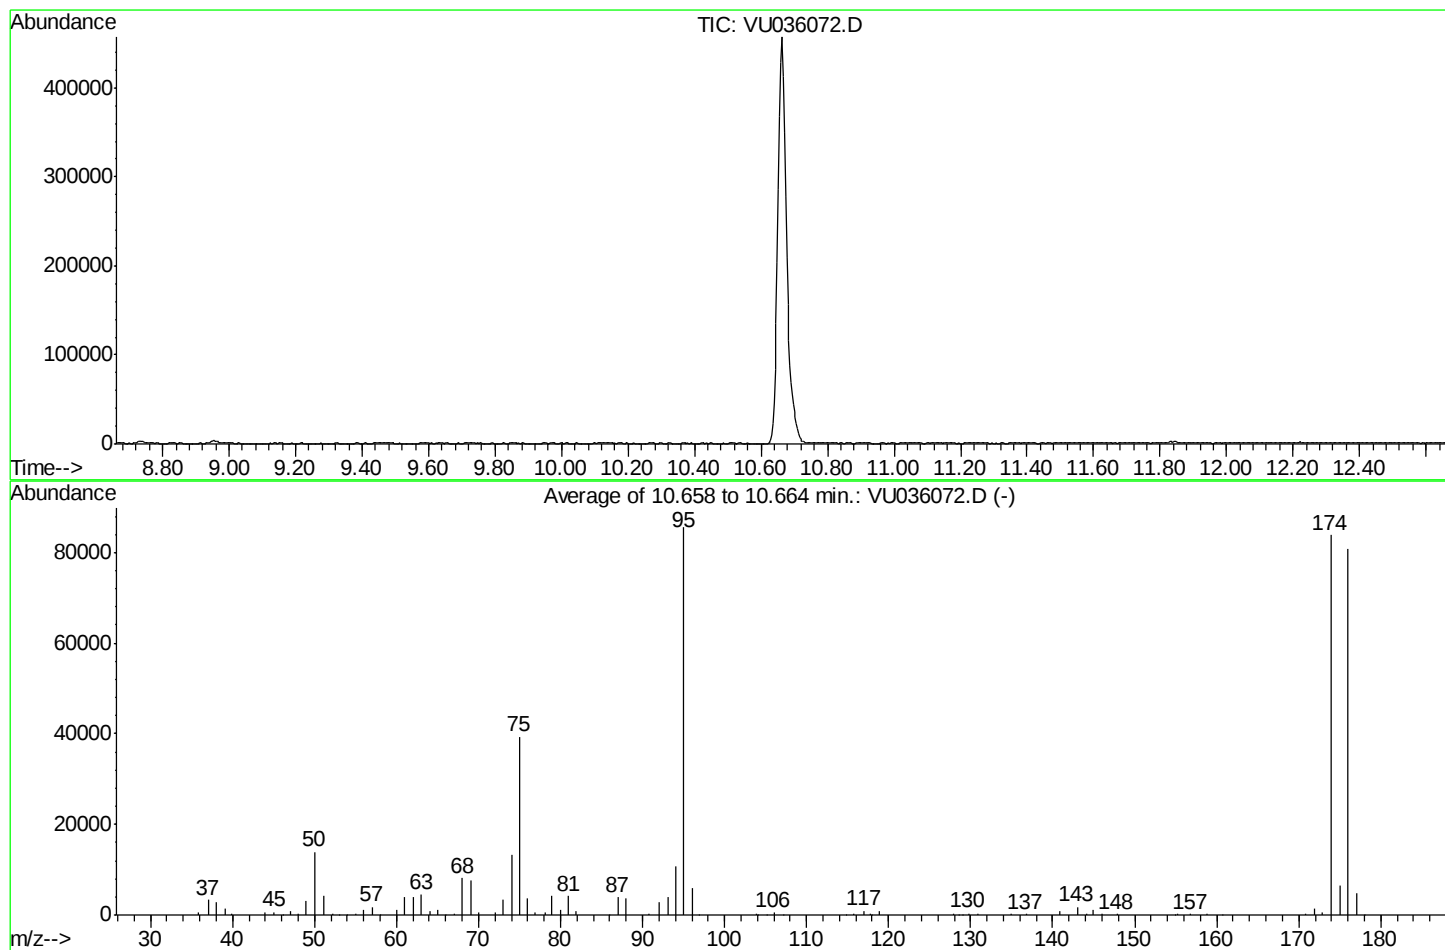

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	13984	PASS
75	95	30	80	46.0	39394	PASS
95	95	100	100	100.0	85565	PASS
96	95	5	9	6.9	5935	PASS
173	174	0.00	2	0.5	457	PASS
174	95	50	120	98.0	83890	PASS
175	174	5	9	7.9	6617	PASS
176	174	95	101	96.5	80912	PASS
177	176	5	9	6.1	4924	PASS

m/z	Abundance
35.90	687.0
37.00	3098.0
38.00	2605.0
39.00	1354.0
39.80	205.0
44.00	719.0
45.00	707.0
47.10	925.0
48.00	377.0
49.00	2822.0
50.00	13369.0
51.00	4219.0
52.10	350.0
55.10	345.0
55.90	1222.0
57.00	1752.0
58.00	162.0
59.90	890.0
61.00	4053.0
62.00	4013.0
63.00	4292.0
64.10	827.0
65.00	927.0
67.10	199.0
68.00	7924.0
69.00	7519.0
69.90	601.0
72.10	544.0
73.00	3185.0
74.10	12760.0
75.00	38728.0
76.00	3613.0
76.90	379.0
78.20	525.0
78.90	3980.0
80.00	1102.0
81.00	4155.0
81.90	1002.0
86.00	210.0
87.00	3499.0
88.00	3690.0
90.80	301.0
92.00	2786.0
93.10	3944.0
94.10	10359.0
95.10	82520.0
96.00	6102.0
96.90	101.0
103.80	316.0
105.10	123.0
106.00	410.0
115.80	356.0
117.00	892.0
117.70	255.0
118.00	266.0
118.90	780.0
127.90	215.0
128.60	168.0
129.80	475.0
130.80	178.0
135.00	116.0
136.80	235.0
140.90	775.0
143.00	1722.0
144.20	167.0
144.90	1037.0
146.00	343.0
147.80	185.0
155.20	256.0
156.90	180.0
158.80	167.0
160.70	107.0
170.90	392.0
171.80	1283.0
172.90	1372.0
174.00	79152.0
175.00	6500.0
176.00	75968.0
177.00	4664.0
178.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
35.90	677.0
37.00	3386.0
38.10	2764.0
39.10	1393.0
39.80	236.0
44.00	931.0
45.00	660.0
47.00	1006.0
48.00	410.0
49.00	3105.0
50.00	14448.0
51.10	4294.0
52.20	358.0
53.00	110.0
53.90	106.0
55.10	373.0
55.90	1167.0
57.00	1857.0
58.00	121.0
60.00	1016.0
61.00	4148.0
62.00	4138.0
63.00	4566.0
64.10	886.0
65.00	1109.0
67.10	239.0
68.00	8415.0
69.00	7934.0
70.00	622.0
72.10	565.0
73.00	3460.0
74.10	13846.0
75.00	40352.0
76.00	3578.0
76.90	508.0
78.20	592.0
78.90	4419.0
79.90	1114.0
81.00	4253.0
81.90	933.0
86.00	129.0
87.00	4029.0
88.00	3716.0
90.80	286.0
92.00	2999.0
93.10	3780.0
94.10	11006.0
95.00	87760.0
96.00	6168.0
96.90	123.0
103.90	353.0
105.00	127.0
106.00	497.0
114.90	119.0
115.80	305.0
117.00	963.0
117.80	333.0
118.90	842.0
127.90	280.0
128.60	163.0
129.00	173.0
129.80	412.0
130.90	174.0
134.80	186.0
136.80	219.0
140.90	861.0
143.00	1795.0
144.10	206.0
144.90	1088.0
146.10	286.0
147.80	223.0
155.10	245.0
156.80	213.0
158.80	216.0
170.90	414.0
171.90	1441.0
173.90	85712.0
175.00	6844.0
175.90	83176.0
177.00	5097.0
178.00	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
35.90	602.0
37.10	3353.0
38.00	2960.0
39.10	1318.0
39.90	211.0
40.10	209.0
44.00	1024.0
45.10	631.0
46.20	116.0
47.00	914.0
48.00	519.0
49.00	3109.0
50.00	14136.0
51.10	4135.0
52.20	284.0
53.00	174.0
54.00	130.0
55.10	339.0
56.00	1118.0
57.00	1855.0
60.00	1139.0
61.00	3764.0
62.10	4089.0
63.00	4400.0
64.10	887.0
65.10	1216.0
66.00	101.0
67.10	221.0
68.00	7985.0
69.00	7721.0
70.10	666.0
72.10	493.0
73.00	3640.0
74.10	13521.0
75.00	39104.0
76.00	3533.0
76.90	514.0
78.20	471.0
78.90	4363.0
79.90	1122.0
80.90	4074.0
81.90	878.0
87.00	4053.0
88.00	3239.0
90.80	327.0
92.00	3081.0
93.00	3779.0
94.00	10660.0
95.00	86416.0
96.00	5536.0
96.90	143.0
104.10	395.0
106.00	502.0
107.10	103.0
114.80	148.0
115.80	256.0
117.00	932.0
117.80	431.0
118.90	813.0
127.80	278.0
129.00	149.0
129.70	347.0
130.90	183.0
134.90	242.0
136.80	184.0
140.90	834.0
143.00	1752.0
144.00	174.0
145.00	980.0
145.90	189.0
147.90	268.0
154.90	310.0
156.80	181.0
158.80	175.0
170.90	483.0
171.90	1348.0
173.90	86808.0
175.00	6509.0
175.90	83592.0
177.00	5013.0
178.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

Scan 2884 (10.613 min): VU036072.D
BFB15

m/z	Abundance
40.10	127.0
44.00	411.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15