


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121020\
 Data File : VU041528.D
 Acq On : 10 Dec 2020 10:55
 Operator : SY/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 11 07:33:47 2020

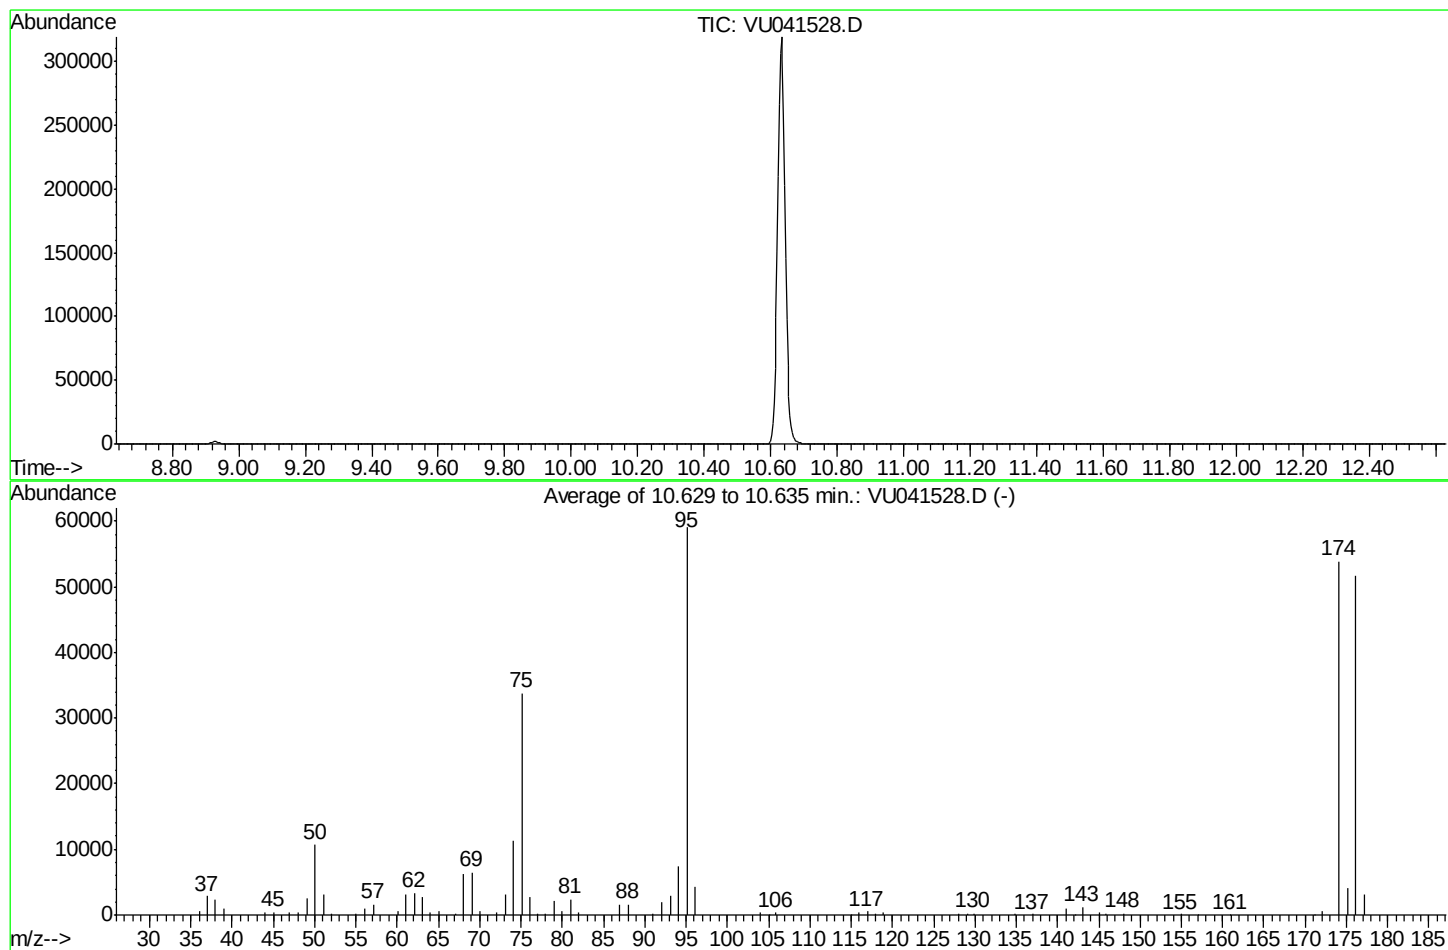

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10651	PASS
75	95	30	80	57.3	33826	PASS
95	95	100	100	100.0	59042	PASS
96	95	5	9	7.2	4223	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.2	53824	PASS
175	174	5	9	7.8	4197	PASS
176	174	95	101	96.1	51722	PASS
177	176	5	9	6.2	3182	PASS

m/z	Abundance
36.00	629.0
37.00	2904.0
38.00	2300.0
39.00	991.0
44.00	374.0
45.00	447.0
47.00	398.0
48.00	465.0
49.10	2628.0
50.10	10681.0
51.10	3041.0
52.00	176.0
55.00	154.0
56.10	1041.0
57.10	1648.0
60.00	701.0
61.00	3391.0
62.10	3639.0
63.00	2750.0
64.00	420.0
65.10	564.0
67.00	186.0
68.10	6339.0
69.10	6591.0
70.00	511.0
72.00	458.0
73.10	3252.0
74.10	11399.0
75.10	33864.0
76.00	2674.0
76.90	282.0
78.00	173.0
79.00	2133.0
80.00	635.0
81.00	2247.0
82.00	489.0
87.00	1587.0
88.00	1656.0
90.90	299.0
92.00	1881.0
93.10	3038.0
94.10	7365.0
95.10	58960.0
96.10	4300.0
103.90	303.0
105.10	111.0
105.90	349.0
116.00	342.0
117.00	489.0
117.90	215.0
118.90	474.0
128.00	272.0
129.10	100.0
129.90	278.0
134.90	113.0
137.00	127.0
141.00	840.0
143.00	1226.0
145.00	472.0
145.80	108.0
148.00	192.0
155.00	164.0
160.90	114.0
172.00	624.0
174.10	52152.0
175.10	4075.0
176.10	50400.0
177.10	3195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	653.0
37.00	2933.0
38.00	2389.0
39.00	1013.0
44.00	418.0
45.00	478.0
47.00	395.0
47.90	501.0
49.10	2644.0
50.10	10969.0
51.10	3199.0
52.00	172.0
55.00	142.0
56.00	1042.0
57.10	1698.0
60.00	662.0
61.10	3271.0
62.10	3494.0
63.00	2940.0
64.00	383.0
65.10	622.0
67.10	216.0
68.10	6412.0
69.10	6687.0
70.00	530.0
72.00	400.0
73.10	3143.0
74.10	11716.0
75.10	34968.0
76.00	2747.0
76.90	320.0
78.00	159.0
79.00	2206.0
80.00	681.0
81.00	2477.0
81.90	510.0
87.00	1650.0
88.00	1740.0
91.00	298.0
92.00	2025.0
93.10	3130.0
94.10	7647.0
95.10	61144.0
96.10	4384.0
103.90	317.0
105.00	115.0
105.90	361.0
116.00	337.0
117.00	511.0
117.90	244.0
118.90	507.0
128.00	263.0
129.10	122.0
129.80	311.0
134.90	111.0
137.00	141.0
141.00	1021.0
143.00	1233.0
145.00	448.0
145.80	129.0
148.00	207.0
154.90	181.0
157.00	103.0
160.90	110.0
171.20	105.0
172.00	632.0
174.10	55688.0
175.10	4370.0
176.10	53176.0
177.10	3229.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	549.0
37.00	2740.0
38.00	2273.0
39.00	885.0
43.90	411.0
45.00	446.0
46.90	298.0
47.90	446.0
49.00	2441.0
50.10	10305.0
51.10	3054.0
52.00	147.0
55.00	153.0
56.00	942.0
57.10	1548.0
60.10	566.0
61.10	2781.0
62.10	3007.0
63.10	2709.0
64.00	342.0
65.00	566.0
67.20	218.0
68.00	5714.0
69.10	6116.0
70.00	474.0
72.10	372.0
73.10	2812.0
74.10	10946.0
75.10	32648.0
76.00	2603.0
77.00	278.0
77.90	148.0
79.00	2153.0
79.90	607.0
81.00	2506.0
81.90	472.0
87.00	1548.0
88.00	1563.0
91.00	242.0
92.10	2007.0
93.10	2828.0
94.10	7358.0
95.10	57024.0
96.10	3987.0
104.00	313.0
105.90	306.0
115.00	103.0
115.90	315.0
116.90	513.0
117.90	264.0
118.90	483.0
127.90	233.0
129.10	135.0
129.80	284.0
134.90	118.0
137.00	118.0
141.10	1079.0
142.20	107.0
143.00	1127.0
145.00	411.0
145.80	132.0
148.00	203.0
154.90	196.0
157.00	116.0
172.00	577.0
174.10	53632.0
175.10	4148.0
176.10	51592.0
177.10	3124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB22