

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046267.D
 Acq On : 10 Dec 2021 15:51
 Operator : SY/MD
 Sample : M4885-22MEDL 20X
 Misc : 3.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW9M7MEDL

Quant Time: Dec 10 22:24:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 03 05:08:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	237944	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	239959	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	131379	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	69477	35.446	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.900%		
7) Chloroethane-d5	1.919	69	54883	36.469	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	72.940%		
11) 1,1-Dichloroethene-d2	2.572	63	98644	28.034	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.060%#		
21) 2-Butanone-d5	4.639	46	125299	80.415	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	80.420%		
24) Chloroform-d	5.070	84	127356	38.909	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.820%		
26) 1,2-Dichloroethane-d4	5.707	65	89888	40.920	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.840%		
32) Benzene-d6	5.732	84	282105	41.018	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.040%		
36) 1,2-Dichloropropane-d6	6.697	67	89614	42.043	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.080%		
41) Toluene-d8	7.903	98	247476	39.520	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.040%#		
43) trans-1,3-Dichloroprop...	8.183	79	43585	42.359	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.720%		
47) 2-Hexanone-d5	8.636	63	88346	87.417	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.420%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	133968	41.444	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.880%		
66) 1,2-Dichlorobenzene-d4	12.195	152	104338	41.238	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.480%		
Target Compounds					Qvalue	
25) Chloroform	5.093	83	13379	3.804	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046267.D
Acq On : 10 Dec 2021 15:51
Operator : SY/MD
Sample : M4885-22MEDL 20X
Misc : 3.59g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW9M7MEDL

Quant Time: Dec 10 22:24:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 03 05:08:36 2021
Response via : Initial Calibration

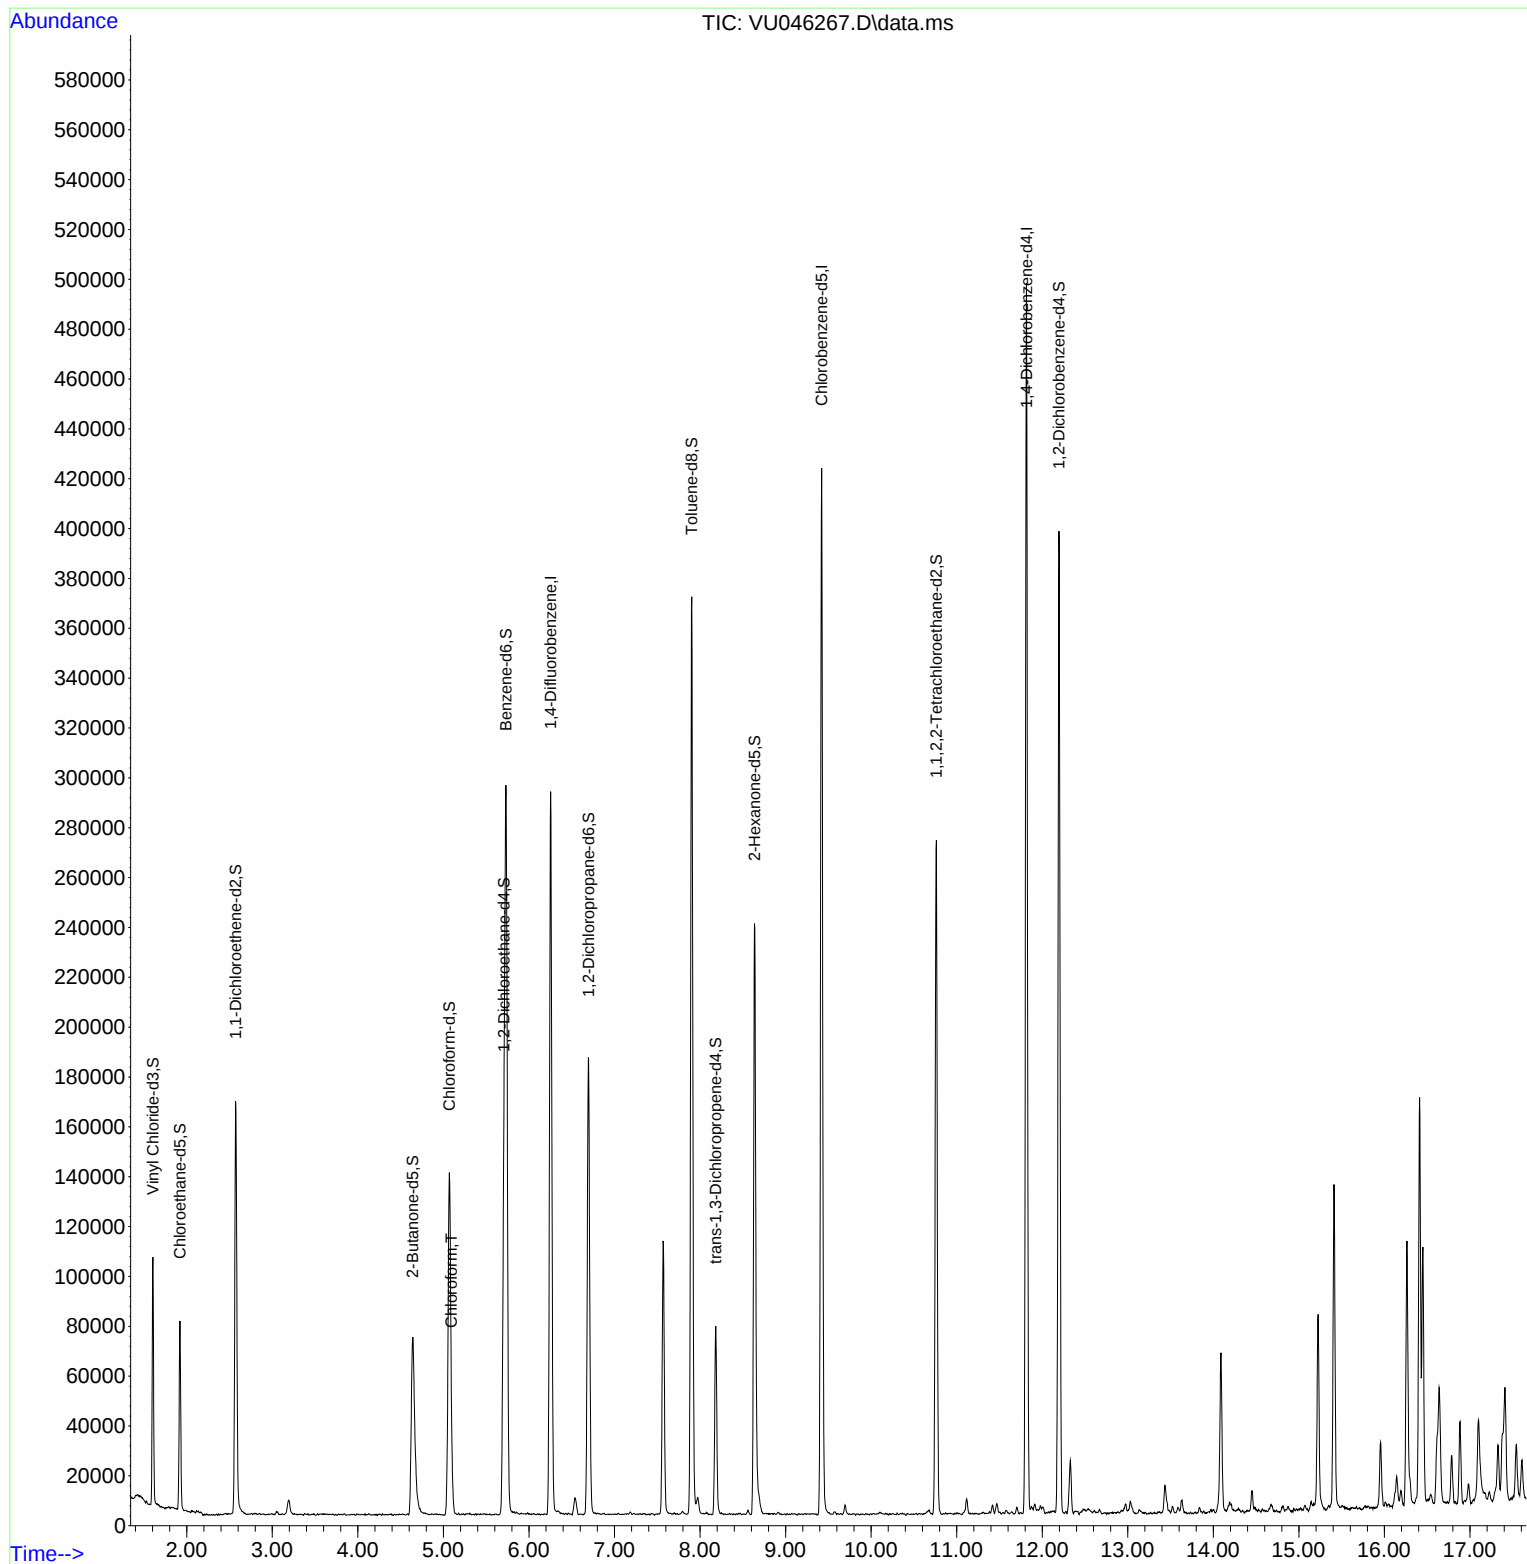

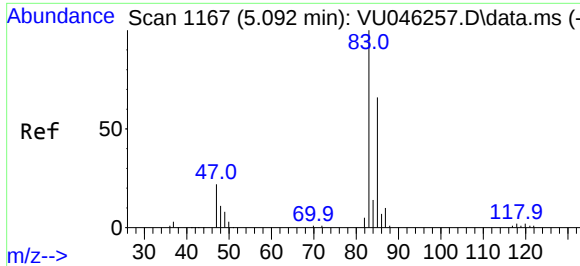

#25
 Chloroform
 Concen: 3.804 ug/L
 RT: 5.093 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VU046267.D
 Acq: 10 Dec 2021 15:51

Instrument :
 MSVOA_U
 ClientSampleId :
 EW9M7MEDL

Tgt Ion: 83 Resp: 13379

Ion	Ratio	Lower	Upper
83	100		
85	61.7	45.8	85.2

