

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046258.D
 Acq On : 10 Dec 2021 12:07
 Operator : SY/MD
 Sample : VU1210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	86846	98858	15.35%	1.948%
2	1.919	171	180	191	rBV	66231	84610	13.13%	1.668%
3	2.269	285	289	291	rBV	409	371	0.06%	0.007%
4	2.572	371	383	406	rBV	134356	225349	34.98%	4.441%
5	2.758	437	441	443	rBV	381	331	0.05%	0.007%
6	3.048	525	531	532	rBV	856	802	0.12%	0.016%
7	3.109	546	550	555	rBV2	398	437	0.07%	0.009%
8	3.150	560	563	566	rVV	398	351	0.05%	0.007%
9	3.192	566	576	589	rVB2	1774	3738	0.58%	0.074%
10	3.289	601	606	610	rBV2	348	338	0.05%	0.007%
11	3.359	625	628	631	rBV3	498	373	0.06%	0.007%
12	3.414	638	645	649	rBV	329	403	0.06%	0.008%
13	3.511	671	675	679	rBV2	401	379	0.06%	0.007%
14	3.565	686	692	699	rBV	431	526	0.08%	0.010%
15	3.851	775	781	784	rVV2	293	335	0.05%	0.007%
16	3.874	784	788	794	rVB2	559	535	0.08%	0.011%
17	3.996	822	826	830	rVB2	364	369	0.06%	0.007%
18	4.047	837	842	847	rBV	279	340	0.05%	0.007%
19	4.118	860	864	869	rVB	566	596	0.09%	0.012%
20	4.642	1006	1027	1056	rBV	57504	178133	27.65%	3.511%
21	4.774	1066	1068	1072	rVB2	586	410	0.06%	0.008%
22	4.935	1116	1118	1124	rVB2	432	476	0.07%	0.009%
23	4.977	1124	1131	1134	rBV	479	457	0.07%	0.009%
24	5.070	1141	1160	1182	rBV	111414	260221	40.39%	5.129%
25	5.244	1212	1214	1222	rVB2	634	595	0.09%	0.012%
26	5.353	1245	1248	1253	rVB	596	439	0.07%	0.009%
27	5.391	1253	1260	1263	rBV2	340	344	0.05%	0.007%
28	5.729	1341	1365	1389	rBV2	237494	644219	100.00%	12.697%
29	5.945	1429	1432	1436	rVB	576	475	0.07%	0.009%
30	5.973	1436	1441	1446	rBV3	383	527	0.08%	0.010%
31	6.089	1472	1477	1480	rBV2	361	334	0.05%	0.007%
32	6.253	1513	1528	1547	rBV	187580	353348	54.85%	6.964%
33	6.414	1575	1578	1582	rBV	503	418	0.06%	0.008%
34	6.475	1592	1597	1599	rBV	395	372	0.06%	0.007%
35	6.533	1608	1615	1632	rVV7	3085	7313	1.14%	0.144%
36	6.626	1640	1644	1650	rVB	481	525	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046258.D
 Acq On : 10 Dec 2021 12:07
 Operator : SY/MD
 Sample : VU1210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	6.697	1650	1666	1683	rBV	150312	288828	44.83%	5.692%
38	6.980	1750	1754	1760	rVB	390	425	0.07%	0.008%
39	7.289	1845	1850	1856	rBV	425	507	0.08%	0.010%
40	7.340	1863	1866	1869	rBV2	489	355	0.06%	0.007%
41	7.424	1888	1892	1895	rBV	489	437	0.07%	0.009%
42	7.478	1905	1909	1913	rBV	430	410	0.06%	0.008%
43	7.571	1925	1938	1955	rBV	81202	141829	22.02%	2.795%
44	7.678	1967	1971	1974	rBV3	426	377	0.06%	0.007%
45	7.787	1999	2005	2010	rBV2	691	794	0.12%	0.016%
46	7.903	2028	2041	2058	rBV	285878	495908	76.98%	9.774%
47	8.089	2096	2099	2103	rVB2	630	438	0.07%	0.009%
48	8.182	2118	2128	2147	rBV	55677	93182	14.46%	1.836%
49	8.282	2156	2159	2164	rBV2	467	348	0.05%	0.007%
50	8.343	2172	2178	2181	rBV	551	504	0.08%	0.010%
51	8.398	2189	2195	2197	rBV2	388	373	0.06%	0.007%
52	8.485	2219	2222	2228	rVB	413	308	0.05%	0.006%
53	8.581	2247	2252	2257	rBV	501	591	0.09%	0.012%
54	8.639	2257	2270	2304	rBV	193302	345161	53.58%	6.803%
55	8.915	2353	2356	2365	rVB4	1210	1625	0.25%	0.032%
56	8.980	2373	2376	2380	rBV2	663	515	0.08%	0.010%
57	9.330	2482	2485	2490	rVB	457	367	0.06%	0.007%
58	9.420	2500	2513	2537	rBV	286871	481964	74.81%	9.499%
59	9.700	2593	2600	2606	rBV2	1004	1439	0.22%	0.028%
60	10.022	2693	2700	2703	rBV2	471	524	0.08%	0.010%
61	10.333	2790	2797	2805	rBV2	557	876	0.14%	0.017%
62	10.568	2866	2870	2873	rBV	408	340	0.05%	0.007%
63	10.668	2896	2901	2904	rBV3	501	550	0.09%	0.011%
64	10.761	2917	2930	2946	rVV	222832	362631	56.29%	7.147%
65	10.829	2946	2951	2956	rVV4	521	633	0.10%	0.012%
66	11.095	3029	3034	3040	rVV3	709	955	0.15%	0.019%
67	11.137	3044	3047	3056	rBV	315	397	0.06%	0.008%
68	11.465	3145	3149	3158	rVB2	1020	1651	0.26%	0.033%
69	11.565	3176	3180	3184	rVB	404	382	0.06%	0.008%
70	11.620	3193	3197	3202	rBV2	379	407	0.06%	0.008%
71	11.751	3232	3238	3243	rVV3	1038	1241	0.19%	0.024%
72	11.816	3246	3258	3273	rVB	302362	475251	73.77%	9.366%
73	11.973	3304	3307	3312	rVB2	421	389	0.06%	0.008%
74	12.195	3363	3376	3392	rBV	296633	479116	74.37%	9.443%
75	12.420	3444	3446	3454	rVB	475	470	0.07%	0.009%
76	12.497	3464	3470	3472	rBV	406	406	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046258.D
 Acq On : 10 Dec 2021 12:07
 Operator : SY/MD
 Sample : VU1210WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.571	3490	3493	3498	rVB2	467	315	0.05%	0.006%
78	12.619	3504	3508	3511	rBV2	413	420	0.07%	0.008%
79	12.800	3558	3564	3570	rBV2	564	736	0.11%	0.015%
80	13.060	3642	3645	3647	rBV	434	318	0.05%	0.006%
81	13.224	3690	3696	3702	rVB4	1476	1791	0.28%	0.035%
82	13.571	3801	3804	3809	rVB	421	366	0.06%	0.007%
83	13.799	3871	3875	3878	rBV2	412	401	0.06%	0.008%
84	13.845	3883	3889	3897	rVV3	1961	2867	0.45%	0.057%
85	14.089	3956	3965	3977	rVB3	3188	5518	0.86%	0.109%
86	14.275	4018	4023	4025	rBV2	468	384	0.06%	0.008%
87	14.291	4025	4028	4034	rVB	424	347	0.05%	0.007%
88	14.333	4034	4041	4048	rBV4	2507	3375	0.52%	0.067%
89	14.706	4153	4157	4163	rVB	504	541	0.08%	0.011%
90	14.738	4163	4167	4171	rBV2	348	345	0.05%	0.007%
91	14.944	4223	4231	4236	rBV2	432	577	0.09%	0.011%
92	15.253	4320	4327	4331	rBV2	376	505	0.08%	0.010%
93	15.391	4365	4370	4375	rBV2	377	501	0.08%	0.010%
94	15.561	4419	4423	4427	rBV2	638	503	0.08%	0.010%
95	15.716	4467	4471	4475	rBV2	667	682	0.11%	0.013%
96	15.864	4512	4517	4519	rBV2	574	540	0.08%	0.011%
97	15.880	4519	4522	4525	rVB	639	413	0.06%	0.008%
98	15.931	4535	4538	4543	rBV3	453	508	0.08%	0.010%
99	16.002	4557	4560	4566	rBV3	392	382	0.06%	0.008%
100	16.960	4853	4858	4863	rBV3	966	1085	0.17%	0.021%




Sum of corrected areas: 5073971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046258.D
Acq On : 10 Dec 2021 12:07
Operator : SY/MD
Sample : VU1210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

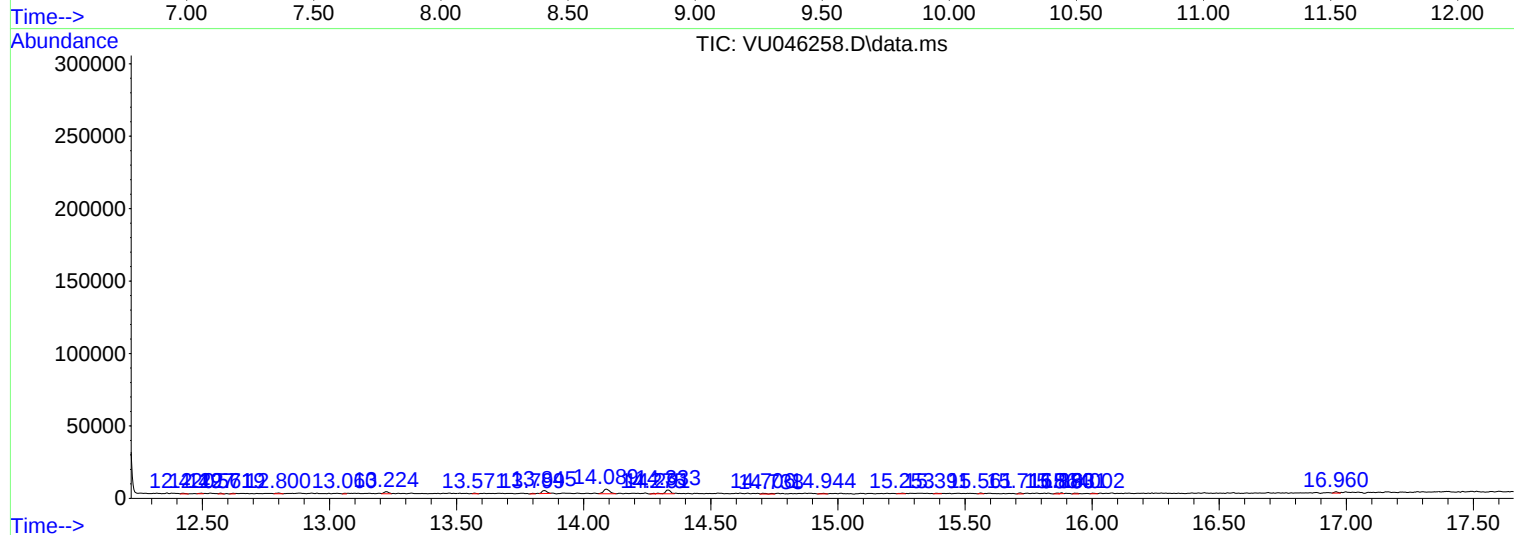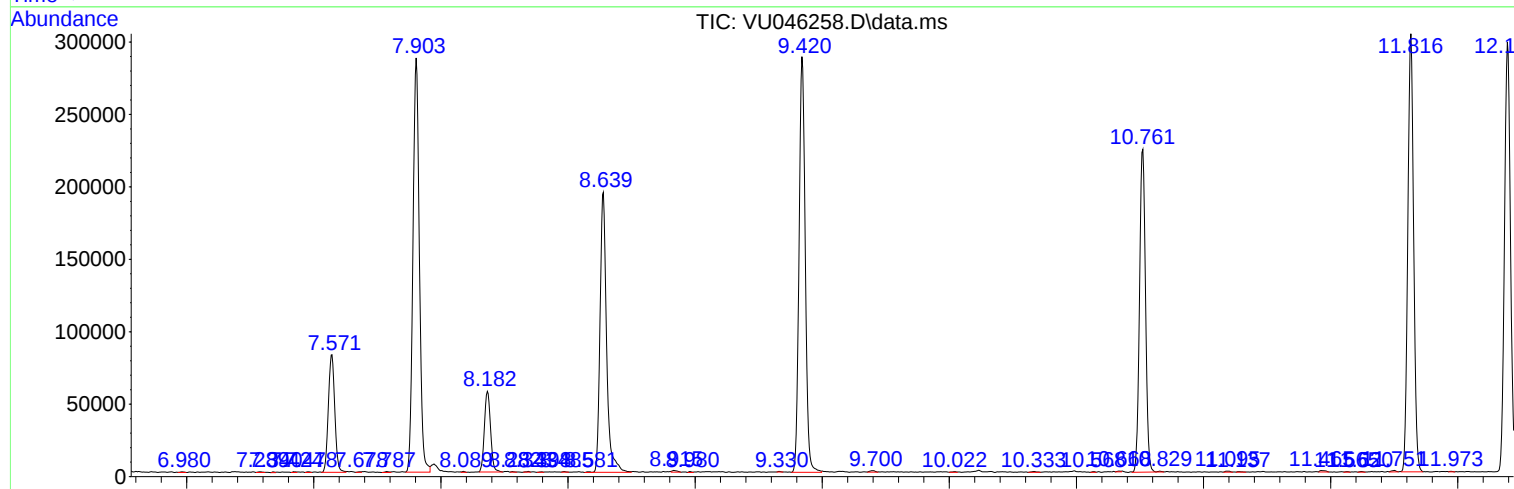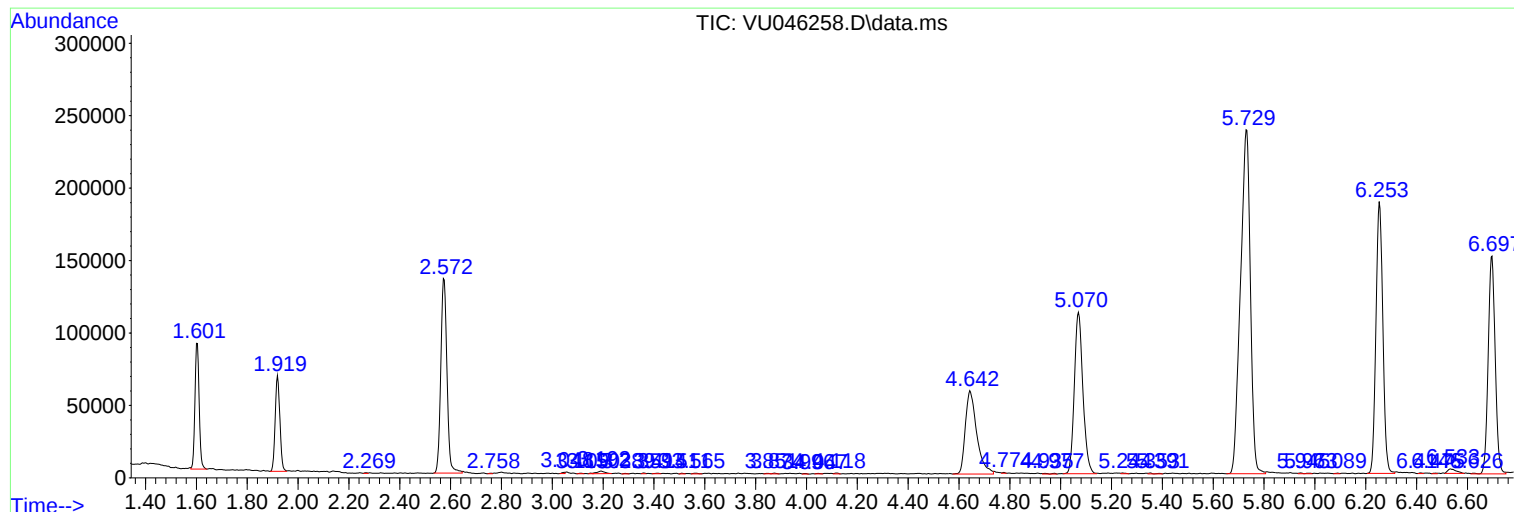

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046258.D
Acq On : 10 Dec 2021 12:07
Operator : SY/MD
Sample : VU1210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046258.D
Acq On : 10 Dec 2021 12:07
Operator : SY/MD
Sample : VU1210WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK055

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------