

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046269.D
 Acq On : 10 Dec 2021 16:46
 Operator : SY/MD
 Sample : M4943-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rBV	98110	106402	13.37%	1.593%
2	1.919	172	180	192	rVB	72443	91343	11.48%	1.367%
3	2.144	246	250	251	rBV2	644	470	0.06%	0.007%
4	2.456	343	347	351	rBV2	505	543	0.07%	0.008%
5	2.507	360	363	367	rBV2	479	356	0.04%	0.005%
6	2.575	371	384	401	rBV	165586	276642	34.76%	4.141%
7	2.951	498	501	509	rVB	719	842	0.11%	0.013%
8	3.006	509	518	521	rBV	619	878	0.11%	0.013%
9	3.054	523	533	544	rVV2	9300	16750	2.10%	0.251%
10	3.192	564	576	590	rVB2	2645	6301	0.79%	0.094%
11	3.327	615	618	622	rBV	425	433	0.05%	0.006%
12	3.398	636	640	642	rBV	469	397	0.05%	0.006%
13	3.562	686	691	695	rBV	361	457	0.06%	0.007%
14	3.694	728	732	735	rVV2	400	446	0.06%	0.007%
15	4.051	840	843	848	rBV2	402	400	0.05%	0.006%
16	4.295	914	919	925	rVB2	442	579	0.07%	0.009%
17	4.334	925	931	933	rBV	358	354	0.04%	0.005%
18	4.427	951	960	966	rBV	664	1003	0.13%	0.015%
19	4.633	1004	1024	1064	rBV2	81710	220812	27.75%	3.305%
20	4.793	1070	1074	1077	rBV2	567	526	0.07%	0.008%
21	4.919	1109	1113	1117	rVB	570	453	0.06%	0.007%
22	5.070	1143	1160	1181	rBV	141188	322973	40.58%	4.834%
23	5.295	1227	1230	1232	rVV2	632	443	0.06%	0.007%
24	5.314	1234	1236	1243	rVB	531	387	0.05%	0.006%
25	5.359	1243	1250	1253	rBV	548	686	0.09%	0.010%
26	5.398	1258	1262	1266	rVB	559	483	0.06%	0.007%
27	5.424	1266	1270	1272	rBV2	485	395	0.05%	0.006%
28	5.456	1276	1280	1287	rBV	577	618	0.08%	0.009%
29	5.729	1343	1365	1389	rBV2	290593	795825	100.00%	11.912%
30	6.121	1483	1487	1491	rVB3	547	459	0.06%	0.007%
31	6.253	1505	1528	1546	rBV	279604	525612	66.05%	7.867%
32	6.533	1605	1615	1630	rVV6	5107	11385	1.43%	0.170%
33	6.607	1634	1638	1644	rVB2	438	546	0.07%	0.008%
34	6.694	1650	1665	1683	rBV	184554	356543	44.80%	5.337%
35	7.031	1761	1770	1771	rBV2	740	817	0.10%	0.012%
36	7.189	1810	1819	1825	rBV4	920	1493	0.19%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046269.D
 Acq On : 10 Dec 2021 16:46
 Operator : SY/MD
 Sample : M4943-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	7.401	1881	1885	1891	rBV	779	970	0.12%	0.015%
38	7.514	1916	1920	1923	rVB	787	604	0.08%	0.009%
39	7.568	1923	1937	1952	rBV	107818	190189	23.90%	2.847%
40	7.755	1990	1995	1998	rBV2	429	406	0.05%	0.006%
41	7.780	1998	2003	2004	rBV	427	397	0.05%	0.006%
42	7.899	2023	2040	2054	rBV	358359	623599	78.36%	9.334%
43	8.067	2086	2092	2098	rBV3	670	851	0.11%	0.013%
44	8.182	2115	2128	2141	rBV	75272	124104	15.59%	1.858%
45	8.375	2185	2188	2192	rBV	394	409	0.05%	0.006%
46	8.555	2239	2244	2250	rVB4	1264	1516	0.19%	0.023%
47	8.632	2255	2268	2297	rBV	250978	439777	55.26%	6.582%
48	8.838	2327	2332	2337	rBV	610	689	0.09%	0.010%
49	8.906	2350	2353	2361	rVB2	923	1181	0.15%	0.018%
50	8.980	2373	2376	2381	rVB	524	501	0.06%	0.007%
51	9.192	2439	2442	2451	rVV	433	551	0.07%	0.008%
52	9.311	2475	2479	2482	rBV	531	374	0.05%	0.006%
53	9.333	2482	2486	2491	rVB	619	637	0.08%	0.010%
54	9.420	2499	2513	2534	rBV	403309	681381	85.62%	10.199%
55	9.697	2594	2599	2608	rVB3	2234	2908	0.37%	0.044%
56	9.867	2646	2652	2655	rVV	545	604	0.08%	0.009%
57	9.957	2677	2680	2683	rBV2	543	393	0.05%	0.006%
58	10.044	2704	2707	2712	rVV	497	428	0.05%	0.006%
59	10.140	2732	2737	2740	rBV	496	429	0.05%	0.006%
60	10.269	2773	2777	2783	rBV	495	611	0.08%	0.009%
61	10.417	2819	2823	2827	rBV	529	541	0.07%	0.008%
62	10.758	2916	2929	2945	rVV	278944	444925	55.91%	6.659%
63	10.899	2968	2973	2976	rVV4	692	635	0.08%	0.010%
64	11.115	3036	3040	3050	rVB5	2575	3707	0.47%	0.055%
65	11.173	3054	3058	3062	rBV	597	505	0.06%	0.008%
66	11.240	3076	3079	3081	rBV2	521	365	0.05%	0.005%
67	11.311	3097	3101	3106	rBV2	666	757	0.10%	0.011%
68	11.353	3110	3114	3116	rBV2	621	386	0.05%	0.006%
69	11.369	3116	3119	3122	rBV2	513	387	0.05%	0.006%
70	11.465	3140	3149	3159	rBV5	2138	3844	0.48%	0.058%
71	11.697	3215	3221	3227	rBV4	1518	1900	0.24%	0.028%
72	11.812	3245	3257	3273	rBV	454993	729429	91.66%	10.918%
73	11.912	3283	3288	3290	rBV4	1168	1066	0.13%	0.016%
74	12.009	3313	3318	3324	rVB5	1120	1250	0.16%	0.019%
75	12.060	3329	3334	3343	rVV5	2170	3480	0.44%	0.052%
76	12.195	3363	3376	3397	rVB	384988	624535	78.48%	9.348%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046269.D
 Acq On : 10 Dec 2021 16:46
 Operator : SY/MD
 Sample : M4943-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.327	3409	3417	3429	rBV5	7683	11895	1.49%	0.178%
78	12.896	3587	3594	3602	rVB4	1262	2035	0.26%	0.030%
79	13.044	3637	3640	3648	rBV3	1086	1093	0.14%	0.016%
80	13.108	3658	3660	3664	rBV	560	408	0.05%	0.006%
81	13.330	3725	3729	3731	rBV2	591	407	0.05%	0.006%
82	13.433	3754	3761	3771	rBV6	3614	5860	0.74%	0.088%
83	14.089	3958	3965	3974	rBV3	3597	5315	0.67%	0.080%
84	14.189	3993	3996	4001	rVB4	814	835	0.10%	0.012%
85	14.452	4071	4078	4084	rVB3	2469	3189	0.40%	0.048%
86	14.822	4190	4193	4197	rVB	709	554	0.07%	0.008%
87	14.844	4197	4200	4205	rBV3	787	641	0.08%	0.010%
88	14.873	4205	4209	4212	rBV4	795	785	0.10%	0.012%
89	14.983	4240	4243	4245	rBV2	885	668	0.08%	0.010%
90	15.005	4248	4250	4253	rVB3	825	444	0.06%	0.007%
91	15.086	4272	4275	4284	rVB3	697	877	0.11%	0.013%
92	15.134	4284	4290	4297	rBV2	595	870	0.11%	0.013%
93	15.169	4297	4301	4303	rBV2	652	411	0.05%	0.006%
94	15.401	4366	4373	4381	rBV7	1763	2621	0.33%	0.039%
95	15.507	4403	4406	4408	rBV3	614	478	0.06%	0.007%
96	15.812	4498	4501	4504	rBV	531	379	0.05%	0.006%
97	15.951	4541	4544	4547	rBV4	809	789	0.10%	0.012%
98	16.259	4636	4640	4646	rVB5	1763	1773	0.22%	0.027%
99	16.407	4680	4686	4688	rBV5	1941	2032	0.26%	0.030%
100	16.716	4780	4782	4785	rBV4	779	430	0.05%	0.006%




Sum of corrected areas: 6681062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046269.D
Acq On : 10 Dec 2021 16:46
Operator : SY/MD
Sample : M4943-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

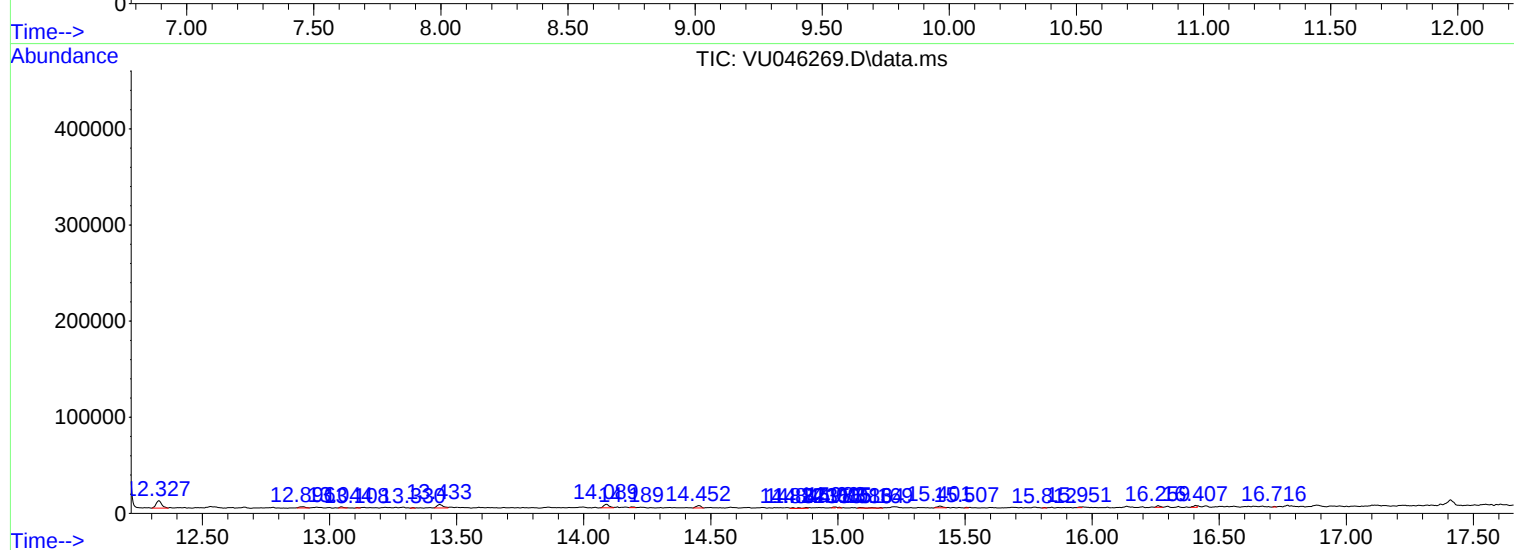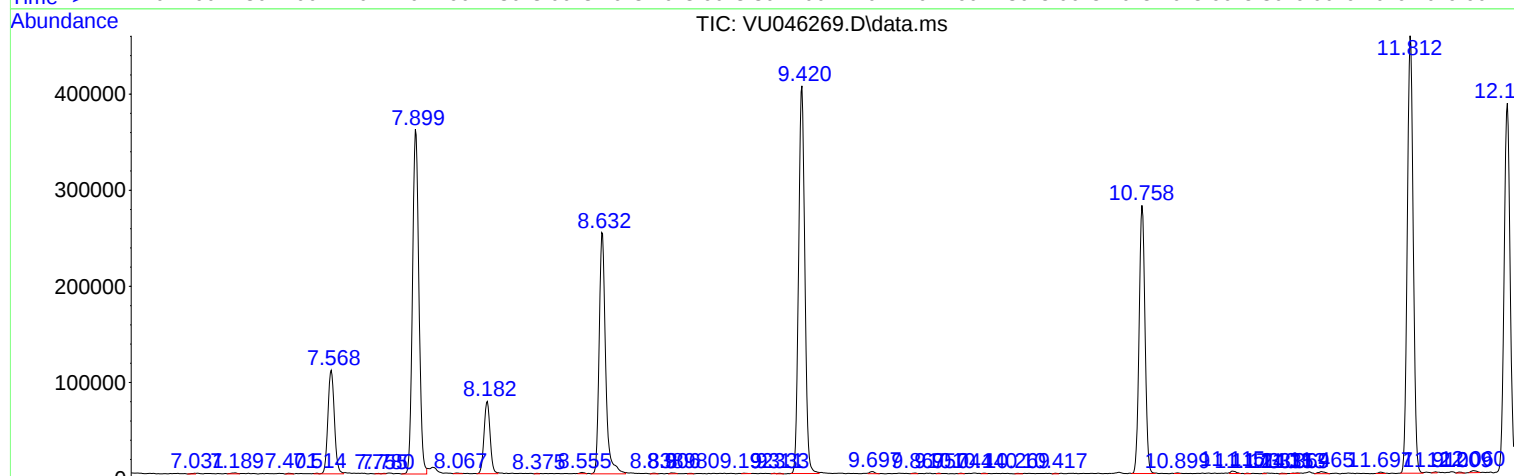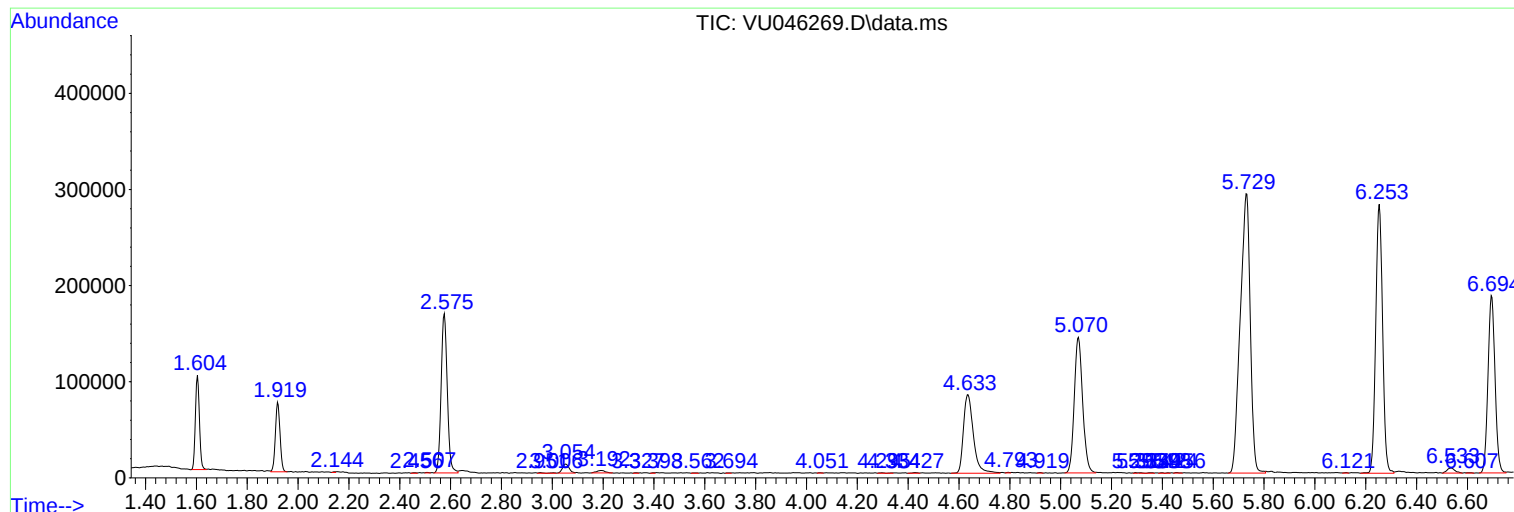

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046269.D
Acq On : 10 Dec 2021 16:46
Operator : SY/MD
Sample : M4943-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046269.D
Acq On : 10 Dec 2021 16:46
Operator : SY/MD
Sample : M4943-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------