

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046270.D
 Acq On : 10 Dec 2021 17:08
 Operator : SY/MD
 Sample : M4943-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	93	rVB	103670	110588	13.48%	1.645%
2	1.919	172	180	192	rVB	74484	93620	11.41%	1.392%
3	2.289	292	295	297	rBV2	430	298	0.04%	0.004%
4	2.575	372	384	401	rBV	168583	281559	34.31%	4.187%
5	2.739	432	435	438	rBV	514	391	0.05%	0.006%
6	3.054	523	533	544	rVB2	8743	15745	1.92%	0.234%
7	3.173	566	570	571	rBV	863	591	0.07%	0.009%
8	3.253	592	595	601	rVB	658	492	0.06%	0.007%
9	3.787	758	761	765	rBV2	455	397	0.05%	0.006%
10	4.035	834	838	842	rBV2	416	421	0.05%	0.006%
11	4.173	878	881	883	rBV	512	323	0.04%	0.005%
12	4.189	884	886	888	rBV2	458	289	0.04%	0.004%
13	4.253	903	906	909	rBV2	491	324	0.04%	0.005%
14	4.636	1010	1025	1052	rBV	85460	223140	27.19%	3.318%
15	5.070	1145	1160	1182	rVB2	146206	331738	40.43%	4.933%
16	5.729	1344	1365	1385	rBV2	300805	820556	100.00%	12.203%
17	6.253	1514	1528	1545	rBV	272035	510629	62.23%	7.594%
18	6.536	1608	1616	1626	rVB4	4774	8090	0.99%	0.120%
19	6.694	1651	1665	1683	rBV	190284	367241	44.76%	5.461%
20	7.115	1792	1796	1799	rBV	668	560	0.07%	0.008%
21	7.182	1814	1817	1826	rVB3	812	1285	0.16%	0.019%
22	7.305	1852	1855	1860	rVB	381	335	0.04%	0.005%
23	7.350	1860	1869	1873	rBV2	474	813	0.10%	0.012%
24	7.423	1887	1892	1895	rBV2	484	549	0.07%	0.008%
25	7.475	1904	1908	1911	rBV	540	515	0.06%	0.008%
26	7.568	1925	1937	1956	rBV	111538	193162	23.54%	2.873%
27	7.687	1971	1974	1978	rBV3	667	647	0.08%	0.010%
28	7.790	2002	2006	2008	rBV4	638	510	0.06%	0.008%
29	7.848	2020	2024	2027	rBV2	632	506	0.06%	0.008%
30	7.899	2027	2040	2057	rBV	367684	642828	78.34%	9.560%
31	8.182	2115	2128	2150	rBV	75805	129043	15.73%	1.919%
32	8.430	2201	2205	2211	rBV	521	668	0.08%	0.010%
33	8.485	2217	2222	2226	rBV2	442	500	0.06%	0.007%
34	8.507	2226	2229	2234	rBV	411	450	0.05%	0.007%
35	8.533	2234	2237	2241	rVB	387	289	0.04%	0.004%
36	8.562	2241	2246	2248	rVB2	561	422	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046270.D
 Acq On : 10 Dec 2021 17:08
 Operator : SY/MD
 Sample : M4943-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.581	2248	2252	2255	rBV	503	350	0.04%	0.005%
38	8.636	2255	2269	2300	rBV	256770	457580	55.76%	6.805%
39	8.796	2313	2319	2323	rBV	479	483	0.06%	0.007%
40	8.816	2323	2325	2330	rVB2	449	409	0.05%	0.006%
41	8.848	2330	2335	2338	rVB2	362	344	0.04%	0.005%
42	8.912	2348	2355	2361	rVB3	1114	1599	0.19%	0.024%
43	9.012	2382	2386	2392	rVV	447	448	0.05%	0.007%
44	9.063	2399	2402	2408	rVB	529	546	0.07%	0.008%
45	9.195	2440	2443	2447	rVB	398	310	0.04%	0.005%
46	9.221	2447	2451	2453	rBV	498	362	0.04%	0.005%
47	9.266	2462	2465	2471	rVV2	322	340	0.04%	0.005%
48	9.359	2490	2494	2496	rBV2	430	307	0.04%	0.005%
49	9.420	2500	2513	2532	rBV	398501	668494	81.47%	9.941%
50	9.565	2553	2558	2559	rBV	538	390	0.05%	0.006%
51	9.645	2579	2583	2589	rVB2	381	447	0.05%	0.007%
52	9.693	2589	2598	2607	rVB3	1878	2716	0.33%	0.040%
53	9.835	2638	2642	2646	rBV	441	451	0.05%	0.007%
54	9.899	2659	2662	2670	rVB	640	836	0.10%	0.012%
55	9.951	2670	2678	2681	rBV2	649	878	0.11%	0.013%
56	10.012	2692	2697	2698	rBV	357	301	0.04%	0.004%
57	10.095	2718	2723	2726	rBV3	620	533	0.06%	0.008%
58	10.214	2757	2760	2767	rVB2	660	489	0.06%	0.007%
59	10.266	2772	2776	2778	rBV	474	389	0.05%	0.006%
60	10.362	2802	2806	2810	rVB2	541	490	0.06%	0.007%
61	10.385	2810	2813	2816	rBV	448	375	0.05%	0.006%
62	10.404	2816	2819	2823	rVB	613	463	0.06%	0.007%
63	10.449	2828	2833	2840	rBV2	609	666	0.08%	0.010%
64	10.539	2859	2861	2864	rVB	559	317	0.04%	0.005%
65	10.623	2884	2887	2889	rBV2	437	332	0.04%	0.005%
66	10.671	2897	2902	2909	rVB4	1156	1374	0.17%	0.020%
67	10.758	2913	2929	2948	rVB	283639	459889	56.05%	6.839%
68	10.828	2948	2951	2954	rBV	568	453	0.06%	0.007%
69	10.861	2957	2961	2964	rVV2	422	338	0.04%	0.005%
70	10.899	2970	2973	2980	rVB2	511	615	0.07%	0.009%
71	10.980	2994	2998	3000	rBV2	791	574	0.07%	0.009%
72	11.063	3021	3024	3028	rBV2	335	311	0.04%	0.005%
73	11.092	3029	3033	3034	rBV	593	390	0.05%	0.006%
74	11.111	3034	3039	3040	rBV2	1060	838	0.10%	0.012%
75	11.160	3049	3054	3057	rBV	365	344	0.04%	0.005%
76	11.324	3100	3105	3110	rVB2	578	673	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046270.D
 Acq On : 10 Dec 2021 17:08
 Operator : SY/MD
 Sample : M4943-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	11.353	3110	3114	3115	rBV	411	290	0.04%	0.004%
78	11.382	3119	3123	3128	rVB2	515	574	0.07%	0.009%
79	11.414	3128	3133	3142	rBV3	1314	1712	0.21%	0.025%
80	11.459	3142	3147	3149	rBV3	1338	1118	0.14%	0.017%
81	11.700	3215	3222	3229	rBV3	1361	2089	0.25%	0.031%
82	11.767	3240	3243	3245	rBV	691	487	0.06%	0.007%
83	11.812	3245	3257	3271	rVV	448736	708600	86.36%	10.538%
84	11.906	3283	3286	3287	rBV2	950	513	0.06%	0.008%
85	11.970	3302	3306	3312	rBV7	1204	1482	0.18%	0.022%
86	12.060	3329	3334	3346	rVB6	2158	3532	0.43%	0.053%
87	12.108	3347	3349	3353	rBV3	610	465	0.06%	0.007%
88	12.195	3363	3376	3397	rVB	393516	634827	77.37%	9.441%
89	12.327	3410	3417	3426	rBV4	6394	8569	1.04%	0.127%
90	12.388	3434	3436	3440	rBV3	632	425	0.05%	0.006%
91	12.626	3508	3510	3516	rBV2	518	373	0.05%	0.006%
92	12.668	3519	3523	3528	rBV5	793	758	0.09%	0.011%
93	12.764	3550	3553	3555	rBV2	570	401	0.05%	0.006%
94	12.816	3566	3569	3571	rBV	524	306	0.04%	0.005%
95	12.890	3588	3592	3603	rBV3	1258	1708	0.21%	0.025%
96	13.208	3689	3691	3697	rVB2	656	515	0.06%	0.008%
97	13.433	3755	3761	3769	rVB5	2691	4115	0.50%	0.061%
98	13.613	3814	3817	3819	rBV	513	343	0.04%	0.005%
99	14.452	4072	4078	4085	rVB5	1998	3143	0.38%	0.047%
100	15.224	4313	4318	4321	rBV4	890	1053	0.13%	0.016%




Sum of corrected areas: 6724356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046270.D
Acq On : 10 Dec 2021 17:08
Operator : SY/MD
Sample : M4943-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

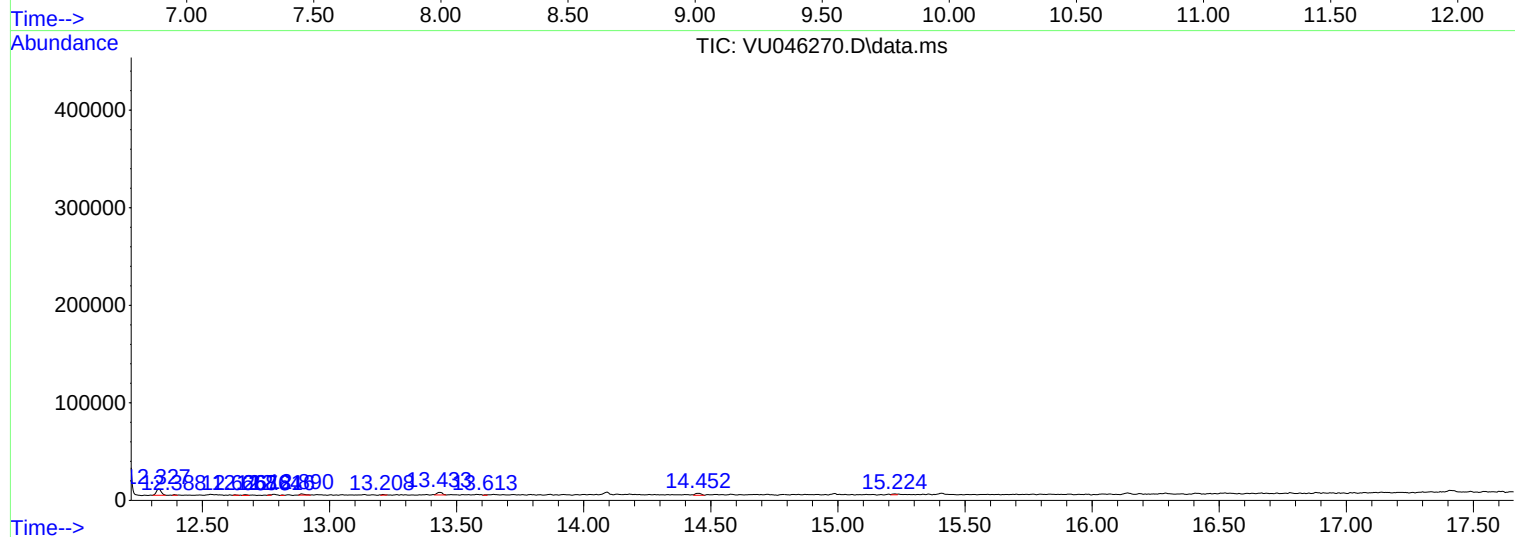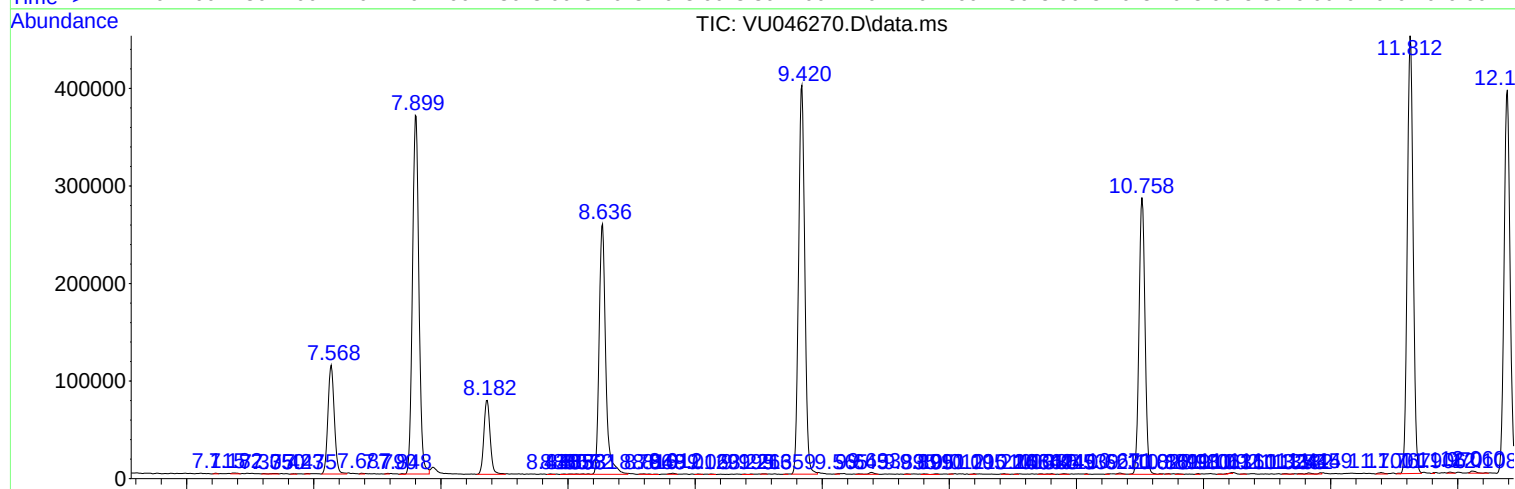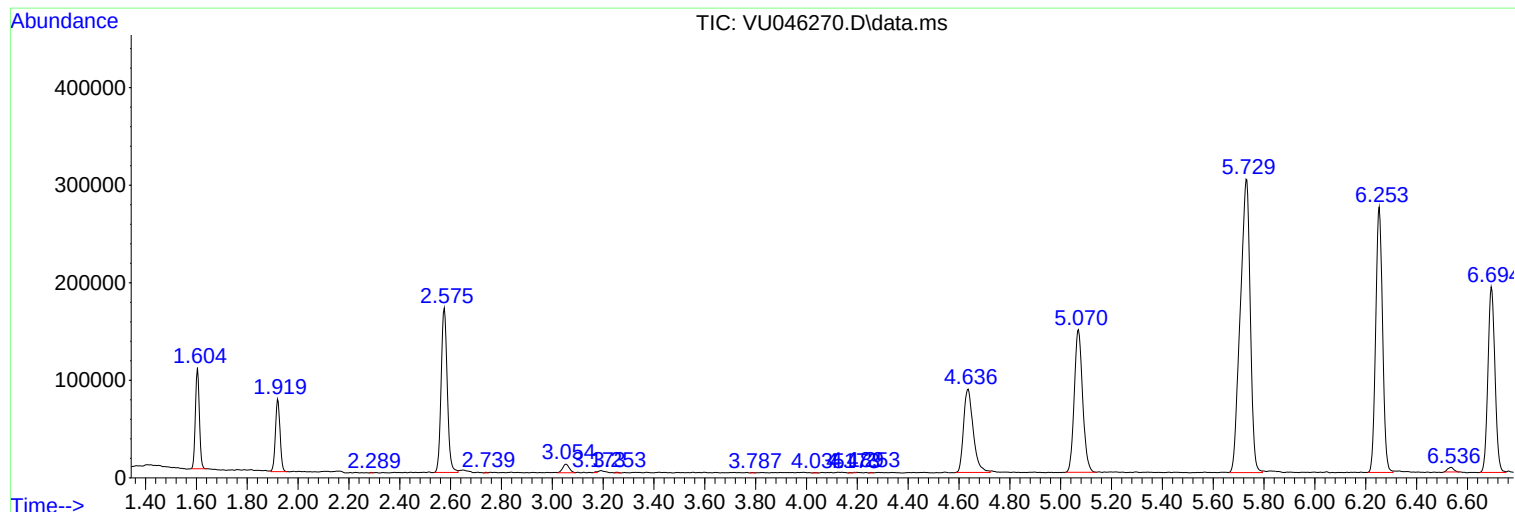

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046270.D
Acq On : 10 Dec 2021 17:08
Operator : SY/MD
Sample : M4943-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046270.D
Acq On : 10 Dec 2021 17:08
Operator : SY/MD
Sample : M4943-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc