

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046275.D
 Acq On : 10 Dec 2021 19:00
 Operator : SY/MD
 Sample : M4943-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

Signal : TIC: VU046275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	92	rVB	87975	95750	12.58%	1.453%
2	1.919	172	180	194	rVB	66015	84516	11.11%	1.283%
3	2.231	274	277	281	rVB2	482	375	0.05%	0.006%
4	2.253	281	284	287	rBV	411	339	0.04%	0.005%
5	2.446	340	344	347	rBV2	590	486	0.06%	0.007%
6	2.485	354	356	359	rBV	516	339	0.04%	0.005%
7	2.575	372	384	401	rBV	151495	253459	33.31%	3.848%
8	2.797	449	453	458	rBV2	503	609	0.08%	0.009%
9	3.054	522	533	550	rVB2	9401	17032	2.24%	0.259%
10	3.189	565	575	589	rVB	5275	11505	1.51%	0.175%
11	3.494	666	670	673	rBV	398	419	0.06%	0.006%
12	3.623	706	710	713	rBV	498	395	0.05%	0.006%
13	3.661	719	722	727	rBV	490	447	0.06%	0.007%
14	3.996	823	826	830	rVV2	536	369	0.05%	0.006%
15	4.636	1011	1025	1055	rBV	78456	222150	29.19%	3.372%
16	4.819	1078	1082	1088	rVB3	555	527	0.07%	0.008%
17	4.989	1130	1135	1137	rBV2	464	360	0.05%	0.005%
18	5.070	1144	1160	1183	rBV	133023	305374	40.13%	4.636%
19	5.295	1227	1230	1235	rBV2	397	426	0.06%	0.006%
20	5.391	1255	1260	1262	rBV	377	390	0.05%	0.006%
21	5.729	1344	1365	1384	rBV2	274897	743545	97.71%	11.287%
22	6.253	1514	1528	1550	rBV	279816	526156	69.14%	7.987%
23	6.533	1605	1615	1628	rBV4	6132	11958	1.57%	0.182%
24	6.694	1651	1665	1683	rBV	174648	334794	43.99%	5.082%
25	6.941	1738	1742	1750	rVB2	492	698	0.09%	0.011%
26	7.176	1811	1815	1816	rBV	504	361	0.05%	0.005%
27	7.568	1925	1937	1958	rVV	102165	179697	23.61%	2.728%
28	7.681	1970	1972	1977	rBV3	409	343	0.05%	0.005%
29	7.742	1984	1991	1993	rBV2	368	417	0.05%	0.006%
30	7.899	2027	2040	2057	rBV	341097	591745	77.76%	8.983%
31	8.182	2116	2128	2150	rVV	71781	119386	15.69%	1.812%
32	8.275	2153	2157	2165	rVB3	742	878	0.12%	0.013%
33	8.465	2210	2216	2219	rVB	393	430	0.06%	0.007%
34	8.488	2219	2223	2228	rVB	454	374	0.05%	0.006%
35	8.526	2228	2235	2239	rBB	504	488	0.06%	0.007%
36	8.636	2254	2269	2303	rBV	250928	446128	58.62%	6.772%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046275.D
 Acq On : 10 Dec 2021 19:00
 Operator : SY/MD
 Sample : M4943-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

37	8.809	2319	2323	2326	rBV	466	384	0.05%	0.006%
38	8.857	2336	2338	2346	rVB2	289	327	0.04%	0.005%
39	8.957	2364	2369	2372	rBV	463	469	0.06%	0.007%
40	8.992	2377	2380	2386	rVB	482	515	0.07%	0.008%
41	9.054	2392	2399	2403	rBV	564	651	0.09%	0.010%
42	9.237	2452	2456	2460	rVB	364	327	0.04%	0.005%
43	9.263	2460	2464	2467	rBV2	625	455	0.06%	0.007%
44	9.420	2499	2513	2542	rBV	410437	693513	91.13%	10.528%
45	9.568	2553	2559	2568	rVB2	1139	1677	0.22%	0.025%
46	9.697	2592	2599	2607	rVB3	2018	3259	0.43%	0.049%
47	9.748	2610	2615	2618	rVB3	599	509	0.07%	0.008%
48	9.896	2657	2661	2665	rVB	534	476	0.06%	0.007%
49	9.967	2680	2683	2692	rVB	379	442	0.06%	0.007%
50	10.102	2721	2725	2731	rBV2	891	987	0.13%	0.015%
51	10.253	2762	2772	2777	rBV5	1084	1865	0.25%	0.028%
52	10.311	2785	2790	2792	rVV	580	562	0.07%	0.009%
53	10.327	2792	2795	2798	rVV	612	430	0.06%	0.007%
54	10.520	2851	2855	2859	rBV	401	382	0.05%	0.006%
55	10.623	2884	2887	2892	rVV3	892	900	0.12%	0.014%
56	10.661	2893	2899	2908	rVB4	1707	2916	0.38%	0.044%
57	10.758	2916	2929	2947	rVB	274874	434110	57.04%	6.590%
58	10.873	2962	2965	2966	rBV2	473	326	0.04%	0.005%
59	10.896	2970	2972	2976	rVB2	540	354	0.05%	0.005%
60	10.963	2990	2993	2998	rBV2	447	341	0.04%	0.005%
61	10.992	2998	3002	3003	rBV	549	395	0.05%	0.006%
62	11.021	3008	3011	3018	rVB3	539	537	0.07%	0.008%
63	11.053	3018	3021	3022	rBV	689	355	0.05%	0.005%
64	11.115	3032	3040	3049	rBV3	6220	8718	1.15%	0.132%
65	11.259	3080	3085	3093	rVB2	561	815	0.11%	0.012%
66	11.298	3093	3097	3098	rBV2	593	451	0.06%	0.007%
67	11.378	3116	3122	3124	rBV4	809	758	0.10%	0.012%
68	11.417	3128	3134	3142	rBV7	2212	2764	0.36%	0.042%
69	11.468	3144	3150	3152	rBV4	1262	1468	0.19%	0.022%
70	11.581	3176	3185	3193	rVB5	1594	2934	0.39%	0.045%
71	11.639	3198	3203	3205	rBV3	761	723	0.10%	0.011%
72	11.697	3213	3221	3231	rVV8	2103	3583	0.47%	0.054%
73	11.812	3245	3257	3271	rBV	489177	761009	100.00%	11.552%
74	12.195	3364	3376	3393	rVB	375967	611478	80.35%	9.282%
75	12.327	3408	3417	3427	rVB2	13275	19485	2.56%	0.296%
76	12.394	3435	3438	3440	rBV2	659	423	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046275.D
 Acq On : 10 Dec 2021 19:00
 Operator : SY/MD
 Sample : M4943-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGKS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis

77	12.741	3540	3546	3548	rVV3	841	831	0.11%	0.013%
78	12.777	3551	3557	3563	rVV6	1260	1505	0.20%	0.023%
79	12.886	3582	3591	3599	rBV4	3297	4737	0.62%	0.072%
80	13.002	3622	3627	3630	rBV4	970	817	0.11%	0.012%
81	13.124	3662	3665	3667	rBV3	574	336	0.04%	0.005%
82	13.205	3686	3690	3691	rBV3	739	530	0.07%	0.008%
83	13.243	3700	3702	3704	rBV	679	413	0.05%	0.006%
84	13.362	3733	3739	3741	rBV2	1166	1211	0.16%	0.018%
85	13.587	3804	3809	3816	rVB4	1064	1307	0.17%	0.020%
86	13.864	3892	3895	3902	rVB7	1523	1663	0.22%	0.025%
87	13.902	3904	3907	3910	rBV3	472	392	0.05%	0.006%
88	14.089	3957	3965	3971	rBV2	7455	11935	1.57%	0.181%
89	14.452	4071	4078	4084	rBV6	3229	4675	0.61%	0.071%
90	14.577	4115	4117	4121	rVB2	1163	660	0.09%	0.010%
91	14.841	4195	4199	4203	rBV3	635	595	0.08%	0.009%
92	14.883	4209	4212	4216	rBV2	666	417	0.05%	0.006%
93	15.227	4311	4319	4327	rVB5	2607	4094	0.54%	0.062%
94	15.317	4345	4347	4352	rBV5	616	652	0.09%	0.010%
95	15.404	4367	4374	4385	rVB8	3527	6009	0.79%	0.091%
96	15.542	4414	4417	4422	rBV2	625	490	0.06%	0.007%
97	16.259	4636	4640	4646	rBV5	2640	2983	0.39%	0.045%
98	16.410	4681	4687	4693	rBV6	3182	4538	0.60%	0.069%
99	16.880	4830	4833	4844	rVB7	3178	3946	0.52%	0.060%
100	17.407	4991	4997	5008	rVB	11687	18087	2.38%	0.275%




Sum of corrected areas: 6587561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046275.D
Acq On : 10 Dec 2021 19:00
Operator : SY/MD
Sample : M4943-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

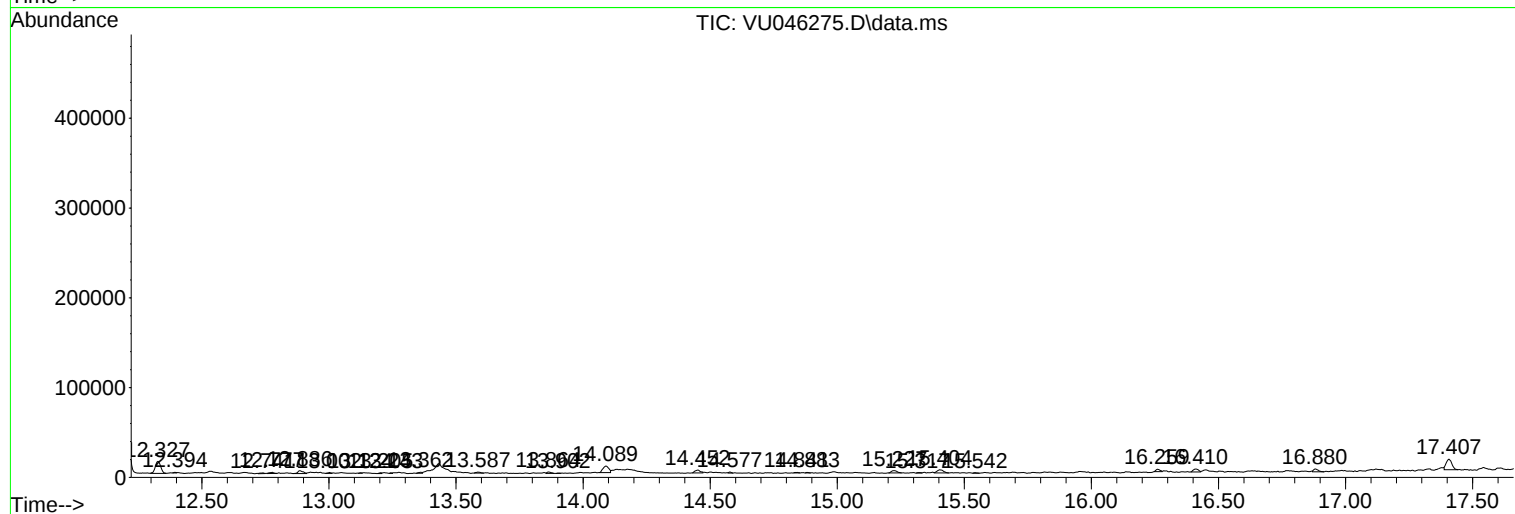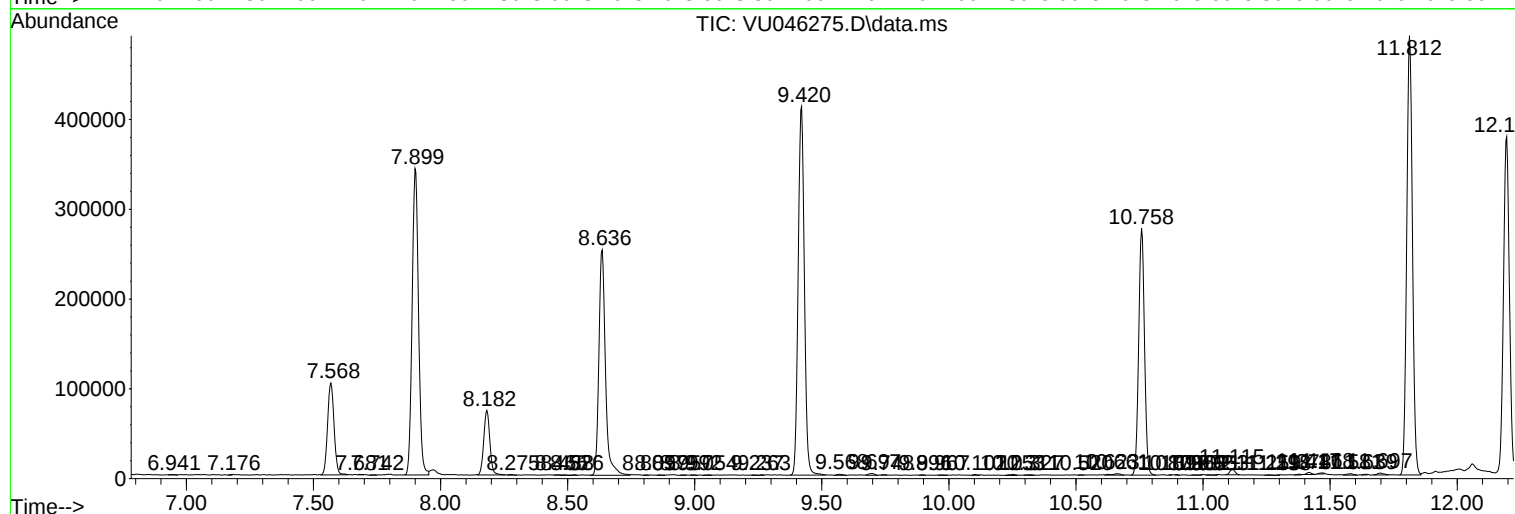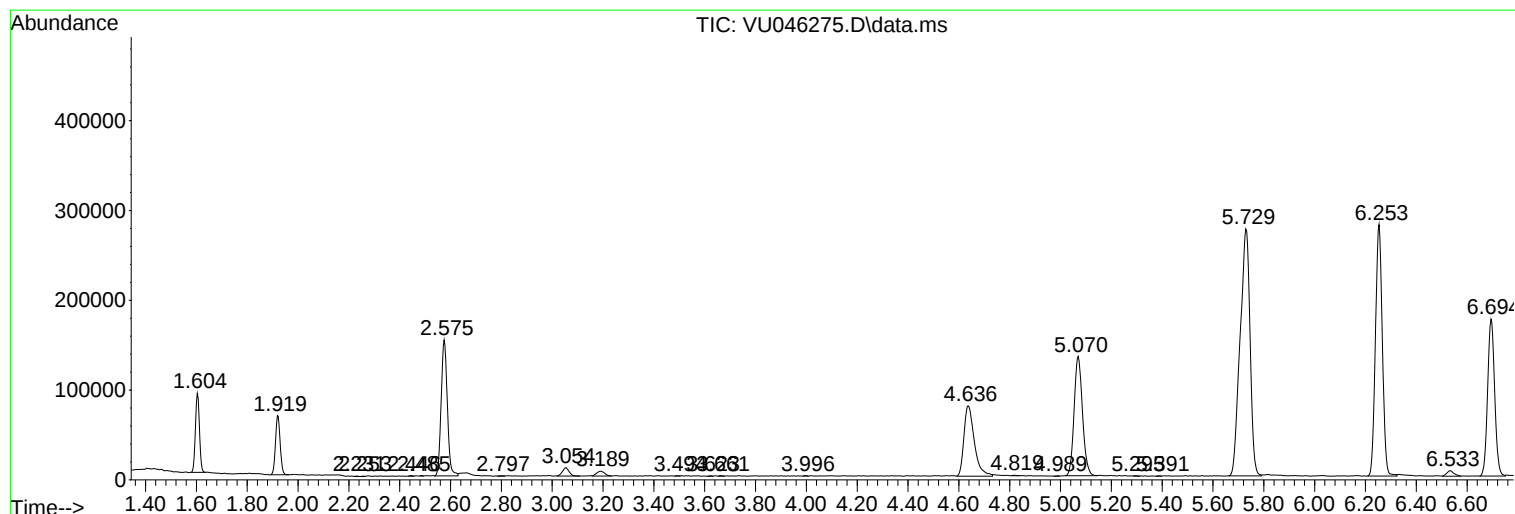

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046275.D
Acq On : 10 Dec 2021 19:00
Operator : SY/MD
Sample : M4943-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
Data File : VU046275.D
Acq On : 10 Dec 2021 19:00
Operator : SY/MD
Sample : M4943-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGKS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc