
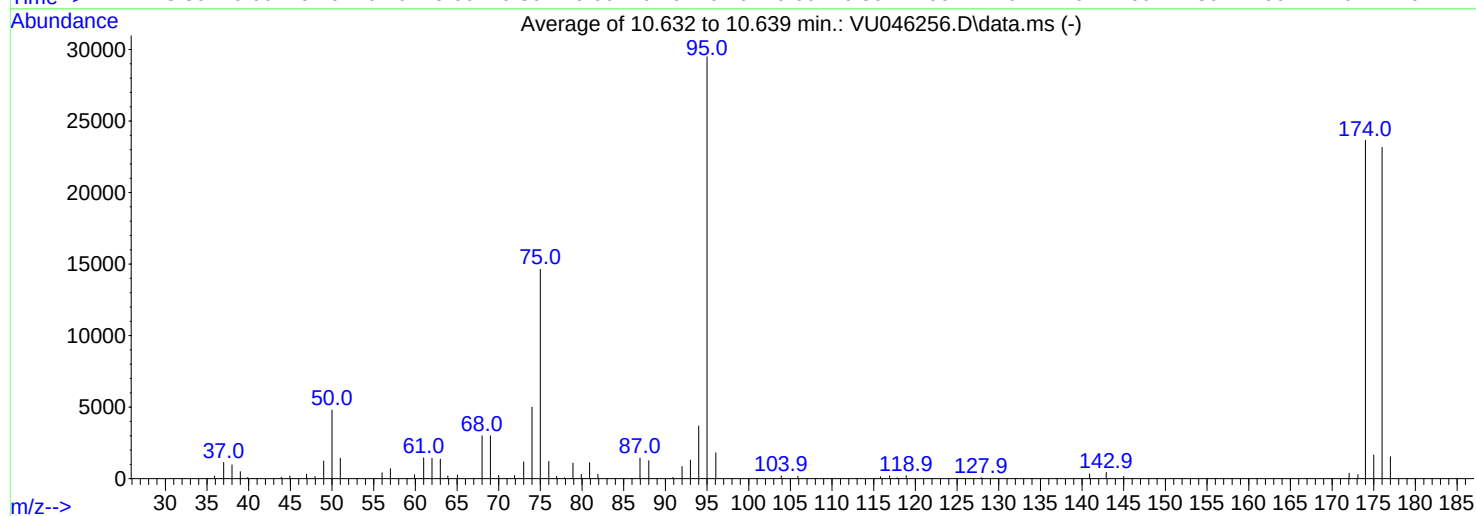


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121021\
 Data File : VU046256.D
 Acq On : 10 Dec 2021 10:50
 Operator : SY/MD
 Sample : BFB028
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB028

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112921WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 16 02:25:11 2021

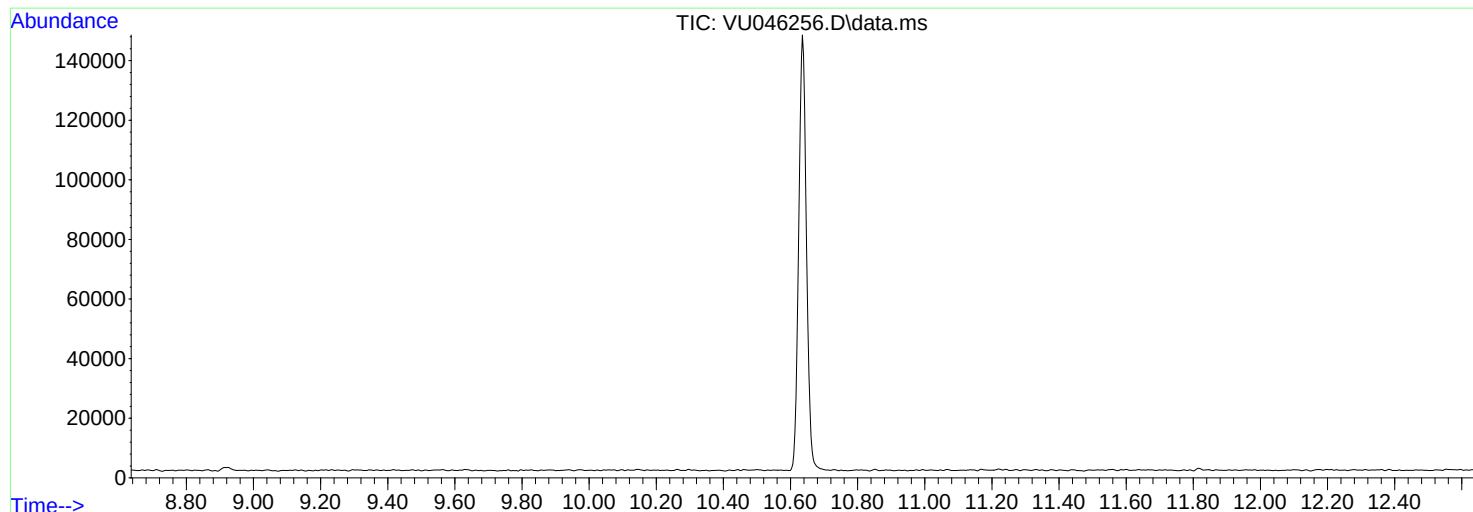

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	4799	PASS
75	95	30	80	49.6	14631	PASS
95	95	100	100	100.0	29488	PASS
96	95	5	9	6.1	1807	PASS
173	174	0.00	2	1.2	283	PASS
174	95	50	120	80.2	23643	PASS
175	174	5	9	7.0	1657	PASS
176	174	95	101	97.9	23152	PASS
177	176	5	9	6.6	1528	PASS

m/z	Abundance
35.90	177.0
37.00	1184.0
38.00	1000.0
39.00	478.0
39.90	2381.0
43.90	262.0
44.90	178.0
46.90	313.0
47.90	139.0
49.00	1224.0
50.00	4687.0
51.00	1395.0
56.00	420.0
57.00	615.0
59.90	227.0
61.00	1399.0
62.00	1403.0
63.00	1228.0
63.90	191.0
65.10	227.0
68.00	2873.0
69.00	2940.0
70.00	242.0
71.90	221.0
73.00	1223.0
74.00	5043.0
75.00	14136.0
76.00	1081.0
77.00	173.0
77.90	104.0
78.90	1032.0
79.90	307.0
80.90	1089.0
81.90	296.0
87.00	1503.0
88.00	1277.0
92.00	845.0
93.00	1287.0
94.00	3602.0
95.00	29040.0
96.00	1670.0
103.90	194.0
105.90	164.0
115.80	137.0
116.90	196.0
117.80	109.0
118.90	194.0
140.90	333.0
142.90	418.0
145.00	138.0
172.00	431.0
173.10	291.0
174.00	23800.0
175.00	1576.0
176.00	23432.0
177.00	1481.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
40.00	2290.0
43.90	170.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	168.0
37.00	1046.0
38.00	894.0
39.00	496.0
39.90	2373.0
43.90	290.0
45.00	189.0
47.00	299.0
48.00	171.0
49.00	1185.0
50.00	4737.0
51.00	1440.0
56.00	385.0
57.00	754.0
59.90	290.0
61.00	1468.0
62.00	1393.0
63.00	1471.0
63.90	191.0
65.00	286.0
67.00	112.0
68.00	2974.0
69.00	2976.0
70.00	223.0
71.90	223.0
73.00	1097.0
74.00	4801.0
75.00	14639.0
76.00	1287.0
76.90	135.0
78.90	1102.0
79.90	293.0
80.90	1116.0
81.90	307.0
86.90	1323.0
88.00	1185.0
90.90	126.0
92.00	830.0
93.00	1279.0
94.00	3632.0
95.00	28968.0
96.10	1913.0
103.90	170.0
105.90	175.0
115.80	110.0
116.90	202.0
118.90	221.0
127.90	103.0
140.90	334.0
142.90	456.0
145.00	161.0
172.10	320.0
173.10	253.0
174.00	22688.0
175.00	1705.0
176.00	21976.0
177.00	1528.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028

m/z	Abundance
35.90	169.0
37.00	1162.0
38.00	1002.0
39.00	511.0
39.90	2399.0
43.90	272.0
45.00	199.0
46.90	315.0
47.90	159.0
49.00	1272.0
50.00	4974.0
51.00	1469.0
56.00	427.0
57.00	700.0
59.90	275.0
61.00	1481.0
62.00	1469.0
63.00	1405.0
63.90	197.0
65.00	270.0
68.00	3139.0
69.00	3080.0
70.00	246.0
71.90	234.0
73.00	1209.0
74.00	5166.0
75.00	15118.0
76.00	1266.0
77.00	160.0
77.90	106.0
78.90	1115.0
79.90	310.0
80.90	1158.0
81.90	321.0
87.00	1501.0
88.00	1294.0
90.90	120.0
92.00	881.0
93.00	1340.0
94.00	3809.0
95.00	30456.0
96.00	1837.0
103.90	194.0
105.90	187.0
115.80	142.0
116.90	216.0
117.80	107.0
118.90	220.0
127.90	105.0
140.90	340.0
142.90	434.0
145.00	169.0
172.00	398.0
173.10	306.0
174.00	24440.0
175.00	1690.0
176.00	24048.0
177.00	1575.0

Instrument :
MSVOA_U
ClientSampleId :
BFB028