


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121118\
 Data File : VU028574.D
 Acq On : 11 Dec 2018 00:26
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
 Title : SW846 8260
 Last Update : Fri Dec 07 00:39:42 2018

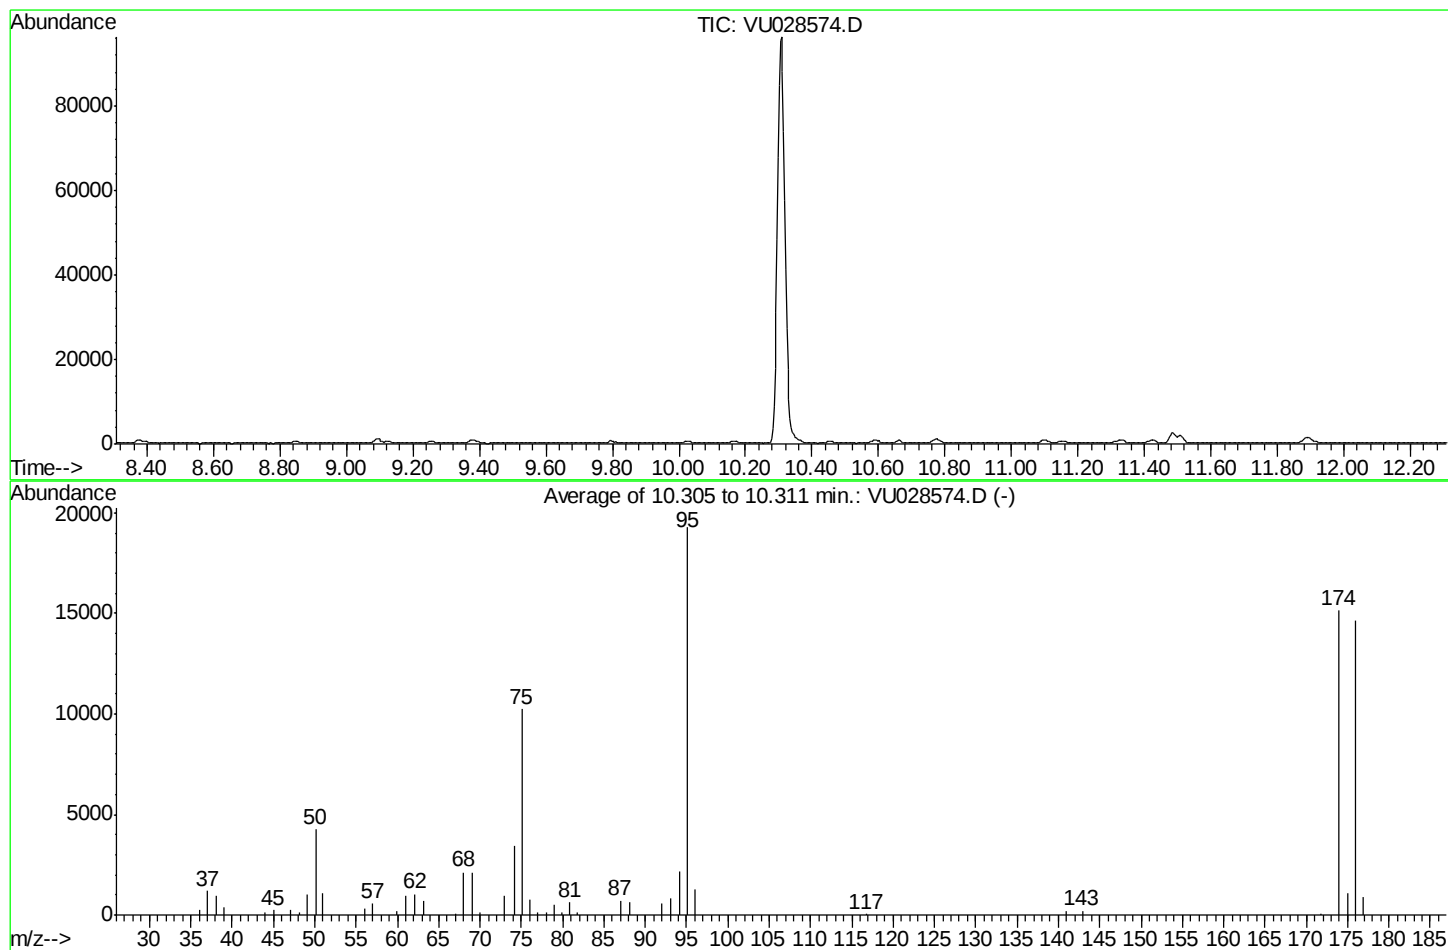

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	4257	PASS
75	95	30	60	53.1	10248	PASS
95	95	100	100	100.0	19285	PASS
96	95	5	9	6.6	1274	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.5	15137	PASS
175	174	5	9	7.3	1103	PASS
176	174	95	101	96.9	14663	PASS
177	176	5	9	6.2	907	PASS