

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU121119\
 Data File : VU036131.D
 Acq On : 11 Dec 2019 14:21
 Operator : JC/MD
 Sample : K6167-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQT8

Quant Time: Dec 12 07:33:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 12 06:08:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	300295	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	337689	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	120828	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	130045	4.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.20%
7) Chloroethane-d5	1.93	69	122926	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.59	63	135568	2.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	55.40%#
20) 2-Butanone-d5	4.70	46	287037	62.93	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.86%
24) Chloroform-d	5.11	84	211323	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	5.75	65	110991	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.77	84	398344	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.73	67	131880	5.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.40%
41) Toluene-d8	7.93	98	316605	4.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.20%
43) trans-1,3-Dichloropropene-	8.21	79	47030	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
46) 2-Hexanone-d5	8.68	63	227490	58.52	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	117.04%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	119300	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.60%
64) 1,2-Dichlorobenzene-d4	12.22	152	116157	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
13) Acetone	2.69	43	17872	3.087 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU121119\
Data File : VU036131.D
Acq On : 11 Dec 2019 14:21
Operator : JC/MD
Sample : K6167-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFQT8

Quant Time: Dec 12 07:33:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 12 06:08:55 2019
Response via : Initial Calibration

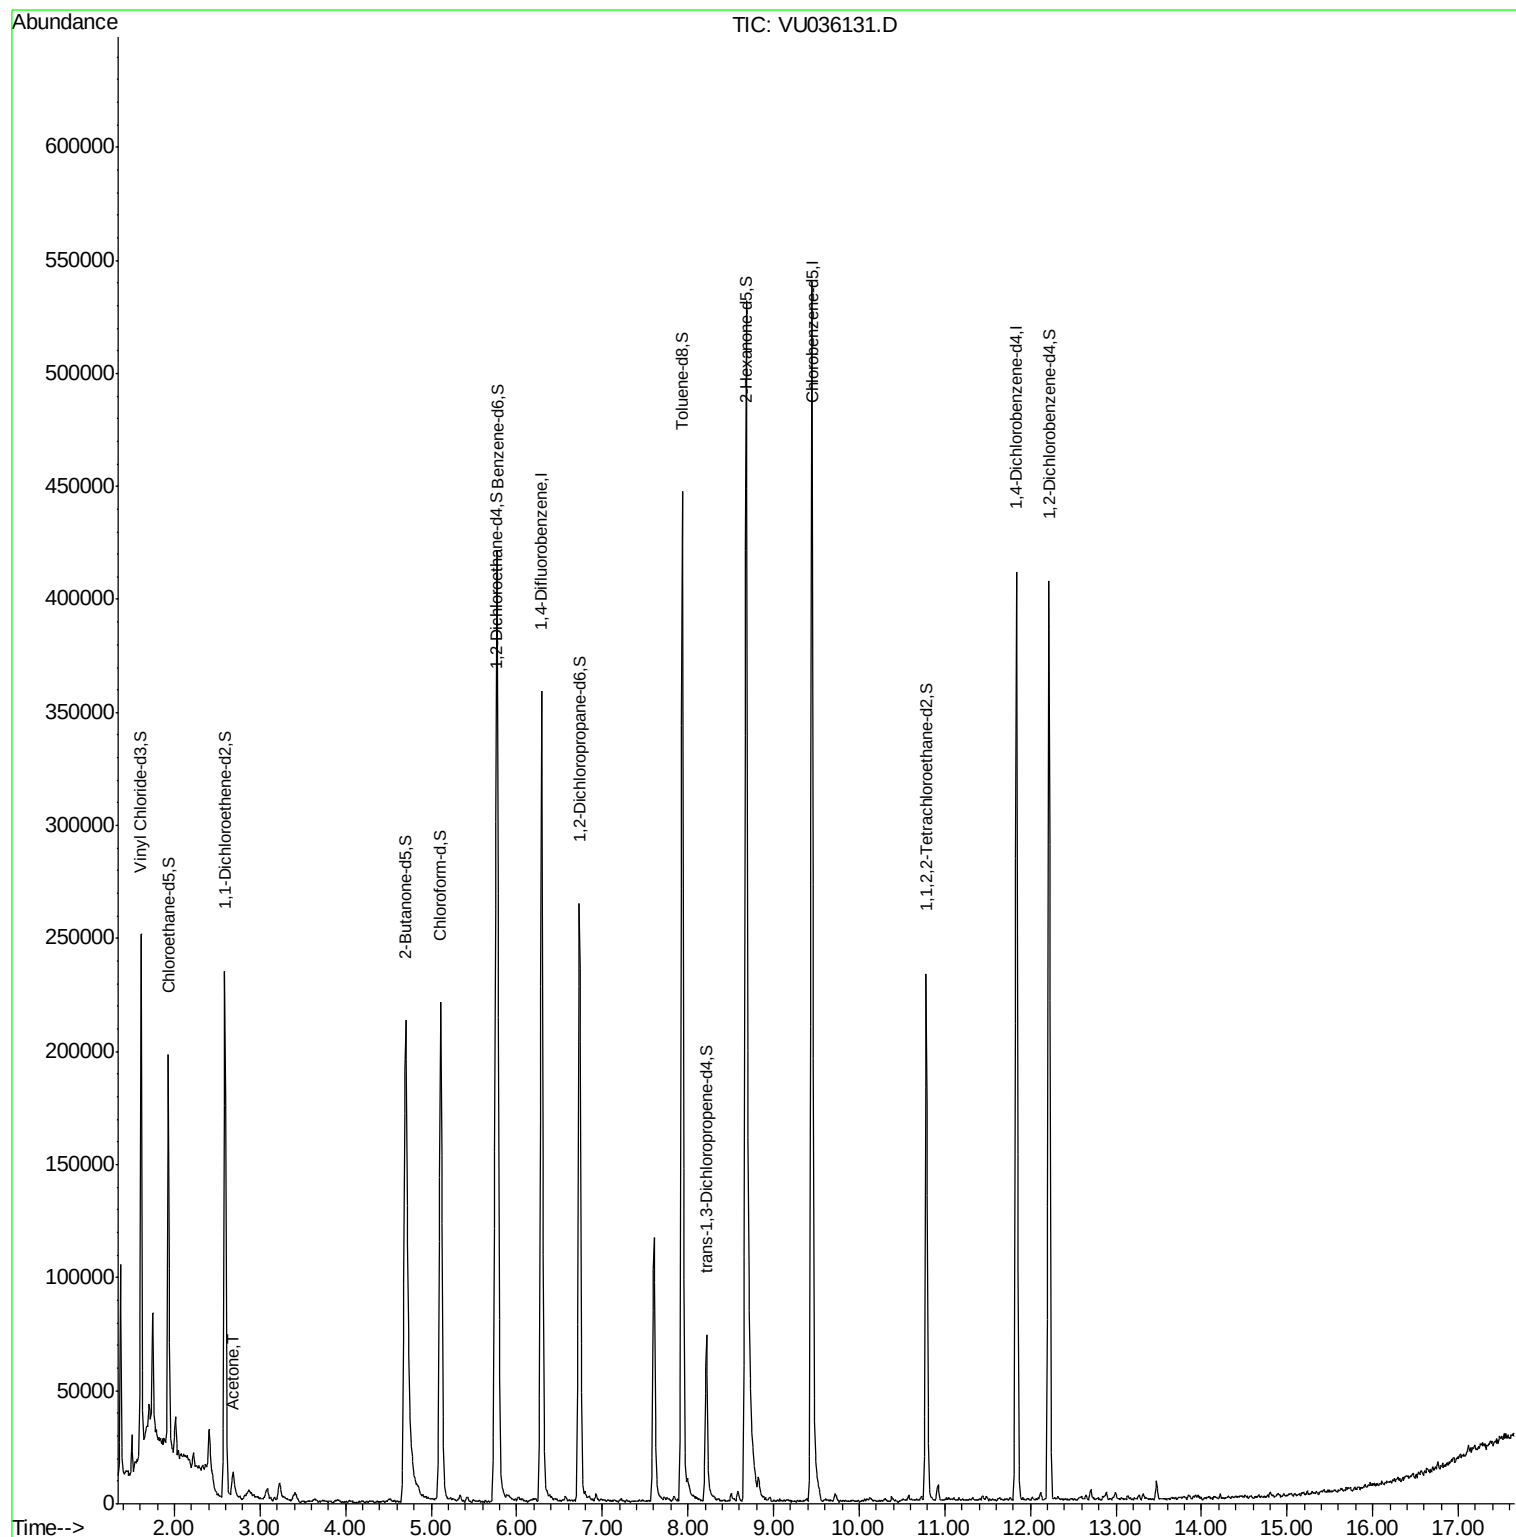

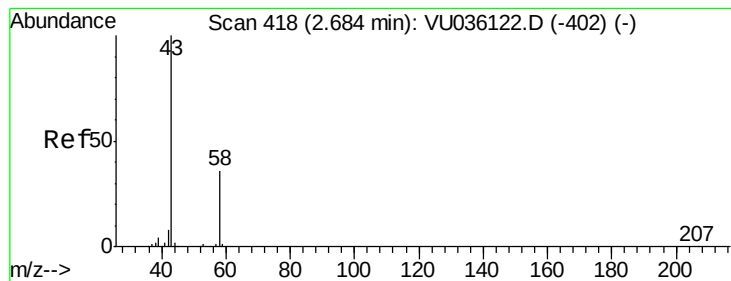

#13
 Acetone
 Concen: 3.087 ug/L
 RT: 2.69 min Scan# 419
 Delta R.T. 0.00 min
 Lab File: VU036131.D
 Acq: 11 Dec 2019 14:21

Instrument :
 MSVOA_U
 ClientSampleId :
 BFQT8

Tot Ion: 43 Resp: 17872
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 74.2

