


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU121119\
 Data File : VU036121.D
 Acq On : 11 Dec 2019 09:26
 Operator : JC/MD
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR120919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Dec 11 17:05:01 2019

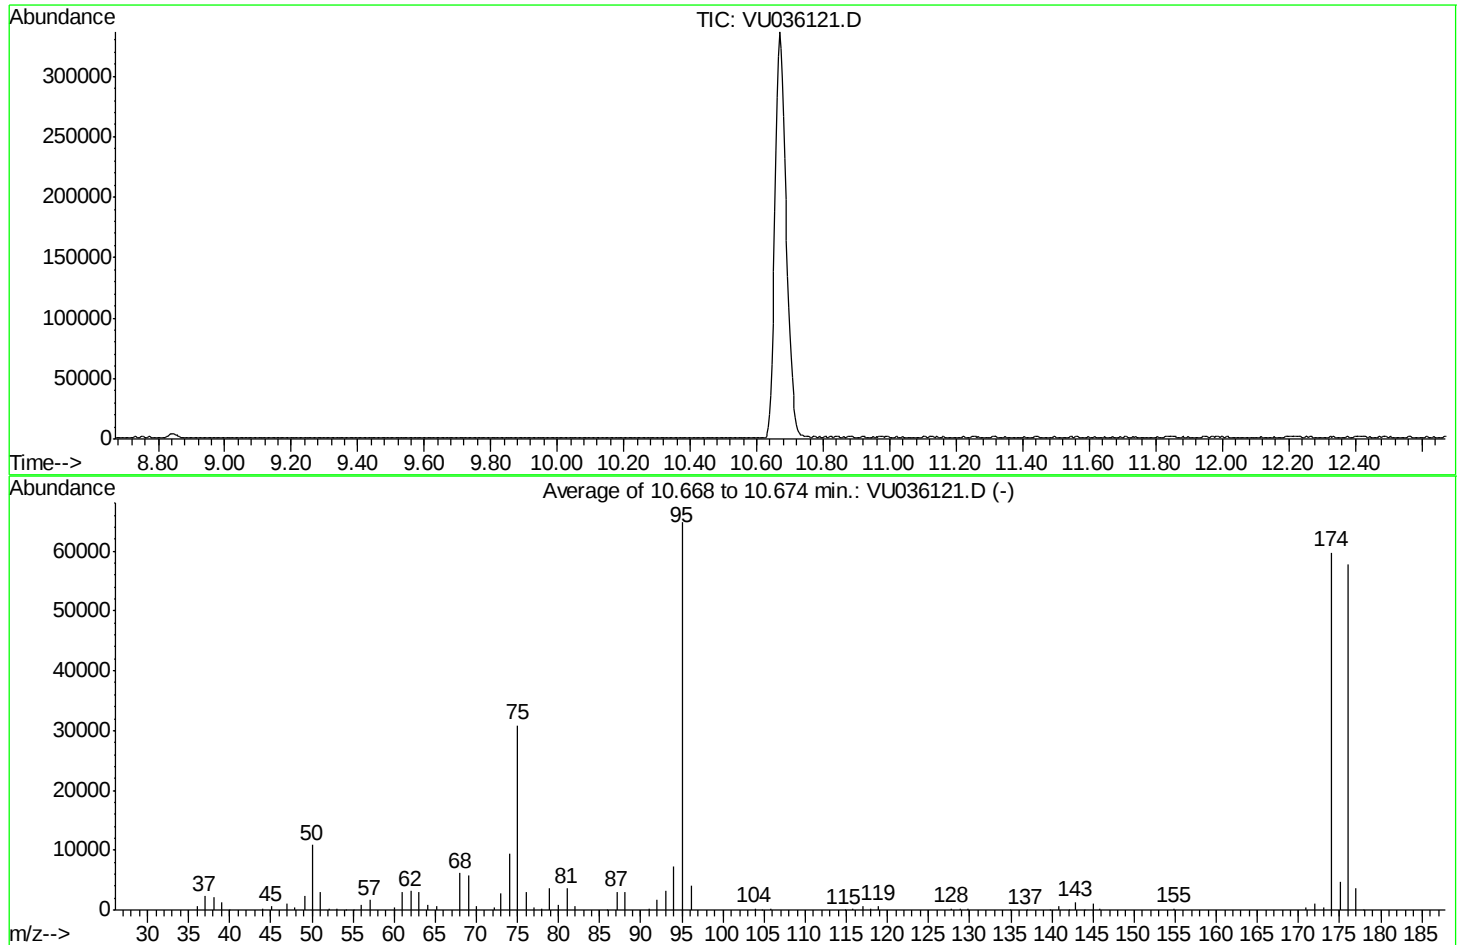

AutoFind: Scans 2901, 2902, 2903; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	10884	PASS
75	95	30	80	47.6	30824	PASS
95	95	100	100	100.0	64818	PASS
96	95	5	9	6.3	4063	PASS
173	174	0.00	2	0.7	393	PASS
174	95	50	120	92.3	59802	PASS
175	174	5	9	8.0	4813	PASS
176	174	95	101	96.7	57829	PASS
177	176	5	9	6.3	3641	PASS

m/z	Abundance
36.10	745.0
37.00	2483.0
38.10	2223.0
39.00	1449.0
40.00	347.0
44.00	924.0
45.00	676.0
47.00	984.0
47.90	298.0
49.10	2314.0
50.00	11400.0
51.10	3363.0
52.10	147.0
53.00	122.0
54.00	177.0
55.10	115.0
56.10	903.0
57.00	1688.0
60.00	510.0
61.00	2947.0
62.00	3129.0
63.00	3204.0
64.10	1076.0
65.20	582.0
68.10	6197.0
69.00	5652.0
70.00	510.0
72.20	334.0
73.00	2692.0
74.10	9422.0
75.00	30936.0
76.10	2855.0
77.00	298.0
77.80	333.0
78.90	3746.0
79.90	973.0
81.00	3585.0
82.00	725.0
87.10	3357.0
88.00	2804.0
90.90	243.0
92.00	1991.0
93.00	3287.0
94.00	7355.0
95.00	65168.0
96.10	4245.0
103.90	294.0
104.80	181.0
105.70	256.0
114.80	150.0
115.80	235.0
117.00	675.0
117.90	298.0
119.00	764.0
127.80	269.0
128.90	157.0
129.80	226.0
139.80	162.0
140.90	706.0
142.00	128.0
142.90	1340.0
143.90	178.0
145.00	1157.0
145.80	136.0
154.90	261.0
170.90	522.0
171.90	1200.0
174.00	60656.0
175.00	5021.0
176.00	56896.0
176.90	3737.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.10	736.0
37.00	2279.0
38.10	2128.0
39.00	1327.0
40.00	325.0
44.00	932.0
45.10	586.0
47.00	1036.0
47.80	332.0
49.10	2387.0
50.00	11072.0
51.10	3193.0
52.10	139.0
53.00	157.0
54.10	117.0
56.10	871.0
57.00	1761.0
60.10	496.0
61.00	3034.0
62.00	3136.0
62.90	2999.0
64.10	977.0
65.20	675.0
68.00	6281.0
69.00	6080.0
69.90	602.0
72.10	344.0
73.00	2868.0
74.10	9593.0
75.00	31320.0
76.10	2916.0
77.10	402.0
77.90	299.0
78.90	3596.0
79.90	914.0
81.00	3722.0
81.90	653.0
85.90	110.0
87.10	3063.0
88.00	2976.0
90.90	272.0
92.00	1765.0
93.00	3316.0
94.00	7504.0
95.00	65912.0
96.10	4086.0
103.90	345.0
104.70	125.0
105.80	304.0
114.80	139.0
115.80	219.0
117.00	606.0
117.90	318.0
119.00	701.0
127.80	244.0
128.80	155.0
129.80	263.0
134.90	105.0
136.90	126.0
139.80	108.0
140.90	563.0
142.90	1349.0
143.90	125.0
145.00	978.0
145.90	140.0
154.80	278.0
170.80	477.0
171.90	1179.0
174.00	60832.0
175.00	4961.0
176.00	58808.0
176.90	3704.0
177.80	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.10	733.0
36.90	2042.0
38.10	2051.0
39.00	1223.0
40.10	334.0
44.00	938.0
45.00	464.0
47.00	952.0
47.80	390.0
49.10	2322.0
50.00	10181.0
51.00	2763.0
52.10	128.0
53.00	195.0
55.00	121.0
56.00	787.0
57.00	1663.0
60.10	533.0
61.00	2921.0
62.00	3112.0
63.00	2687.0
64.00	834.0
65.10	677.0
68.00	6015.0
69.00	5939.0
69.90	573.0
72.10	319.0
73.00	3101.0
74.10	9197.0
75.00	30216.0
76.00	3030.0
77.00	514.0
78.00	322.0
78.90	3302.0
80.00	903.0
81.00	3590.0
81.90	643.0
87.00	2651.0
88.00	3203.0
91.00	244.0
92.00	1480.0
93.00	2891.0
94.00	7262.0
95.00	63376.0
96.10	3859.0
103.90	310.0
105.80	302.0
115.70	199.0
116.90	514.0
117.90	270.0
118.90	542.0
127.80	312.0
128.70	145.0
129.80	291.0
134.90	116.0
136.90	147.0
140.90	407.0
142.90	1344.0
145.10	790.0
145.90	144.0
154.80	219.0
170.80	419.0
172.00	1165.0
173.00	1181.0
174.00	57920.0
175.10	4457.0
176.00	57784.0
177.00	3482.0
177.90	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Scan 2884 (10.613 min): VU036121.D
BFB16

m/z	Abundance
39.90	247.0
43.90	625.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16