

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
 Data File : VU056739.D
 Acq On : 11 Dec 2023 18:06
 Operator : MD/SY
 Sample : 05678-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	85	95	105	rBV	127165	149845	17.26%	2.127%
2	1.907	183	192	206	rVB	91511	127931	14.73%	1.816%
3	2.563	381	396	411	rBV	197230	324912	37.42%	4.612%
4	3.181	574	588	599	rBV	7065	15455	1.78%	0.219%
5	4.618	1023	1035	1064	rBV	106904	293459	33.80%	4.165%
6	5.055	1155	1171	1197	rBV	168780	385382	44.38%	5.470%
7	5.721	1357	1378	1409	rBV2	332490	868272	100.00%	12.324%
8	6.245	1525	1541	1564	rBV	301749	589512	67.89%	8.367%
9	6.685	1662	1678	1706	rBV	197225	397809	45.82%	5.646%
10	7.563	1939	1951	1975	rBV	85576	155600	17.92%	2.208%
11	7.795	2014	2023	2035	rBV4	5054	9651	1.11%	0.137%
12	7.894	2040	2054	2073	rBV	377879	681164	78.45%	9.668%
13	8.177	2130	2142	2162	rBV	51783	91342	10.52%	1.296%
14	8.631	2271	2283	2323	rBV2	379293	758377	87.34%	10.764%
15	9.415	2514	2527	2550	rBV	421833	750239	86.41%	10.648%
16	10.749	2931	2942	2963	rVB2	135474	223563	25.75%	3.173%
17	10.888	2976	2985	2997	rBV3	7742	12454	1.43%	0.177%
18	11.807	3258	3271	3291	rBV	387729	645347	74.33%	9.160%
19	12.187	3376	3389	3413	rBV	331241	565198	65.09%	8.022%




Sum of corrected areas: 7045512

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056739.D
Acq On : 11 Dec 2023 18:06
Operator : MD/SY
Sample : 05678-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

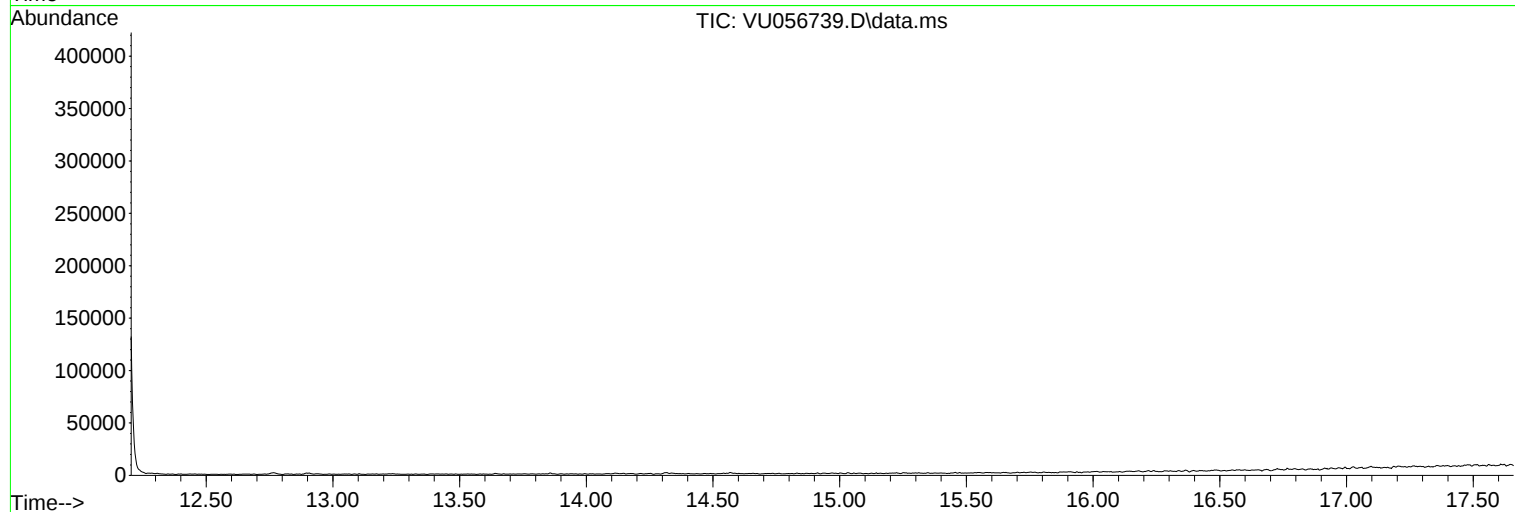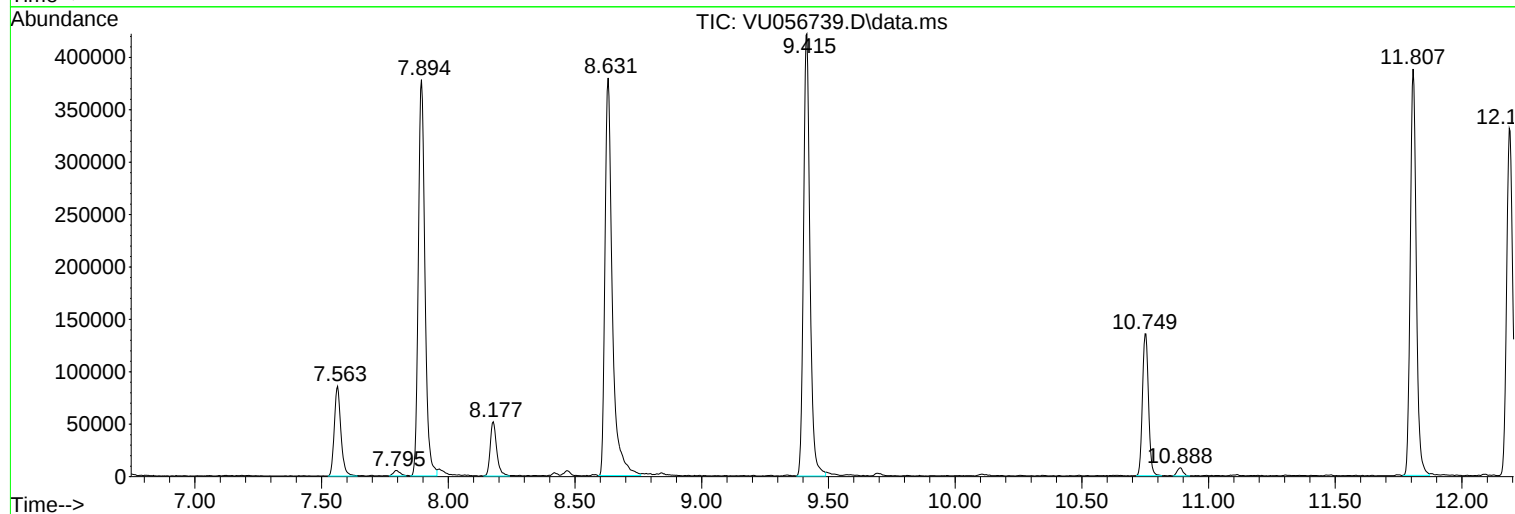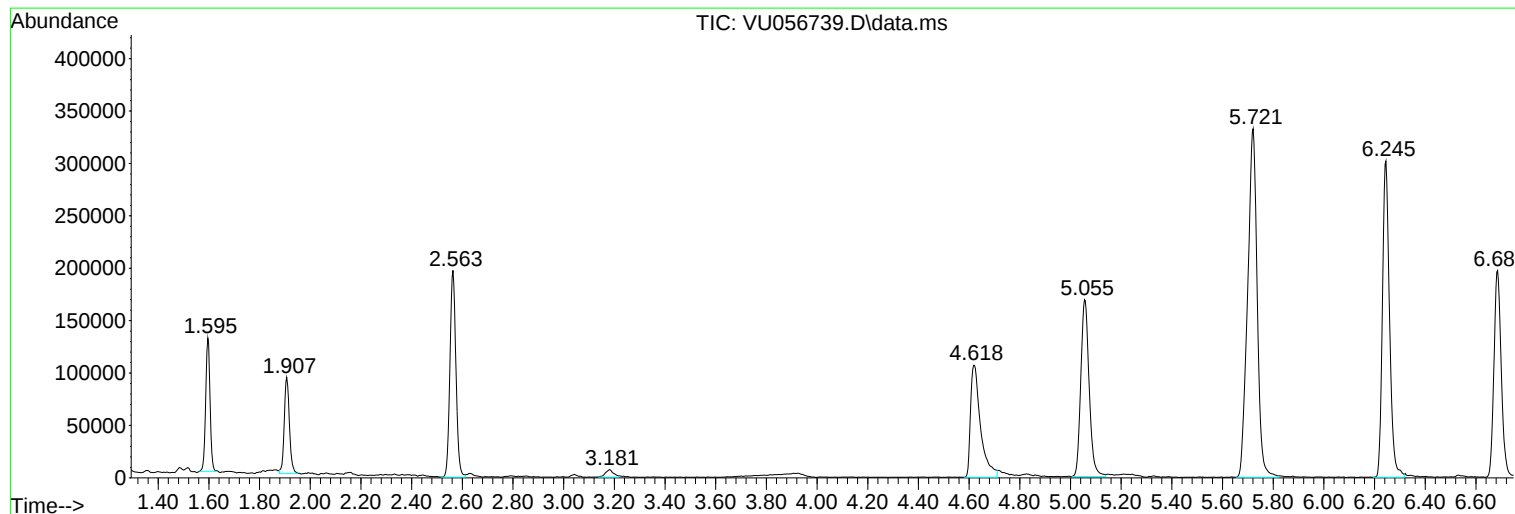

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056739.D
Acq On : 11 Dec 2023 18:06
Operator : MD/SY
Sample : 05678-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU121123\
Data File : VU056739.D
Acq On : 11 Dec 2023 18:06
Operator : MD/SY
Sample : 05678-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR121123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc